

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092

Reviewed by : AS

12/28/2017 11:30

Test: ^{Reactive} ~~Total~~ CN Mg/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.118	0.0	0.095	
ICB1	-0.061	0.0	0.004	
CCV1	243.023	0.0	0.235	
CCB1	-0.048	0.0	0.004	
PB105384BL	0.065	0.0	0.004	
I7082-01	-0.008	0.0	0.004	
I7082-01DUP	-0.204	0.0	0.004	
I7083-01	-0.163	0.0	0.004	
I7083-02	-0.307	0.0	0.004	
I7083-03	0.019	0.0	0.004	
CCV2	254.620	0.0	0.246	
CCB2	-0.033	0.0	0.004	

N	12
Mean	49.419
SD	97.1523
CV%	196.59

AS.

Aquakem v. 7.2AQ1

Results from time period:

Thu Dec 28 10:58:04 2017

Thu Dec 28 11:28:57 2017

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.3366	µg/l	12/28/2017 10:58:04	
5.OPPBCN	A	Reactive CN	P	4.8815	µg/l	12/28/2017 10:58:05	
10PPBCN	A	Reactive CN	P	9.8451	µg/l	12/28/2017 10:58:06	
50PPBCN	A	Reactive CN	P	50.1051	µg/l	12/28/2017 10:58:07	
100PPBCN	A	Reactive CN	P	100.3461	µg/l	12/28/2017 10:58:08	
250PPBCN	A	Reactive CN	P	250.4687	µg/l	12/28/2017 10:58:09	
500PPBCN	A	Reactive CN	P	499.6902	µg/l	12/28/2017 10:58:10	
ICV1	S	Reactive CN	P	96.1182	µg/l	12/28/2017 11:24:07	
ICB1	S	Reactive CN	P	-0.0607	µg/l	12/28/2017 11:24:08	
CCV1	S	Reactive CN	P	243.0234	µg/l	12/28/2017 11:24:11	
CCB1	S	Reactive CN	P	-0.0476	µg/l	12/28/2017 11:24:13	
PB105384BL	S	Reactive CN	P	0.0648	µg/l	12/28/2017 11:24:14	
I7082-01	S	Reactive CN	P	-0.0076	µg/l	12/28/2017 11:24:15	
I7082-01DUP	S	Reactive CN	P	-0.2039	µg/l	12/28/2017 11:24:16	
I7083-01	S	Reactive CN	P	-0.1632	µg/l	12/28/2017 11:28:53	
I7083-02	S	Reactive CN	P	-0.3072	µg/l	12/28/2017 11:28:54	
I7083-03	S	Reactive CN	P	0.0194	µg/l	12/28/2017 11:28:55	
CCV2	S	Reactive CN	P	254.62	µg/l	12/28/2017 11:28:56	
CCB2	S	Reactive CN	P	-0.0333	µg/l	12/28/2017 11:28:57	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

12/28/2017 11:00


Test Total CN

Accepted 12/28/2017 11:00

Factor 1051
 Bias 0.004

Coeff. of det. 0.999997

Errors

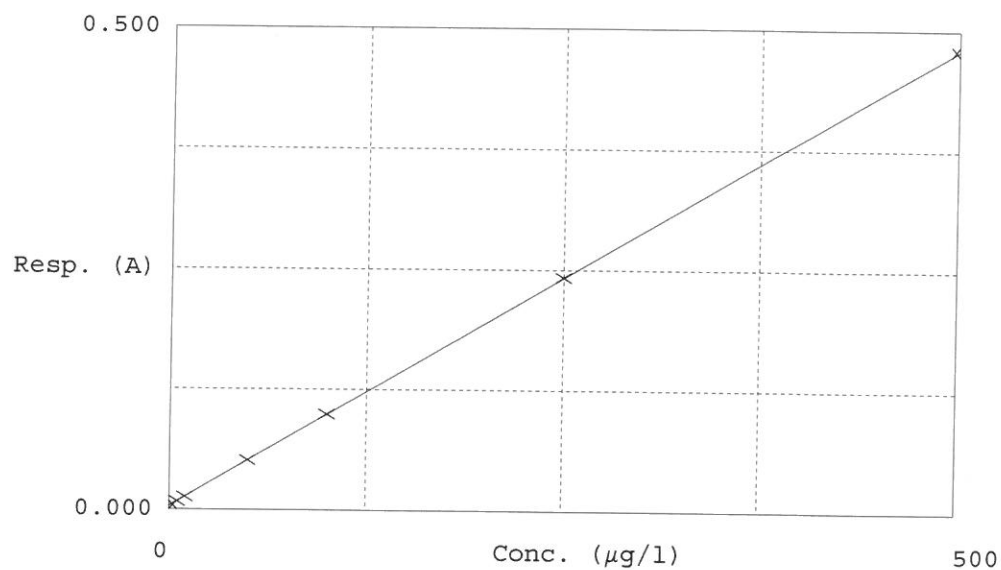

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.3366	0.0000	
2	5.0PPBCN	0.008	4.8815	5.0000	
3	10PPBCN	0.013	9.8451	10.0000	
4	50PPBCN	0.051	50.1051	50.0000	
5	100PPBCN	0.099	100.3461	100.0000	
6	250PPBCN	0.242	250.4687	250.0000	
7	500PPBCN	0.479	499.6902	500.0000	