

6892496

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

1/5/2018 14:58

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.428	0.0	0.092	
ICB1	0.528	0.0	0.004	
CCV1	240.460	0.0	0.225	
CCB1	0.539	0.0	0.004	
PB105498BL	0.418	0.0	0.004	
PB105498BS	96.282	0.0	0.092	
MIDPB105498	242.602	0.0	0.227	
I7026-01	6.071	0.0	0.009	
I7026-01DUP	5.793	0.0	0.009	
I7026-01MS	35.110	0.0	0.036	
I7026-01MSD	35.458	0.0	0.036	
CCV2	255.664	0.0	0.239	
CCB2	0.417	0.0	0.004	

N	13
Mean	78.059
SD	101.5575
CV%	130.10

UB 92496

Aquakem v. 7.2AQ1

AK

Results from time period:

Fri Jan 05 14:54:47 2018

Fri Jan 05 14:58:11 2018

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.4067	µg/l	1/5/2018 12:03:23	
5.OPPBCN	A	Total CN	P	5.7922	µg/l	1/5/2018 12:03:24	
10PPBCN	A	Total CN	P	9.1858	µg/l	1/5/2018 12:03:25	
50PPBCN	A	Total CN	P	50.6381	µg/l	1/5/2018 12:03:26	
100PPBCN	A	Total CN	P	99.5216	µg/l	1/5/2018 12:03:27	
250PPBCN	A	Total CN	P	250.4576	µg/l	1/5/2018 12:03:28	
500PPBCN	A	Total CN	P	499.8114	µg/l	1/5/2018 12:03:29	
ICV1	S	Total CN	P	95.428	µg/l	1/5/2018 14:54:47	
ICB1	S	Total CN	P	0.528	µg/l	1/5/2018 14:54:48	
CCV1	S	Total CN	P	240.4604	µg/l	1/5/2018 14:54:49	
CCB1	S	Total CN	P	0.5387	µg/l	1/5/2018 14:54:50	
PB105498BL	S	Total CN	P	0.4181	µg/l	1/5/2018 14:54:51	
PB105498BS	S	Total CN	P	96.2818	µg/l	1/5/2018 14:54:52	
MIDPB105498	S	Total CN	P	242.6024	µg/l	1/5/2018 14:54:53	
I7026-01	S	Total CN	P	6.0713	µg/l	1/5/2018 14:54:54	
I7026-01DUP	S	Total CN	P	5.7931	µg/l	1/5/2018 14:54:55	
I7026-01MS	S	Total CN	P	35.11	µg/l	1/5/2018 14:54:56	
I7026-01MSD	S	Total CN	P	35.458	µg/l	1/5/2018 14:54:57	
CCV2	S	Total CN	P	255.6643	µg/l	1/5/2018 14:58:10	
CCB2	S	Total CN	P	0.4171	µg/l	1/5/2018 14:58:11	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : ALC

1/5/2018 13:53


Test Total CN

Accepted 1/5/2018 12:03

Factor 1085
Bias 0.004

Coeff. of det. 0.999989

Errors

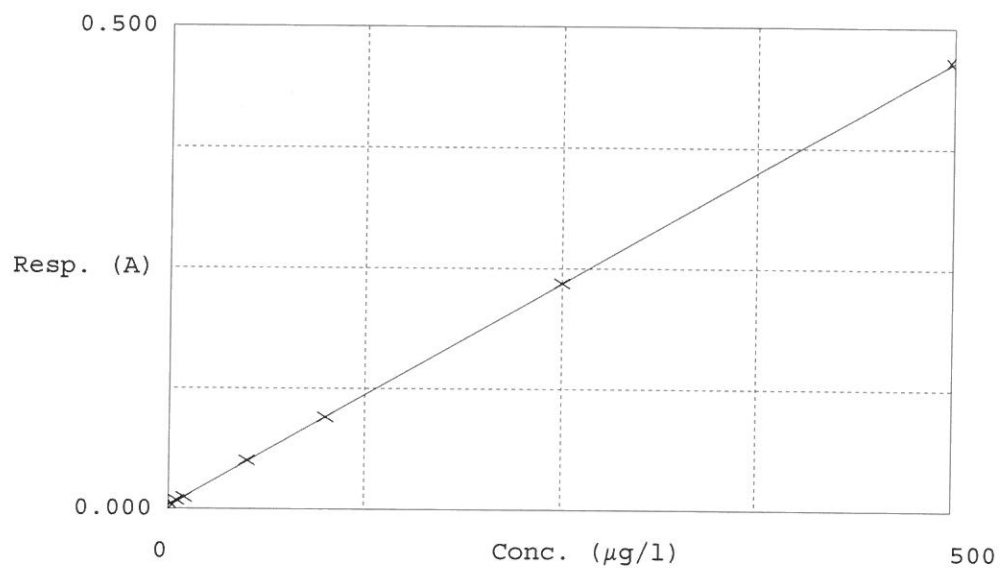

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.4067	0.0000	
2	5.0PPBCN	0.009	5.7922	5.0000	
3	10PPBCN	0.012	9.1858	10.0000	
4	50PPBCN	0.050	50.6381	50.0000	
5	100PPBCN	0.095	99.5216	100.0000	
6	250PPBCN	0.235	250.4576	250.0000	
7	500PPBCN	0.464	499.8114	500.0000	