

LB92570

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

1/11/2018 15:47

Test: Total CN. ug/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.599	0.0	0.095	
ICB1	1.025	0.0	0.004	
CCV1	249.183	0.0	0.236	
CCB1	0.952	0.0	0.004	
PB105584BL	1.037	0.0	0.004	
PB105584BS	97.603	0.0	0.095	
MIDPB105584	244.146	0.0	0.231	
J1086-01	3.876	0.0	0.007	
J1086-01DUP	4.109	0.0	0.007	
J1086-01MS	38.471	0.0	0.039	
J1086-01MSD	38.011	0.0	0.039	
CCV2	247.390	0.0	0.234	
CCB2	1.218	0.0	0.004	

N	13
Mean	78.894
SD	101.7332
CV%	128.95

AS

Aquakem v. 7.2AQ1

Results from time period:

Thu Jan 11 15:38:15 2018

Thu Jan 11 15:46:00 2018

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.1524	µg/l	1/11/2018 11:35:55	
5.OPPBCN	A	Total CN	P	4.747	µg/l	1/11/2018 11:35:56	
10PPBCN	A	Total CN	P	10.2514	µg/l	1/11/2018 11:35:57	
50PPBCN	A	Total CN	P	49.3987	µg/l	1/11/2018 11:35:58	
100PPBCN	A	Total CN	P	100.2679	µg/l	1/11/2018 11:35:59	
250PPBCN	A	Total CN	P	250.3571	µg/l	1/11/2018 11:36:00	
500PPBCN	A	Total CN	P	499.8255	µg/l	1/11/2018 11:36:01	
ICV1	S	Total CN	P	98.5988	µg/l	1/11/2018 15:38:16	
ICB1	S	Total CN	P	1.0248	µg/l	1/11/2018 15:38:18	
CCV1	S	Total CN	P	249.183	µg/l	1/11/2018 15:38:20	
CCB1	S	Total CN	P	0.952	µg/l	1/11/2018 15:38:22	
PB105584BL	S	Total CN	P	1.0368	µg/l	1/11/2018 15:38:23	
PB105584BS	S	Total CN	P	97.6033	µg/l	1/11/2018 15:38:24	
MIDPB105584	S	Total CN	P	244.1464	µg/l	1/11/2018 15:38:25	
J1086-01	S	Total CN	P	3.8757	µg/l	1/11/2018 15:45:50	
J1086-01DUP	S	Total CN	P	4.109	µg/l	1/11/2018 15:45:51	
J1086-01MS	S	Total CN	P	38.4714	µg/l	1/11/2018 15:45:52	
J1086-01MSD	S	Total CN	P	38.0109	µg/l	1/11/2018 15:45:53	
CCV2	S	Total CN	P	247.3899	µg/l	1/11/2018 15:45:54	
CCB2	S	Total CN	P	1.2176	µg/l	1/11/2018 15:45:55	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

1/11/2018 11:45


Test Total CN

Accepted 1/11/2018 11:45

Factor 1071
 Bias 0.003

Coeff. of det. 0.999996

Errors

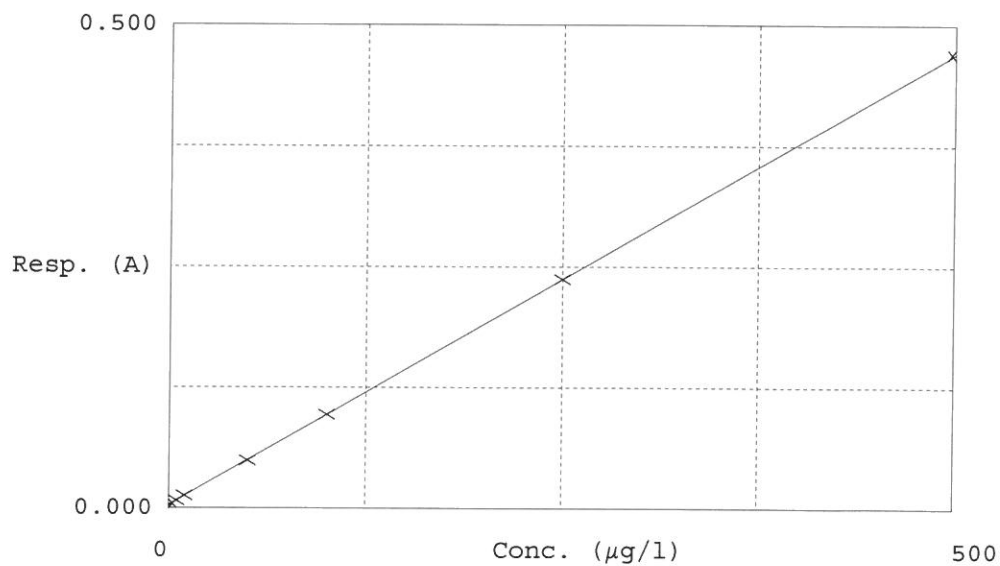

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.1524	0.0000	
2	5.0PPBCN	0.008	4.7470	5.0000	
3	10PPBCN	0.013	10.2514	10.0000	
4	50PPBCN	0.049	49.3987	50.0000	
5	100PPBCN	0.097	100.2679	100.0000	
6	250PPBCN	0.237	250.3571	250.0000	
7	500PPBCN	0.470	499.8255	500.0000	