

IC-3 3000

1-18-18 AK


Clear table

ident	concentrati on F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-01-09_	1/9/18 12:09
STD2	0.1660	0.2120	0.2250	0.7940	0.2070	-0.0930	1.3540	_2018-01-09_	1/9/18 12:40
STD3	0.3880	0.6080	0.6160	2.0890	0.5330	0.9880	3.1130	_2018-01-09_	1/9/18 13:11
STD4	0.7380	1.1810	1.1890	3.9420	0.9760	2.1650	5.5560	_2018-01-09_	1/9/18 13:42
STD5	1.7890	2.8320	2.8080	9.3340	2.3060	4.9990	13.0650	_2018-01-09_	1/9/18 14:13
STD6	3.8580	5.8310	5.8960	19.3940	4.8460	9.3770	27.6040	_2018-01-09_	1/9/18 14:44
STD7	5.1890	7.7580	7.6570	25.5600	6.4020	12.4120	38.5060	_2018-01-09_	1/9/18 15:15
ICV	2.0260	2.9550	3.0120	9.8840	2.4630	5.4030	14.7440	_2018-01-09_	1/9/18 16:48
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-01-09_	1/9/18 17:18
CCV	2.0250	2.8930	2.8550	9.5820	2.3760	5.3140	14.4490	_2018-01-17_	1/17/18 11:31
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-01-17_	1/17/18 12:02
LB92657BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-01-17_	1/17/18 12:33
LB92657BSW	2.1300	2.9460	2.9630	9.9030	2.5190	6.0030	14.9970	_2018-01-17_	1/17/18 13:04
J1176-01	0.0000	0.5930	0.0000	0.0000	0.4270	0.0000	1.0450	_2018-01-17_	1/17/18 13:38
J1176-01DUP	0.0000	0.5770	0.0000	0.0000	0.4280	0.0000	1.0390	_2018-01-17_	1/17/18 14:09
J1176-01MS	1.9770	3.4140	2.9670	9.9340	2.8370	5.7820	15.8040	_2018-01-17_	1/17/18 14:40
CCV	2.0200	2.8960	2.8670	9.6450	2.3840	5.5940	14.3050	_2018-01-17_	1/17/18 15:11
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-01-17_	1/17/18 15:41

IC-1 Cal
1-9-18
AK

CALIBRATION OF COMPONENT F-

Method: ANIONS 01-09-18.mtw
Equation: $Q = 0.865253 \cdot A + 3.32613$
RSD: 8.391 %
Correlation coefficient: 0.997123

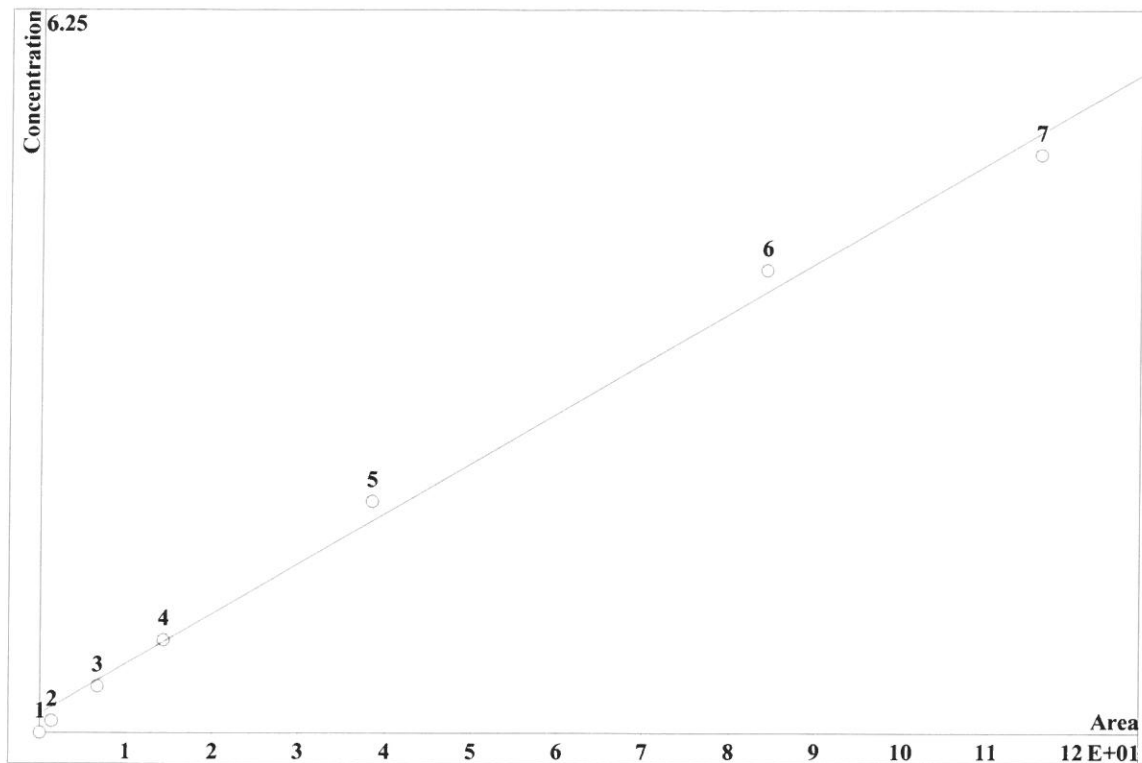

K3 = 0 K2 = 0 K1 = 0.865253 K0 = 3.32613

Base: Area

Ref.channel: Cond

ISTD:

Formula: Linear


Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
-------	--------	------	-------	---------	-----------	------	------

1	0	0	0	0	0	No
2	0.0766	1.337	0.1	20	5.921	Yes
3	0.3686	6.688	0.4	20	5.921	Yes
4	0.8104	14.36	0.8	20	5.921	Yes
5	2.285	38.49	2	20	5.921	Yes
6	5.011	84.26	4	20	5.921	Yes
7	6.577	116.1	5	20	5.921	Yes

CALIBRATION OF COMPONENT CL-

Method: ANIONS 01-09-18.mtw
 Equation: $Q = 1.22609 \cdot A + 2.78279$
 RSD: 7.158 %
 Correlation coefficient: 0.997907

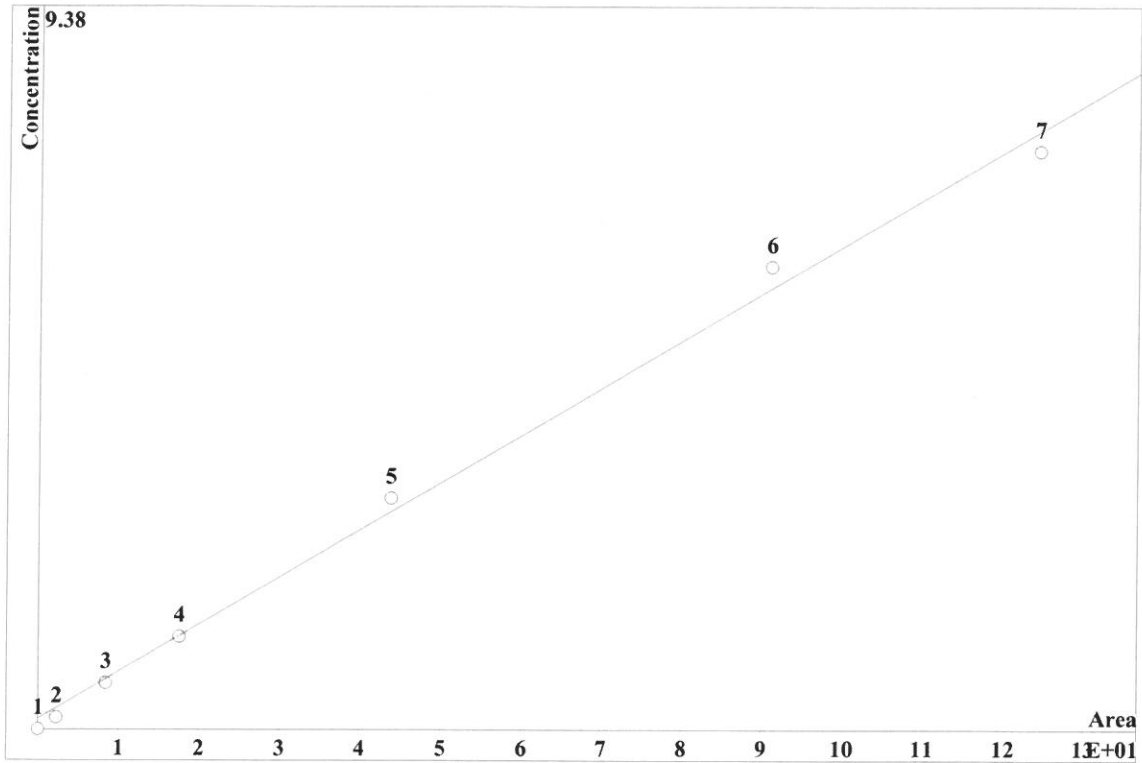


K3 = 0 K2 = 0 K1 = 1.22609 K0 = 2.78279
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.1306	2.234	0.15	20	8.982			Yes
3	0.5148	8.446	0.6	20	8.982			Yes
4	1.055	17.52	1.2	20	8.982			Yes
5	2.696	43.8	3	20	8.982			Yes
6	5.668	91.07	6	20	8.982			Yes
7	7.498	124.3	7.5	20	8.982			Yes

CALIBRATION OF COMPONENT NO2

Method: ANIONS 01-09-18.mtw
 Equation: $Q = 0.528875 \cdot A + 2.77123$
 RSD: 4.862 %
 Correlation coefficient: 0.999035

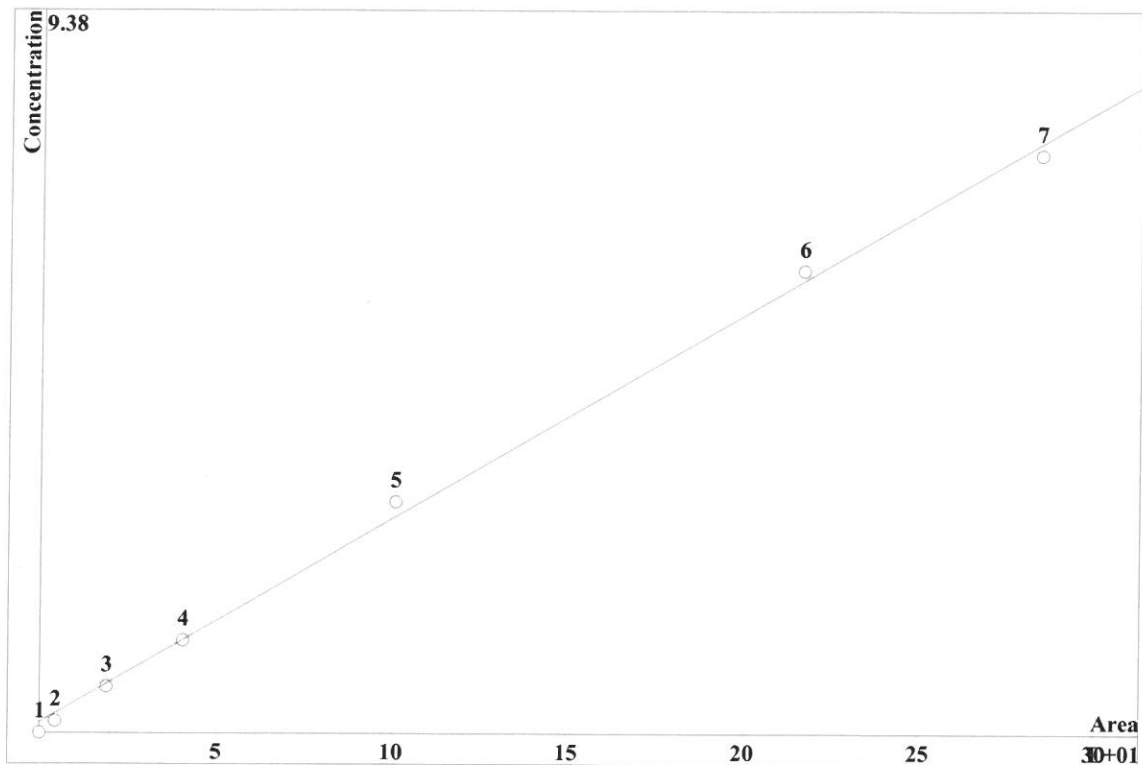


K3 = 0 K2 = 0 K1 = 0.528875 K0 = 2.77123
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0	0	0	0	0			No
2	0.2277	4.437	0.15	20	10.72			Yes
3	0.9898	19.04	0.6	20	10.72			Yes
4	2.054	40.53	1.2	20	10.72			Yes
5	5.295	101	3	20	10.72			Yes
6	11.06	216.9	6	20	10.72			Yes
7	14.37	284.3	7.5	20	10.72			Yes

CALIBRATION OF COMPONENT BR-

Method: ANIONS 01-09-18.mtw
 Equation: $Q = 2.78796 \cdot A + 8.78242$
 RSD: 4.933 %
 Correlation coefficient: 0.999006

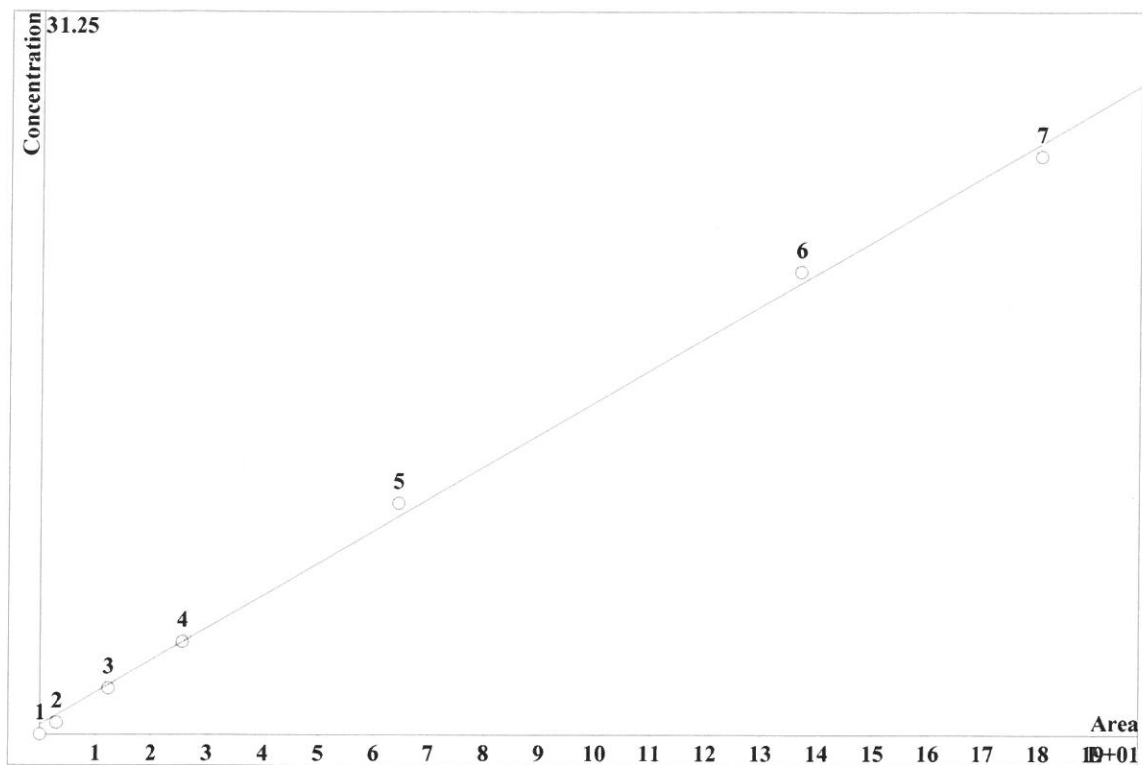


K3 = 0 K2 = 0 K1 = 2.78796 K0 = 8.78242

Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0	No	
2	0.1503	2.896	0.5	20	13.6	Yes	
3	0.6345	12.29	2	20	13.6	Yes	
4	1.33	25.59	4	20	13.6	Yes	
5	3.484	64.49	10	20	13.6	Yes	
6	7.314	136.8	20	20	13.6	Yes	
7	9.625	180.2	25	20	13.6	Yes	

CALIBRATION OF COMPONENT NO3

Method: ANIONS 01-09-18.mtw
 Equation: $Q = 0.49287 \cdot A + 2.43944$
 RSD: 5.457 %
 Correlation coefficient: 0.998784

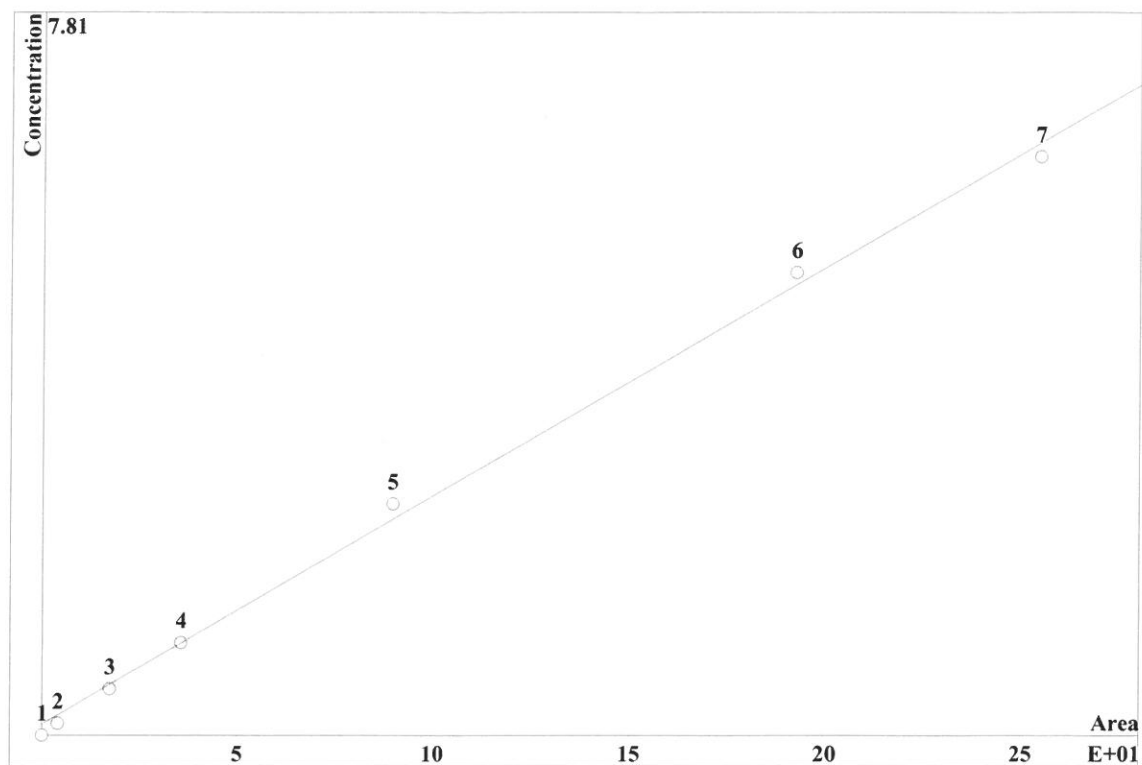


K3 = 0 K2 = 0 K1 = 0.49287 K0 = 2.43944
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File	
1	0		0	0	0		0	No
2	0.1766		3.98	0.125	20		15.49	Yes
3	0.7693		17.39	0.5	20		15.49	Yes
4	1.608		35.48	1	20		15.49	Yes
5	4.242		89.87	2.5	20		15.49	Yes
6	9.115		192.7	5	20		15.49	Yes
7	12.19		254.8	6.25	20		15.49	Yes

CALIBRATION OF COMPONENT HPO4

Method: ANIONS 01-09-18.mtw
 Equation: $Q = 0.869476 \cdot A - 9.63248$
 RSD: 5.661 %
 Correlation coefficient: 0.998691

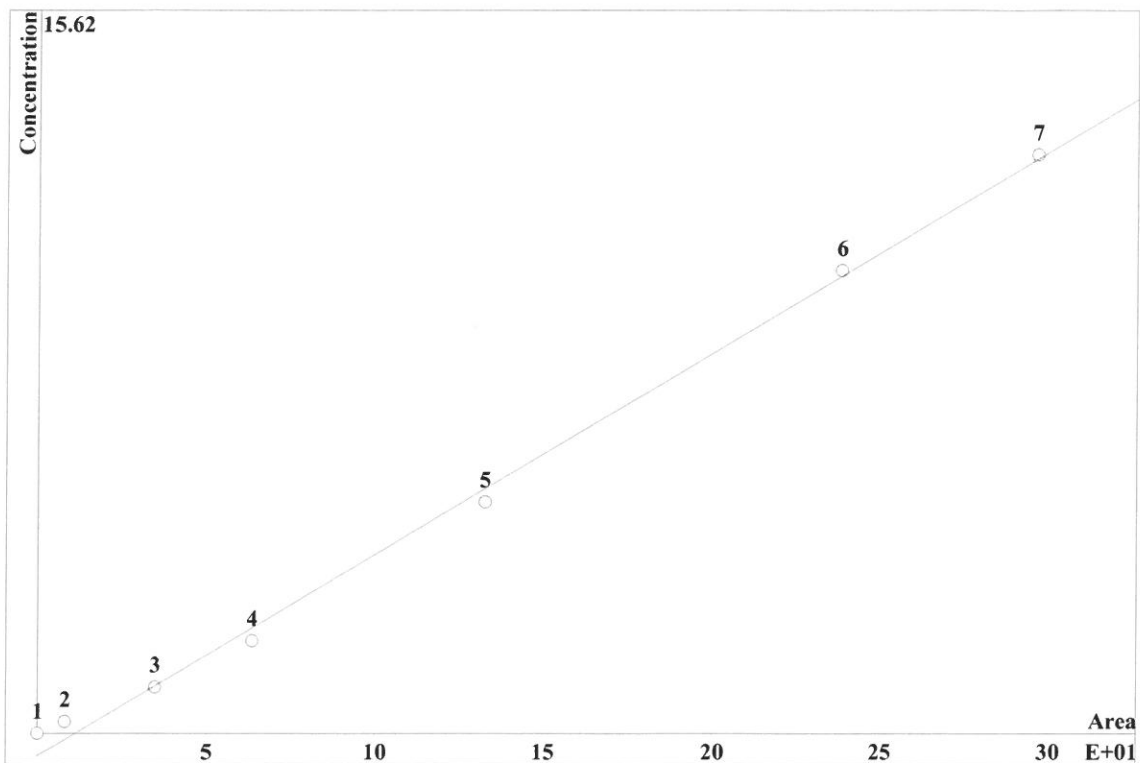


K3 = 0 K2 = 0 K1 = 0.869476 K0 = -9.63248
 Base: Area
 Ref.channel: Cond
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0	No	
2	0.1969	7.867	0.25	20	22.72	Yes	
3	0.8415	34.68	1	20	22.72	Yes	
4	1.57	63.47	2	20	22.72	Yes	
5	3.489	132.8	5	20	22.72	Yes	
6	6.655	238.4	10	20	22.72	Yes	
7	8.553	296.6	12.5	20	22.72	Yes	

CALIBRATION OF COMPONENT SO4

Method: ANIONS 01-09-18.mtw
 Equation: $Q = 1.5738 \cdot A + 15.6978$
 RSD: 5.979 %
 Correlation coefficient: 0.998540

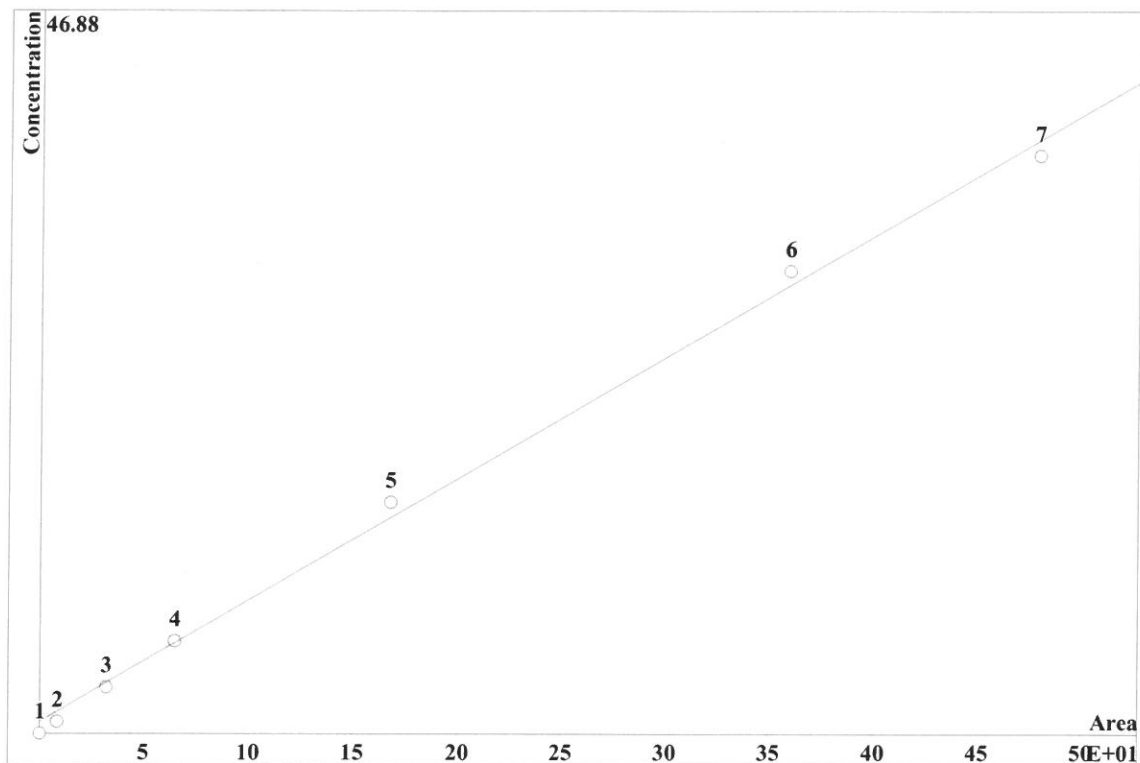

K3 = 0 K2 = 0 K1 = 1.5738 K0 = 15.6978

Base: Area

Ref.channel: Cond

ISTD:

Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
-------	--------	------	-------	---------	-----------	------	------

1	0	0	0	0	0	No
2	0.263	8.206	0.75	20	25.7	Yes
3	1.043	32.09	3	20	25.7	Yes
4	2.153	64.97	6	20	25.7	Yes
5	5.656	168	15	20	25.7	Yes
6	12.21	359.8	30	20	25.7	Yes
7	16.26	479.4	37.5	20	25.7	Yes

Report date: 1/10/2018 2:00:18 PM
Printed by: wet


Ident: STD1
Analysis from: 1/9/2018 12:09:55 PM
File: _2018-01-09_

Last save: 1/10/2018 8:56:20 AM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60598

Last save: 1/9/2018 11:36:28 AM

SAMPLE:
: AP/AK
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

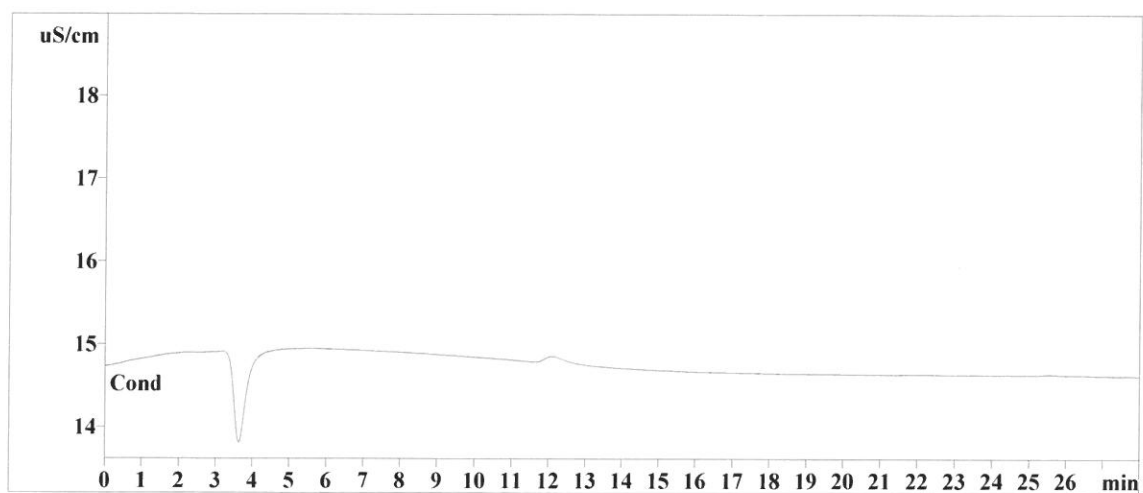

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/10/2018 2:00:29 PM
Printed by: wet


Ident: STD2
Analysis from: 1/9/2018 12:40:50 PM
File: _2018-01-09_

Last save: 1/9/2018 1:08:38 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60599

Last save: 1/9/2018 12:37:44 PM

SAMPLE:
: AP/AK
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

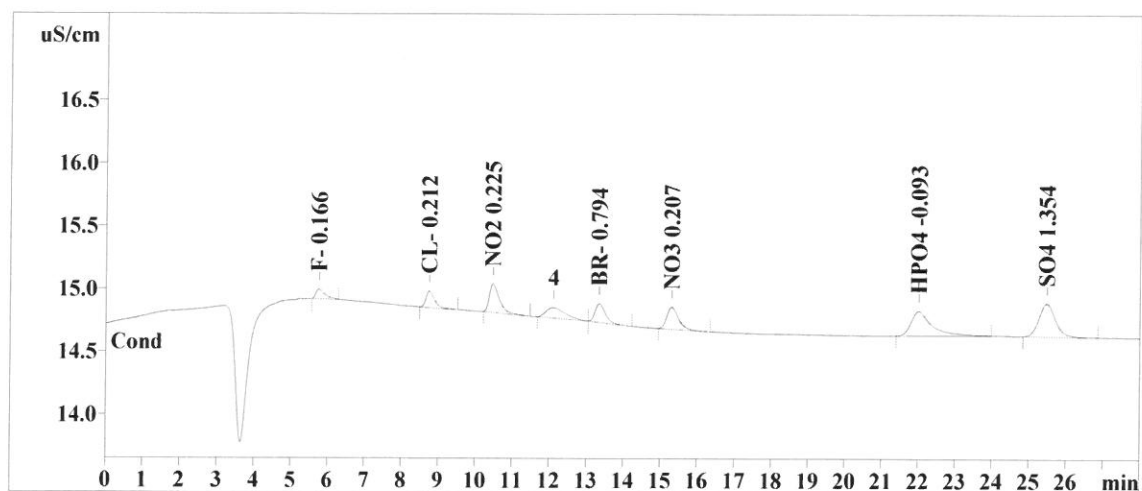

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.75	0.259	0.08	5.81	1.337	3.94	0.
2	8.74	0.253	0.13	10.00	2.234	6.58	0.
3	10.48	0.283	0.23	17.44	4.437	13.07	0.
4	13.35	0.288	0.15	11.47	2.896	8.53	0.
5	15.30	0.339	0.18	13.47	3.980	11.72	0.
6	22.01	0.526	0.20	15.00	7.867	23.17	0.
7	25.48	0.466	0.26	20.12	8.206	24.17	0.
7	28.00	0.345	1.22	93.31	30.957	91.17	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/10/2018 2:00:54 PM
Printed by: wet


Ident: STD3
Analysis from: 1/9/2018 1:11:44 PM
File: _2018-01-09_

Last save: 1/9/2018 1:39:32 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60600

Last save: 1/9/2018 1:08:38 PM

SAMPLE:
: AP/AK
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

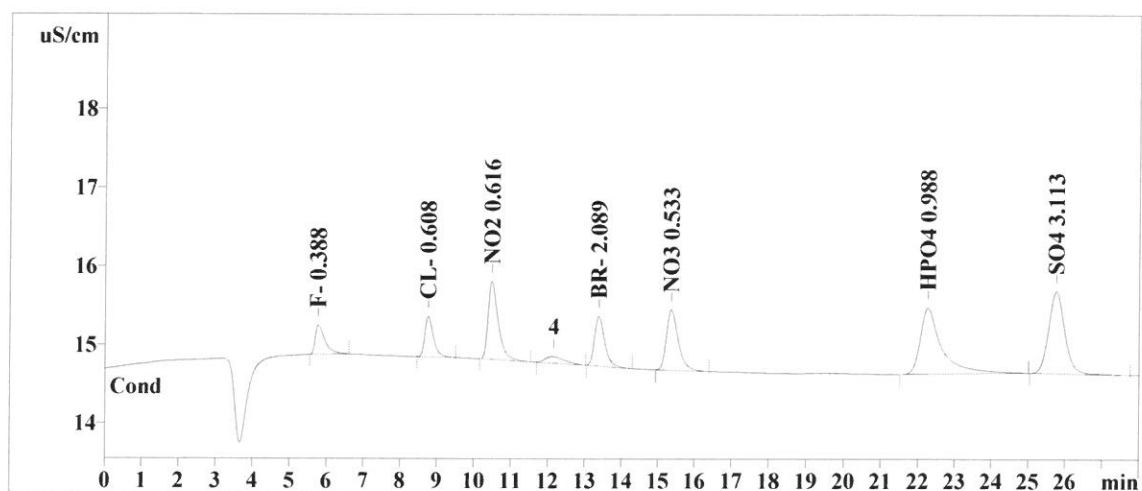

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.78	0.257	0.37	7.02	6.688	5.00	0.
2	8.75	0.244	0.51	9.80	8.446	6.32	0.
3	10.48	0.281	0.99	18.84	19.036	14.24	0.
4	13.38	0.290	0.63	12.08	12.293	9.20	0.
5	15.35	0.333	0.77	14.65	17.390	13.01	0.
6	22.26	0.518	0.84	16.02	34.678	25.94	0.
7	25.76	0.459	1.04	19.87	32.094	24.01	0.
7	28.00	0.340	5.16	98.28	130.626	97.72	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/10/2018 2:01:08 PM
Printed by: wet


Ident: STD4
Analysis from: 1/9/2018 1:42:38 PM
File: _2018-01-09_

Last save: 1/9/2018 2:10:28 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60601

Last save: 1/9/2018 1:39:32 PM

SAMPLE:
: AP/AK
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

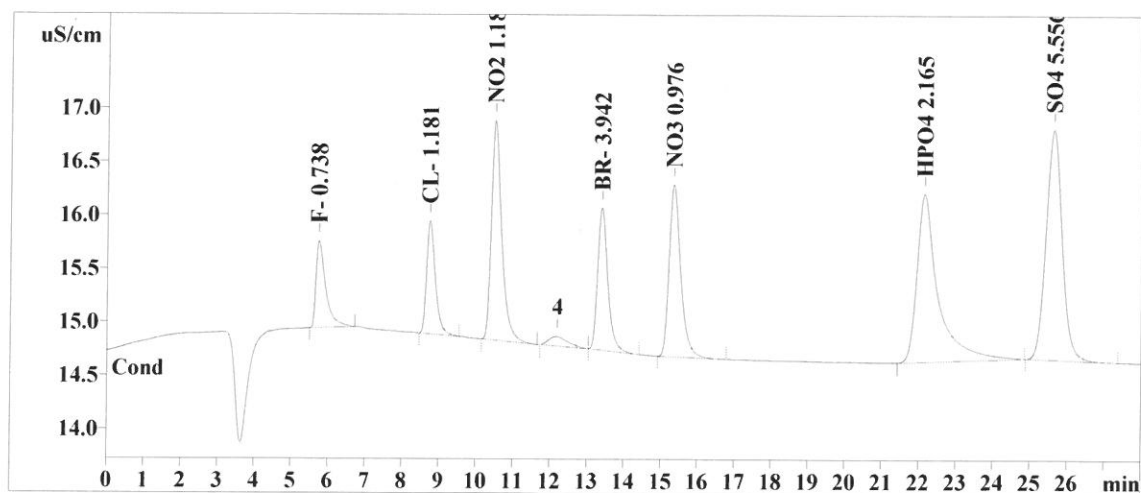

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.75	0.247	0.81	7.59	14.357	5.42	0.
2	8.74	0.247	1.06	9.89	17.517	6.61	0.
3	10.49	0.289	2.05	19.24	40.531	15.29	0.
4	13.39	0.286	1.33	12.46	25.592	9.65	0.
5	15.32	0.324	1.61	15.07	35.478	13.38	0.
6	22.14	0.508	1.57	14.72	63.472	23.94	0.
7	25.62	0.453	2.15	20.17	64.970	24.51	0.
7	28.00	0.336	10.58	99.15	261.916	98.79	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/10/2018 2:01:20 PM
Printed by: wet


Ident: STD5
Analysis from: 1/9/2018 2:13:33 PM
File: _2018-01-09_

Last save: 1/9/2018 2:41:22 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60602

Last save: 1/9/2018 2:10:28 PM

SAMPLE:
: AP/AK
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

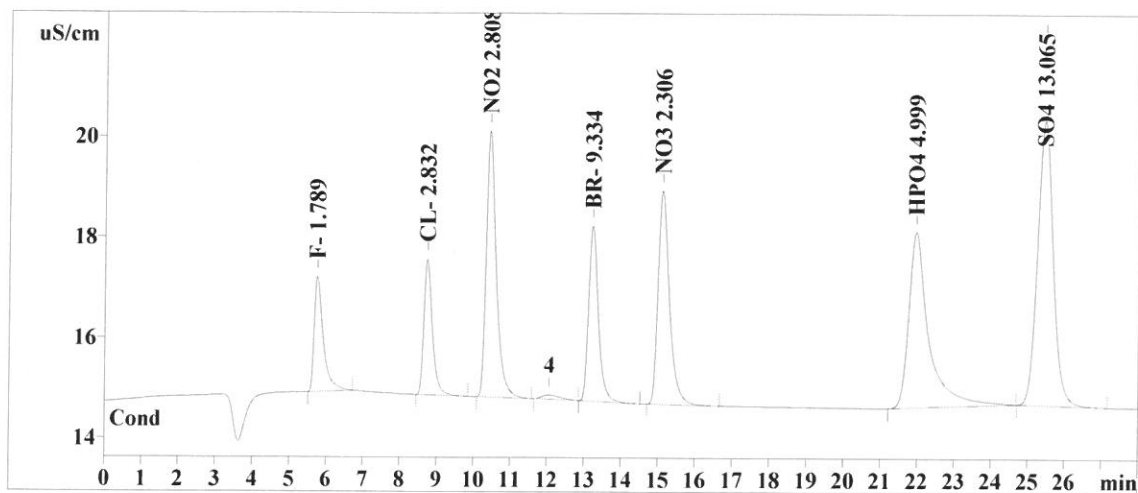

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.74	0.236	2.28	8.39	38.494	6.00	0.
2	8.72	0.239	2.70	9.90	43.798	6.83	0.
3	10.42	0.279	5.30	19.44	101.010	15.75	0.
4	13.23	0.274	3.48	12.79	64.487	10.05	0.
5	15.09	0.309	4.24	15.57	89.874	14.01	0.
6	21.95	0.487	3.49	12.81	132.810	20.70	0.
7	25.44	0.446	5.66	20.76	168.027	26.19	0.
7	28.00	0.324	27.15	99.67	638.500	99.54	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/10/2018 2:01:32 PM
Printed by: wet


Ident: STD6
Analysis from: 1/9/2018 2:44:27 PM
File: _2018-01-09_

Last save: 1/9/2018 3:12:16 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60603

Last save: 1/9/2018 2:41:22 PM

SAMPLE:
: AP/AK
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

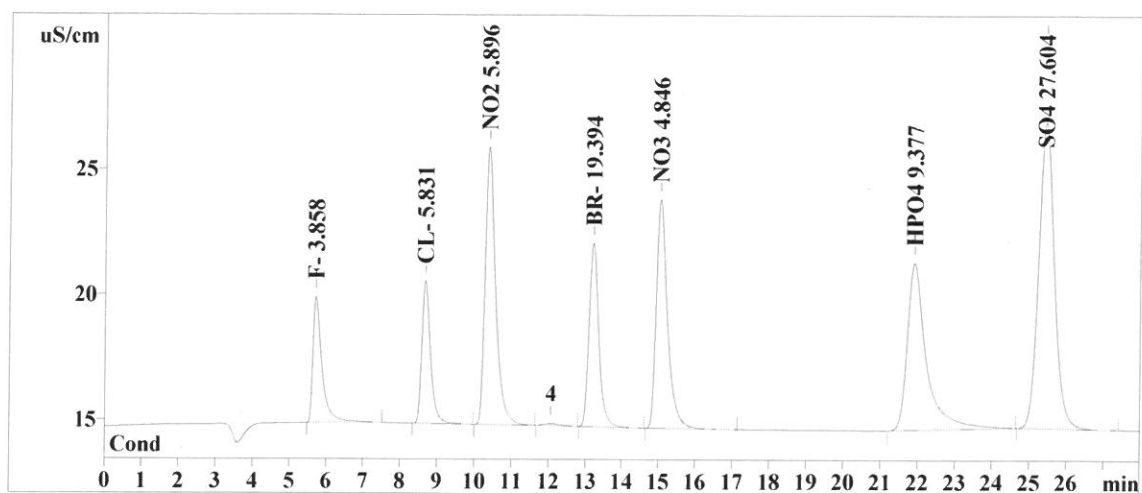

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.229	5.01	8.77	84.262	6.37	0.
2	8.67	0.235	5.67	9.92	91.070	6.89	0.
3	10.36	0.288	11.05	19.36	216.946	16.40	0.
4	13.20	0.277	7.31	12.80	136.802	10.34	0.
5	15.04	0.306	9.11	15.96	192.657	14.57	0.
6	21.90	0.467	6.66	11.65	238.377	18.02	0.
7	25.43	0.442	12.21	21.38	359.816	27.20	0.
7	28.00	0.321	57.03	99.85	1319.930	99.80	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/10/2018 2:01:43 PM
Printed by: wet


Ident: STD7
Analysis from: 1/9/2018 3:15:22 PM
File: _2018-01-09_

Last save: 1/9/2018 3:43:10 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60604

Last save: 1/9/2018 3:12:16 PM

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

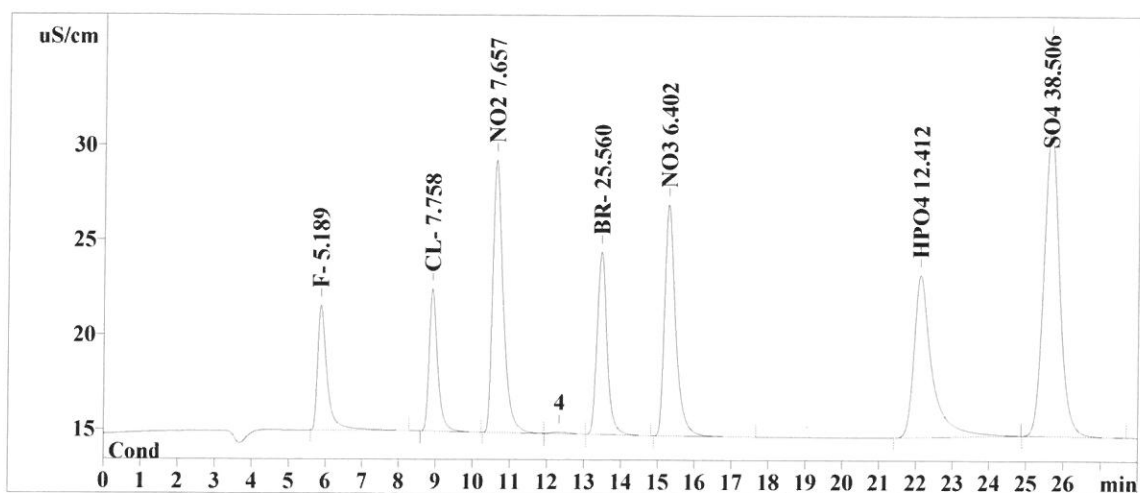

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.86	0.239	6.58	8.75	116.107	6.68	0.
2	8.90	0.244	7.50	9.98	124.273	7.15	0.
3	10.62	0.292	14.37	19.13	284.309	16.36	0.
4	13.46	0.279	9.63	12.81	180.213	10.37	0.
5	15.27	0.303	12.19	16.22	254.821	14.66	0.
6	22.11	0.457	8.55	11.38	296.590	17.06	0.
7	25.64	0.441	16.26	21.63	479.365	27.58	0.
7	28.00	0.322	75.07	99.90	1735.678	99.86	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/10/2018 2:02:52 PM
Printed by: wet


Ident: ICV
Analysis from: 1/9/2018 4:48:05 PM
File: _2018-01-09_

Last save: 1/9/2018 5:15:54 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60607

Last save: 1/9/2018 3:43:10 PM

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

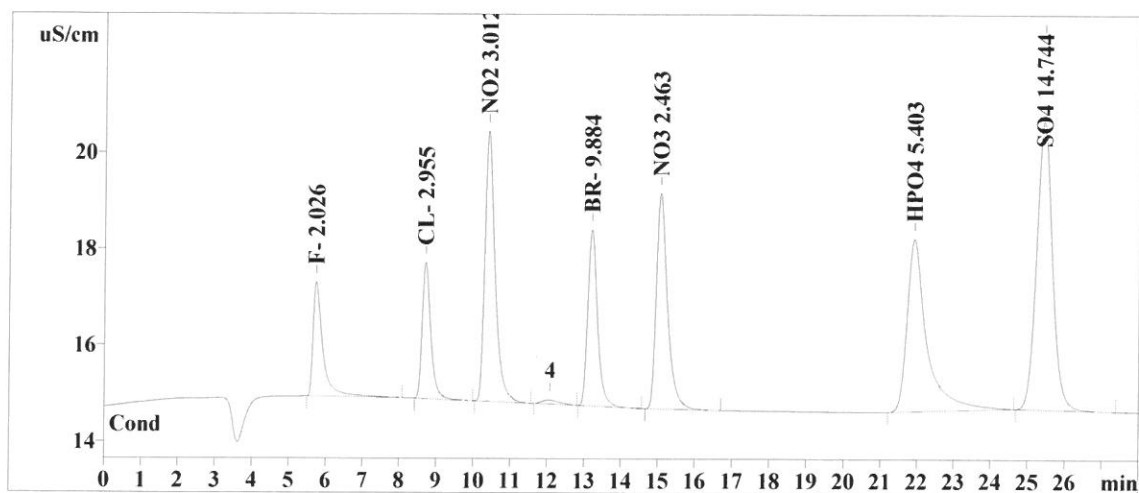

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.73	0.239	2.37	8.29	42.978	6.36	0.
2	8.69	0.240	2.82	9.88	45.935	6.80	0.
3	10.39	0.285	5.60	19.62	108.668	16.08	0.
4	13.20	0.275	3.65	12.79	67.756	10.02	0.
5	15.05	0.311	4.47	15.66	95.007	14.06	0.
6	21.91	0.484	3.57	12.52	135.372	20.03	0.
7	25.42	0.446	5.98	20.95	177.399	26.25	0.
7	28.00	0.326	28.46	99.70	673.115	99.59	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/10/2018 2:03:31 PM
Printed by: wet


Ident: ICB
Analysis from: 1/9/2018 5:18:59 PM
File: _2018-01-09_

Last save: 1/10/2018 2:03:28 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60608

Last save: 1/9/2018 3:43:10 PM

SAMPLE:
: AK/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

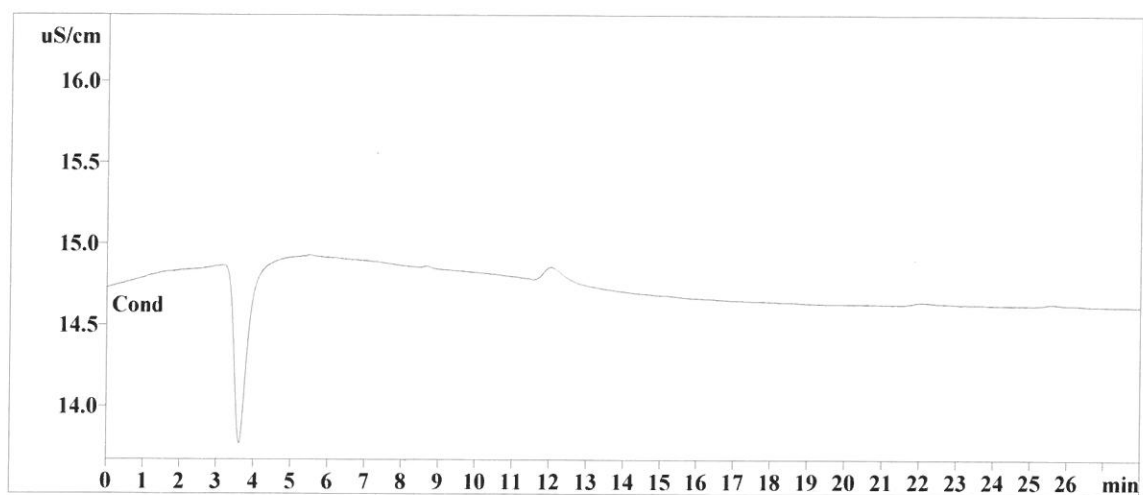

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/18/2018 9:30:28 AM
Printed by: wet


Ident: CCV
Analysis from: 1/17/2018 11:31:02 AM
File: _2018-01-17_

Last save: 1/17/2018 11:58:52 AM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60700

Last save: 1/9/2018 3:43:10 PM

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

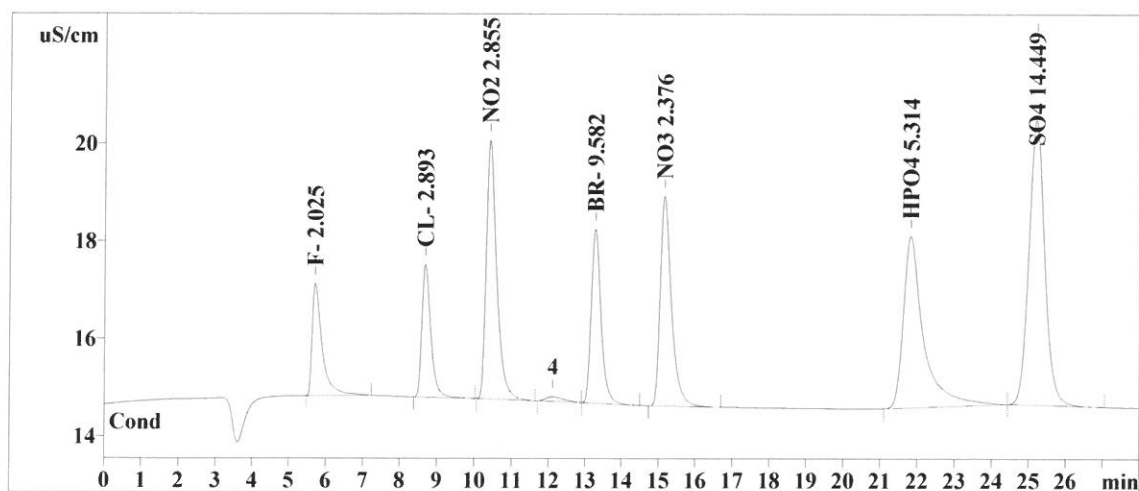

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.71	0.255	2.30	8.33	42.955	6.53	0.
2	8.68	0.242	2.72	9.84	44.915	6.83	0.
3	10.40	0.284	5.30	19.20	102.724	15.61	0.
4	13.27	0.273	3.56	12.88	65.586	9.97	0.
5	15.14	0.311	4.29	15.55	91.482	13.90	0.
6	21.81	0.486	3.52	12.73	133.320	20.26	0.
7	25.18	0.447	5.83	21.11	173.641	26.39	0.
7	28.00	0.328	27.52	99.64	654.623	99.49	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/18/2018 9:30:59 AM
Printed by: wet


Ident: CCB
Analysis from: 1/17/2018 12:02:55 PM
File: _2018-01-17_

Last save: 1/18/2018 9:30:56 AM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60701

Last save: 1/9/2018 3:43:10 PM

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

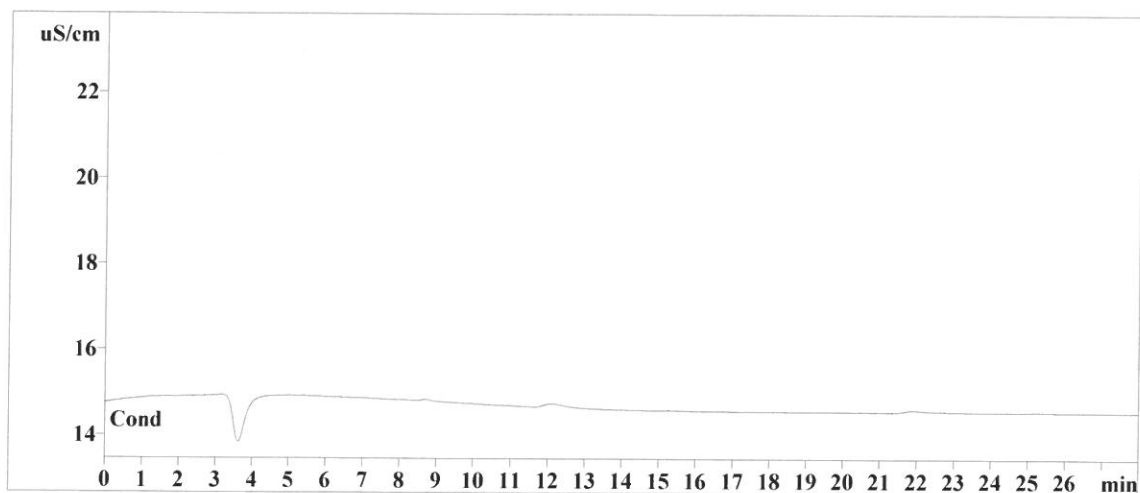

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/18/2018 9:31:19 AM
Printed by: wet


Ident: LB92657BLW
Analysis from: 1/17/2018 12:33:49 PM
File: _2018-01-17_

Last save: 1/18/2018 9:31:16 AM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60702

Last save: 1/9/2018 3:43:10 PM

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

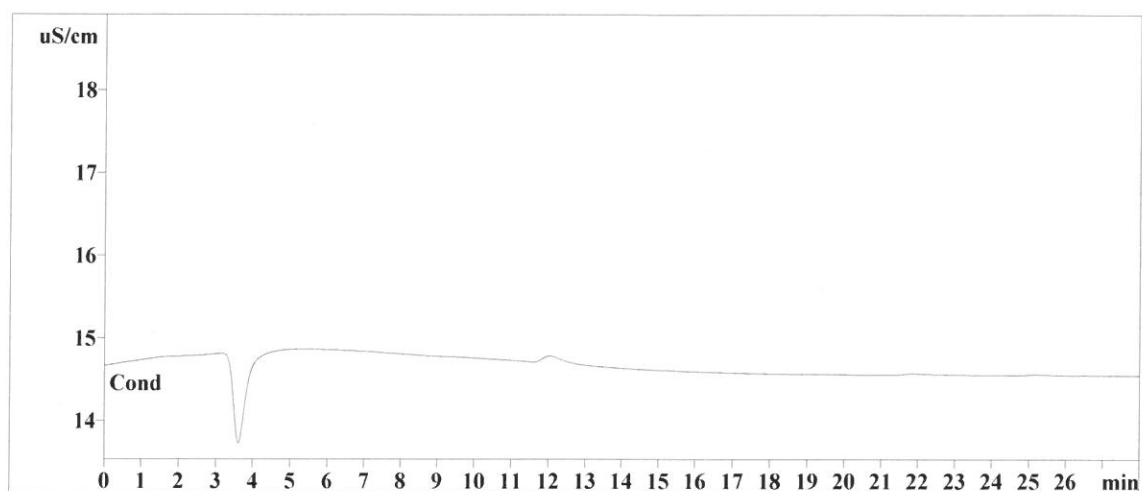

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 1/18/2018 9:31:57 AM
Printed by: wet


Ident: LB92657BSW
Analysis from: 1/17/2018 1:04:44 PM
File: _2018-01-17_

Last save: 1/18/2018 9:27:54 AM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60703

Last save: 1/9/2018 3:43:10 PM

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

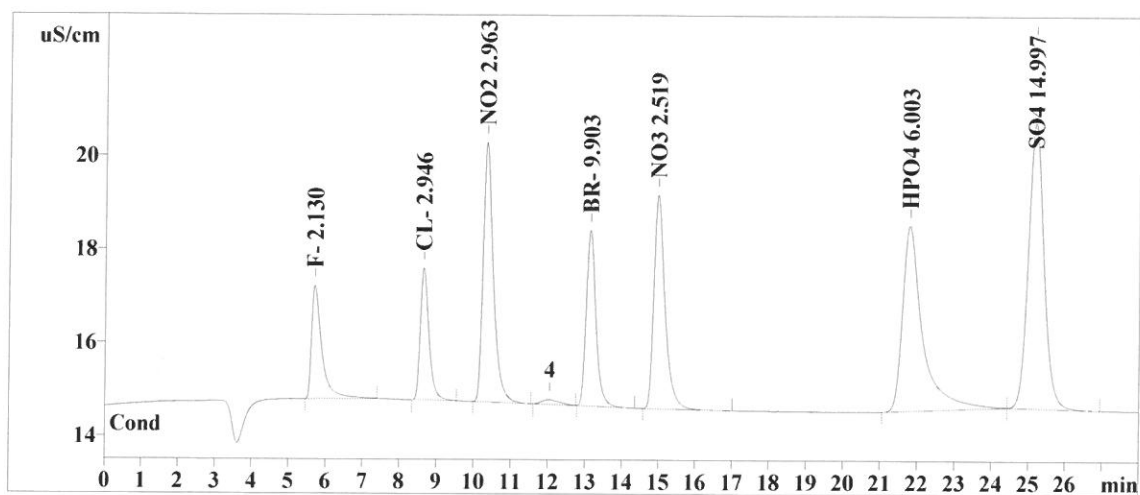

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.70	0.254	2.42	8.25	45.389	6.52	0.
2	8.64	0.240	2.82	9.63	45.784	6.58	0.
3	10.32	0.282	5.55	18.95	106.828	15.34	0.
4	13.13	0.268	3.76	12.83	67.888	9.75	0.
5	14.96	0.311	4.57	15.61	97.283	13.97	0.
6	21.78	0.483	3.96	13.53	149.173	21.42	0.
7	25.17	0.446	6.11	20.85	180.614	25.94	0.
7	28.00	0.326	29.19	99.64	692.957	99.52	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/18/2018 9:32:11 AM
Printed by: wet


Ident: J1176-01
Analysis from: 1/17/2018 1:38:17 PM
File: _2018-01-17_

Last save: 1/18/2018 9:30:00 AM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60704

Last save: 1/9/2018 3:43:10 PM

SAMPLE:
: AK/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

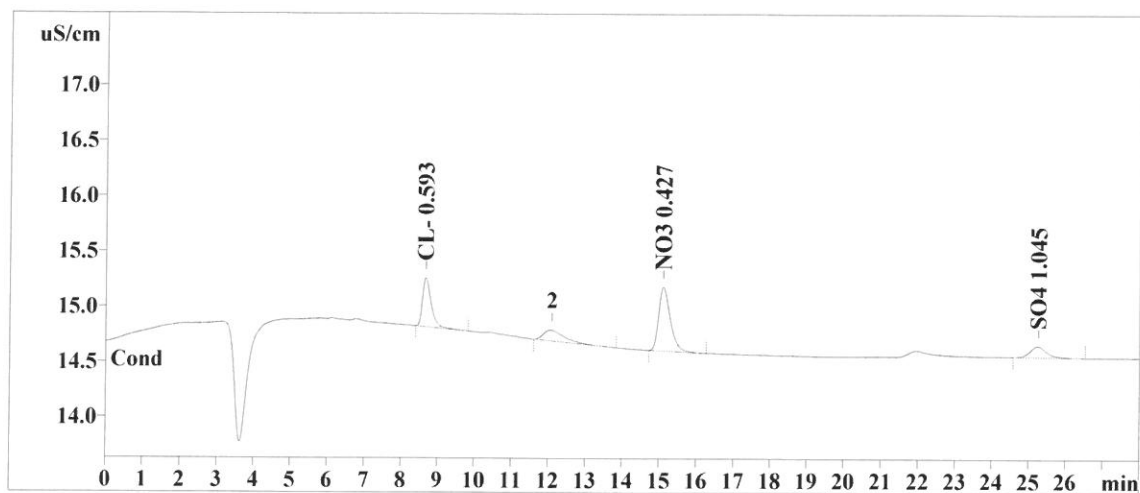

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	0.00	0.000	0.00	0.00	0.000	0.00	0.
2	8.66	0.245	0.44	36.14	7.409	27.34	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	0.00	0.000	0.00	0.00	0.000	0.00	0.
5	15.10	0.319	0.58	47.26	12.364	45.62	0.
6	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	25.24	0.468	0.10	8.31	3.311	12.22	0.
7	28.00	0.148	1.12	91.70	23.085	85.17	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/18/2018 9:32:25 AM
Printed by: wet


Ident: J1176-01DUP
Analysis from: 1/17/2018 2:09:12 PM
File: _2018-01-17_

Last save: 1/17/2018 2:37:00 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60705

Last save: 1/9/2018 3:43:10 PM

SAMPLE:
: AK/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

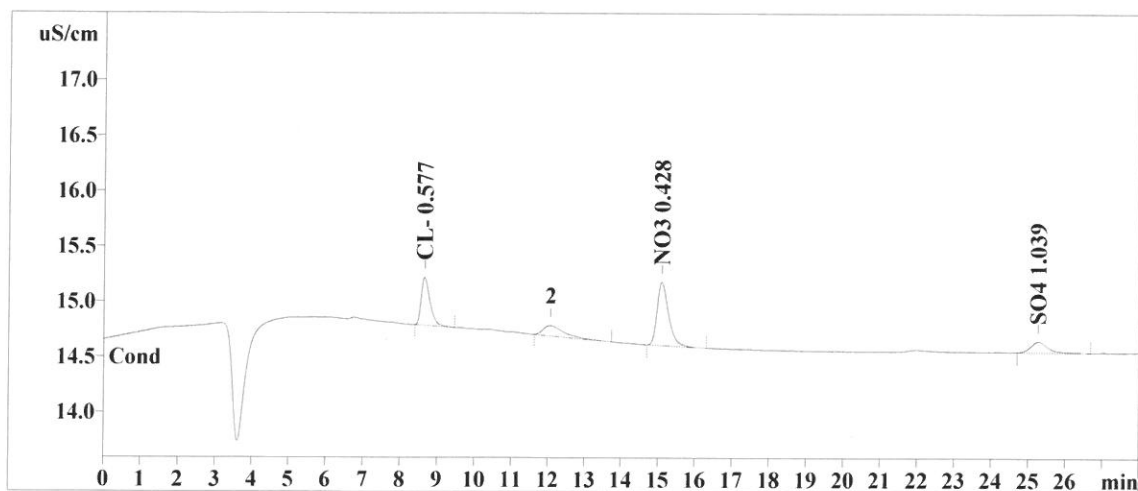

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	0.00	0.000	0.00	0.00	0.000	0.00	0.
2	8.65	0.246	0.43	36.01	7.145	26.80	0.
3	0.00	0.000	0.00	0.00	0.000	0.00	0.
4	0.00	0.000	0.00	0.00	0.000	0.00	0.
5	15.08	0.321	0.57	47.62	12.418	46.58	0.
6	0.00	0.000	0.00	0.00	0.000	0.00	0.
7	25.27	0.468	0.10	8.26	3.223	12.09	0.
7	28.00	0.148	1.10	91.88	22.787	85.46	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/18/2018 9:32:36 AM
Printed by: wet


Ident: J1176-01MS
Analysis from: 1/17/2018 2:40:06 PM
File: _2018-01-17_

Last save: 1/17/2018 3:07:54 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60706

Last save: 1/9/2018 3:43:10 PM

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

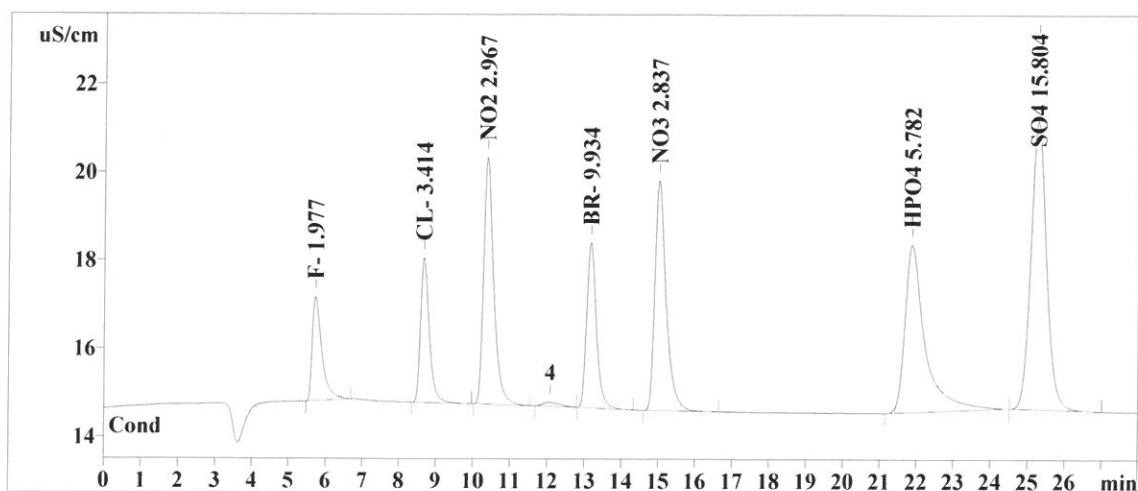

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.72	0.252	2.36	7.71	41.865	5.83	0.
2	8.67	0.240	3.27	10.70	53.416	7.43	0.
3	10.36	0.281	5.59	18.27	106.964	14.89	0.
4	13.16	0.270	3.74	12.24	68.111	9.48	0.
5	15.00	0.308	5.21	17.02	110.184	15.34	0.
6	21.87	0.485	3.79	12.39	144.071	20.05	0.
7	25.26	0.439	6.53	21.35	190.867	26.57	0.
7	28.00	0.325	30.50	99.68	715.478	99.59	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/18/2018 9:32:50 AM
Printed by: wet


Ident: CCV
Analysis from: 1/17/2018 3:11:00 PM
File: _2018-01-17_

Last save: 1/17/2018 3:38:50 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60707

Last save: 1/9/2018 3:43:10 PM

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

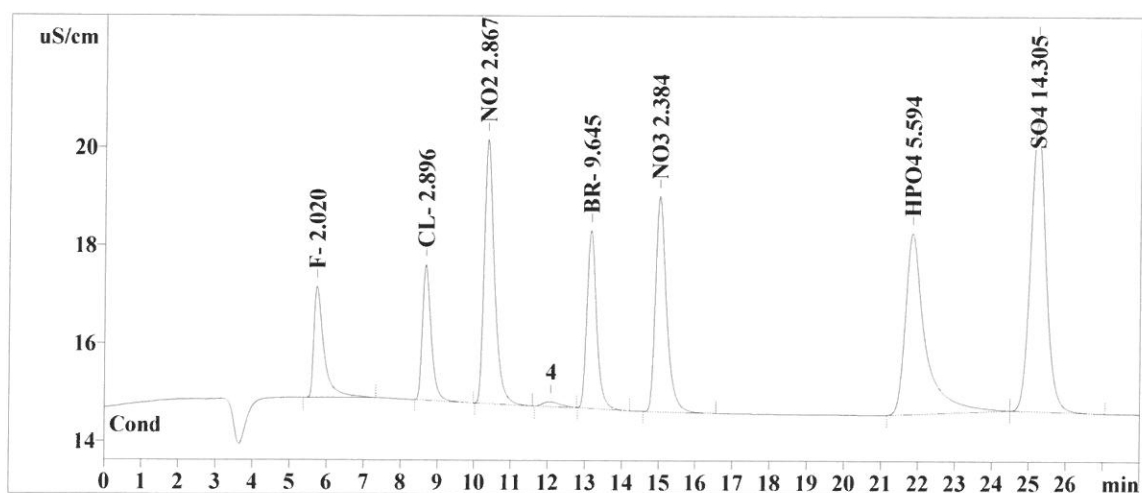

Quantitation method: Custom

No	Retention min	Width/2 min	Height uS/cm	Height %	Area uS/cm*sec	Area %	
1	5.73	0.255	2.26	8.05	42.843	6.46	0.
2	8.67	0.240	2.76	9.83	44.962	6.78	0.
3	10.35	0.281	5.39	19.17	103.191	15.55	0.
4	13.15	0.271	3.62	12.90	66.041	9.95	0.
5	15.00	0.306	4.39	15.63	91.775	13.83	0.
6	21.83	0.485	3.69	13.12	139.757	21.06	0.
7	25.22	0.439	5.88	20.95	171.813	25.89	0.
7	28.00	0.325	27.99	99.65	660.382	99.52	0.

This report has been created by IC Net
METROHM LTD

Report date: 1/18/2018 9:34:54 AM
Printed by: wet


Ident: CCB
Analysis from: 1/17/2018 3:41:55 PM
File: _2018-01-17_

Last save: 1/17/2018 4:09:44 PM

Method: ANIONS 01-09-18.mtw
Run operator: wet
Analysis number: 60708

Last save: 1/9/2018 3:43:10 PM

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

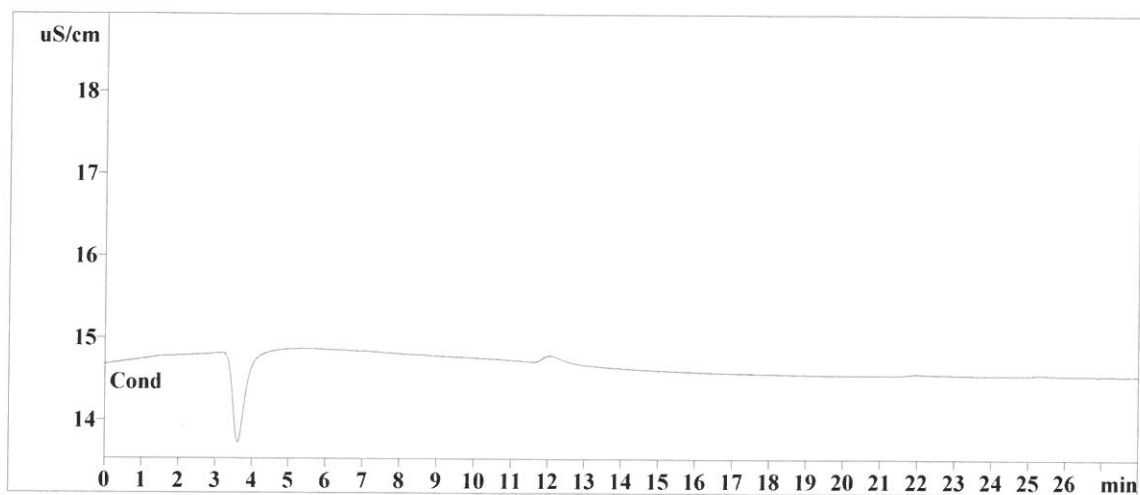

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD