

21392853

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

1/24/2018 17:14

Reactive
Test: Total CN. ug/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.467	0.0	0.092	
ICB1	0.118	0.0	0.004	
CCV1	239.003	0.0	0.225	
CCB1	0.123	0.0	0.004	
PB105957BL	-0.046	0.0	0.004	
J1279-02	-0.132	0.0	0.004	
J1279-02DUP	-0.042	0.0	0.004	
J1281-08	-0.173	0.0	0.004	
PB105956BL	-0.239	0.0	0.003	
J1270-01	-0.235	0.0	0.003	
J1270-01DUP	-0.180	0.0	0.004	
CCV2	249.023	0.0	0.234	
CCB2	0.056	0.0	0.004	

N	13
Mean	44.826
SD	92.2527
CV%	205.80

AS

Aquakem v. 7.2AQ1

Results from time period:

Wed Jan 24 17:08:31 2018

Wed Jan 24 17:13:52 2018

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.0996	µg/l	1/24/2018 11:50:08	
5.0PPBCN	A	Reactive CN	P	4.6879	µg/l	1/24/2018 11:50:09	
10PPBCN	A	Reactive CN	P	10.2417	µg/l	1/24/2018 11:50:10	
50PPBCN	A	Reactive CN	P	51.4474	µg/l	1/24/2018 11:50:11	
100PPBCN	A	Reactive CN	P	100.7528	µg/l	1/24/2018 11:50:12	
250PPBCN	A	Reactive CN	P	246.5336	µg/l	1/24/2018 11:50:13	
500PPBCN	A	Reactive CN	P	501.4362	µg/l	1/24/2018 11:50:14	
ICV1	S	Reactive CN	P	95.467	µg/l	1/24/2018 17:08:32	
ICB1	S	Reactive CN	P	0.1182	µg/l	1/24/2018 17:08:34	
CCV1	S	Reactive CN	P	239.0035	µg/l	1/24/2018 17:08:35	
CCB1	S	Reactive CN	P	0.123	µg/l	1/24/2018 17:08:38	
PB105957BL	S	Reactive CN	P	-0.0461	µg/l	1/24/2018 17:08:39	
J1279-02	S	Reactive CN	P	-0.132	µg/l	1/24/2018 17:08:40	
J1279-02DUP	S	Reactive CN	P	-0.0423	µg/l	1/24/2018 17:08:41	
J1281-08	S	Reactive CN	P	-0.1728	µg/l	1/24/2018 17:13:47	
PB105956BL	S	Reactive CN	P	-0.2392	µg/l	1/24/2018 17:13:48	
J1270-01	S	Reactive CN	P	-0.2348	µg/l	1/24/2018 17:13:49	
J1270-01DUP	S	Reactive CN	P	-0.1796	µg/l	1/24/2018 17:13:50	
CCV2	S	Reactive CN	P	249.0225	µg/l	1/24/2018 17:13:51	
CCB2	S	Reactive CN	P	0.056	µg/l	1/24/2018 17:13:52	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

1/24/2018 11:52


Test Total CN

Accepted 1/24/2018 11:52

Factor 1080
 Bias 0.004

Coeff. of det. 0.999918

Errors

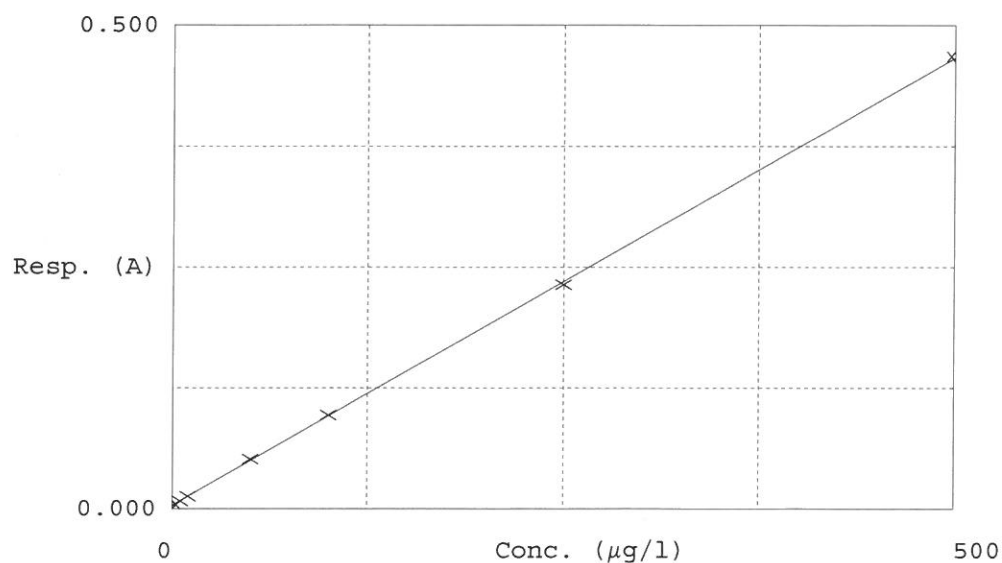

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.0996	0.0000	
2	5.0PPBCN	0.008	4.6879	5.0000	
3	10PPBCN	0.013	10.2417	10.0000	
4	50PPBCN	0.051	51.4474	50.0000	
5	100PPBCN	0.097	100.7528	100.0000	
6	250PPBCN	0.232	246.5336	250.0000	
7	500PPBCN	0.468	501.4362	500.0000	