

2B93385

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

2/19/2018 14:16

Test: ^{Reactive} ~~Total~~ CN ^{Mg/d}

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.911	0.0	0.090	
ICB1	0.779	0.0	0.004	
CCV1	250.292	0.0	0.226	
CCB1	0.921	0.0	0.004	
PB106649BL	0.544	0.0	0.004	
J1392-02	0.410	0.0	0.004	
J1392-02DUP	0.676	0.0	0.004	
J1604-03	0.449	0.0	0.004	
J1604-06	0.714	0.0	0.004	
J1604-09	0.483	0.0	0.004	
J1604-12	0.518	0.0	0.004	
PB106650BL	0.425	0.0	0.004	
J1601-03	0.367	0.0	0.004	
J1601-03DUP	0.475	0.0	0.004	
CCV2	263.436	0.0	0.238	
CCB2	0.627	0.0	0.004	

N 16
Mean 38.689
SD 88.5761
CV% 228.94

AS

Aquakem v. 7.2AQ1

Results from time period:

Mon Feb 19 14:10:46 2018

Mon Feb 19 14:15:37 2018

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.1759	µg/l	2/19/2018 12:31:21	
5.OPPBCN	A	Reactive CN	P	4.9028	µg/l	2/19/2018 12:31:22	
10PPBCN	A	Reactive CN	P	9.9386	µg/l	2/19/2018 12:31:23	
50PPBCN	A	Reactive CN	P	50.094	µg/l	2/19/2018 12:31:24	
100PPBCN	A	Reactive CN	P	98.8742	µg/l	2/19/2018 12:31:25	
250PPBCN	A	Reactive CN	P	251.5932	µg/l	2/19/2018 12:31:26	
500PPBCN	A	Reactive CN	P	499.4214	µg/l	2/19/2018 12:31:27	
ICV1	S	Reactive CN	P	97.9108	µg/l	2/19/2018 14:10:46	
ICB1	S	Reactive CN	P	0.779	µg/l	2/19/2018 14:10:47	
CCV1	S	Reactive CN	P	250.2915	µg/l	2/19/2018 14:10:48	
CCB1	S	Reactive CN	P	0.9209	µg/l	2/19/2018 14:10:49	
PB106649BL	S	Reactive CN	P	0.5444	µg/l	2/19/2018 14:10:50	
J1392-02	S	Reactive CN	P	0.41	µg/l	2/19/2018 14:10:51	
J1392-02DUP	S	Reactive CN	P	0.6761	µg/l	2/19/2018 14:10:52	
J1604-03	S	Reactive CN	P	0.4488	µg/l	2/19/2018 14:10:53	
J1604-06	S	Reactive CN	P	0.714	µg/l	2/19/2018 14:10:54	
J1604-09	S	Reactive CN	P	0.4829	µg/l	2/19/2018 14:10:55	
J1604-12	S	Reactive CN	P	0.5175	µg/l	2/19/2018 14:10:56	
PB106650BL	S	Reactive CN	P	0.4251	µg/l	2/19/2018 14:15:33	
J1601-03	S	Reactive CN	P	0.3672	µg/l	2/19/2018 14:15:34	
J1601-03DUP	S	Reactive CN	P	0.4751	µg/l	2/19/2018 14:15:35	
CCV2	S	Reactive CN	P	263.4364	µg/l	2/19/2018 14:15:36	
CCB2	S	Reactive CN	P	0.6272	µg/l	2/19/2018 14:15:37	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

2/19/2018 12:34


Test Total CN

Accepted 2/19/2018 12:33

Factor 1122
Bias 0.003

Coeff. of det. 0.999980

Errors

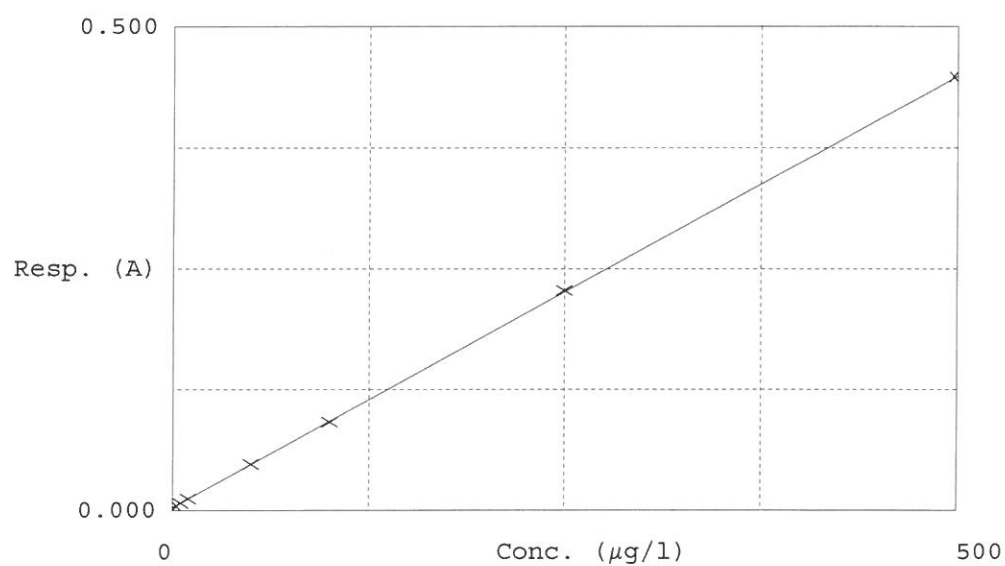

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.1759	0.0000	
2	5.0PPBCN	0.008	4.9028	5.0000	
3	10PPBCN	0.012	9.9386	10.0000	
4	50PPBCN	0.048	50.0940	50.0000	
5	100PPBCN	0.091	98.8742	100.0000	
6	250PPBCN	0.227	251.5932	250.0000	
7	500PPBCN	0.448	499.4214	500.0000	