

LB 94036

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

3/20/2018 15:00

Test: ^{Reactive} Total CN MyId

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.388	0.0	0.097	
ICB1	-0.276	0.0	0.004	
CCV1	245.205	0.0	0.237	
CCB1	-0.302	0.0	0.004	
PB107511BL	0.011	0.0	0.004	
J1760-04	0.024	0.0	0.004	
J1760-04DUP	-0.098	0.0	0.004	
J1974-02	-0.082	0.0	0.004	
J1975-07	-0.022	0.0	0.004	
J1977-04	0.053	0.0	0.004	
J1979-04	-0.032	0.0	0.004	
PB107512BL	-0.392	0.0	0.004	
J1979-06	0.291	0.0	0.004	
J1979-06DUP	-0.114	0.0	0.004	
CCV2	263.738	0.0	0.254	
CCB2	0.221	0.0	0.004	

N	16
Mean	37.851
SD	88.0322
CV%	232.58

AS

Aquakem v. 7.2AQ1

Results from time period:

Tue Mar 20 14:53:09 2018

Tue Mar 20 14:58:00 2018

Sample Id	Sam/Ctr/c/	Test short narr	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.5947	µg/l	3/20/2018 13:25:24	
5.OPPBCN	A	Reactive CN	P	4.4882	µg/l	3/20/2018 13:25:25	
10PPBCN	A	Reactive CN	P	9.7086	µg/l	3/20/2018 13:25:26	
50PPBCN	A	Reactive CN	P	49.0807	µg/l	3/20/2018 13:25:27	
100PPBCN	A	Reactive CN	P	101.1829	µg/l	3/20/2018 13:25:28	
250PPBCN	A	Reactive CN	P	252.5361	µg/l	3/20/2018 13:25:29	
500PPBCN	A	Reactive CN	P	498.5982	µg/l	3/20/2018 13:25:30	
ICV1	S	Reactive CN	P	97.3882	µg/l	3/20/2018 14:53:09	
ICB1	S	Reactive CN	P	-0.2758	µg/l	3/20/2018 14:53:10	
CCV1	S	Reactive CN	P	245.205	µg/l	3/20/2018 14:53:11	
CCB1	S	Reactive CN	P	-0.3015	µg/l	3/20/2018 14:53:12	
PB107511BL	S	Reactive CN	P	0.0109	µg/l	3/20/2018 14:53:13	
J1760-04	S	Reactive CN	P	0.0237	µg/l	3/20/2018 14:53:14	
J1760-04DUP	S	Reactive CN	P	-0.0981	µg/l	3/20/2018 14:53:15	
J1974-02	S	Reactive CN	P	-0.0824	µg/l	3/20/2018 14:53:16	
J1975-07	S	Reactive CN	P	-0.0225	µg/l	3/20/2018 14:53:17	
J1977-04	S	Reactive CN	P	0.0533	µg/l	3/20/2018 14:53:18	
J1979-04	S	Reactive CN	P	-0.0317	µg/l	3/20/2018 14:53:19	
PB107512BL	S	Reactive CN	P	-0.3925	µg/l	3/20/2018 14:57:56	
J1979-06	S	Reactive CN	P	0.2906	µg/l	3/20/2018 14:57:57	
J1979-06DUP	S	Reactive CN	P	-0.1145	µg/l	3/20/2018 14:57:58	
CCV2	S	Reactive CN	P	263.7377	µg/l	3/20/2018 14:57:59	
CCB2	S	Reactive CN	P	0.2215	µg/l	3/20/2018 14:58:00	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

3/20/2018 13:26


Test Total CN

Accepted 3/20/2018 13:26

Factor 1053
 Bias 0.004

Coeff. of det. 0.999945

Errors

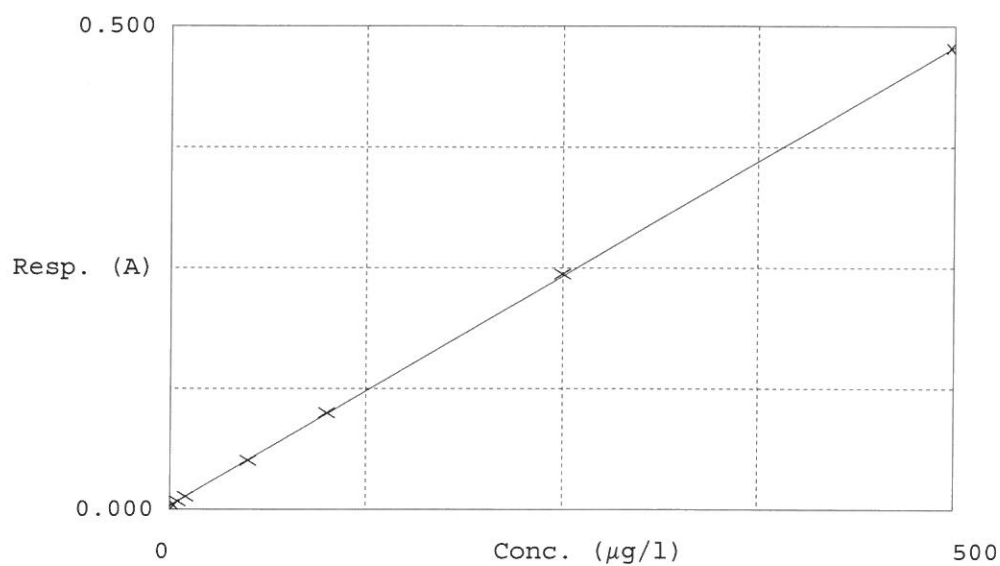

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	-0.5947	0.0000	
2	5.0PPBCN	0.008	4.4882	5.0000	
3	10PPBCN	0.013	9.7086	10.0000	
4	50PPBCN	0.051	49.0807	50.0000	
5	100PPBCN	0.100	101.1829	100.0000	
6	250PPBCN	0.244	252.5361	250.0000	
7	500PPBCN	0.477	498.5982	500.0000	