

IC-2 300.0
3-30-18 AK

Clear table

ident	concentrati on F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-03-12_	3/12/18 14:48
STD2	0.0990	0.1700	0.1920	0.5550	0.1400	0.0800	0.9150	_2018-03-12_	3/12/18 15:19
STD3	0.3930	0.5930	0.6030	1.9660	0.4940	1.1310	3.0090	_2018-03-12_	3/12/18 15:50
STD4	0.7850	1.1340	1.1260	3.7810	0.9390	1.9910	5.6420	_2018-03-12_	3/12/18 16:21
STD5	2.0420	3.0590	3.0180	10.2330	2.5570	5.2610	15.1600	_2018-03-12_	3/12/18 16:52
STD6	3.9820	6.0440	6.0430	20.1410	5.0470	9.6050	30.2060	_2018-03-12_	3/12/18 17:22
STD7	5.0010	7.4500	7.4680	24.8250	6.1980	12.6820	37.3180	_2018-03-12_	3/12/18 17:53
ICV	1.9420	2.8620	2.8360	9.5800	2.3790	4.6970	14.2480	_2018-03-12_	3/12/18 19:26
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-03-12_	3/12/18 19:57
CCV	2.0540	3.1220	3.0670	10.4650	2.6030	5.9890	14.3810	_2018-03-28_	3/28/18 9:38
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-03-28_	3/28/18 10:09
LB94228BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-03-28_	3/28/18 10:40
LB94228BSW	2.0760	3.1380	3.1140	10.5720	2.6500	6.3170	15.2620	_2018-03-28_	3/28/18 11:11
J2116-01	0.5360	308.5520	0.0000	0.4210	0.0000	0.0000	68.4920	_2018-03-28_	3/28/18 13:37
J2116-04	0.1610	255.2590	0.0000	0.2790	0.0000	0.0000	36.2140	_2018-03-28_	3/28/18 14:08
J2116-06	0.1580	256.4760	0.0000	0.2810	0.0000	0.0000	37.5980	_2018-03-28_	3/28/18 14:39
J2116-05	0.3380	264.6070	0.0000	0.0000	2.4720	0.0000	45.4890	_2018-03-28_	3/28/18 15:10
J2116-07	0.0850	242.3140	0.0000	0.0000	1.3990	0.0000	15.6700	_2018-03-28_	3/28/18 15:41
J2116-01DUP	0.3620	282.8870	0.0000	0.3270	0.0000	0.0000	45.7560	_2018-03-28_	3/28/18 16:12
J2116-02MS	2.8320	261.3490	2.9770	10.7820	2.6530	0.0820	55.6860	_2018-03-28_	3/28/18 16:43
J2116-03MSD	2.6830	259.4300	2.7270	9.9980	2.4770	0.2210	52.2340	_2018-03-28_	3/28/18 17:14
CCV	2.1170	3.2130	3.1430	10.6780	2.7070	7.7680	14.7060	_2018-03-28_	3/28/18 17:45
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-03-28_	3/28/18 18:16
J2116-01DLX5	0.0670	105.5680	0.0000	0.0000	0.0000	0.0000	8.1060	_2018-03-28_	3/28/18 18:47
J2116-01DL2X100	0.0000	5.0780	0.0000	0.0000	0.0000	0.0000	0.6240	_2018-03-28_	3/28/18 19:18
J2116-04DLX50	0.0000	7.4380	0.0000	0.0000	0.0000	0.0000	0.9570	_2018-03-28_	3/28/18 19:49
J2116-06DLX2	0.0740	154.0230	0.0000	0.0000	0.0000	0.0000	17.5720	_2018-03-28_	3/28/18 20:20
J2116-06DL2X50	0.0000	7.3030	0.0000	0.0000	0.0000	0.0000	0.9230	_2018-03-28_	3/28/18 20:51
J2116-05DLX2	0.0650	178.4150	0.0000	0.0000	1.1080	0.0000	18.2970	_2018-03-28_	3/28/18 21:22
CCV	2.0360	3.1110	3.0320	10.2770	2.5680	6.7530	14.2560	_2018-03-28_	3/28/18 22:55


CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2018-03-28	3/28/18 23:26
CCV	1.9190	2.9090	2.8770	9.7920	2.4410	5.6690	13.2810	2018-03-29	3/29/18 8:30
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2018-03-29	3/29/18 9:03
LB94228BLW2	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2018-03-29	3/29/18 9:34
LB94228BSW2	2.0250	3.0660	3.0390	10.3060	2.5820	6.2270	14.8880	2018-03-29	3/29/18 10:05
J2116-05DLX100	0.0000	4.6090	0.0000	0.0000	0.0000	0.0000	0.0000	2018-03-29	3/29/18 10:36
J2116-07DLX100	0.0000	4.6120	0.0000	0.0000	0.0000	0.0000	0.0000	2018-03-29	3/29/18 11:07
CCV	1.9650	2.9750	2.9190	9.9350	2.4820	6.0780	13.5810	2018-03-29	3/29/18 11:38
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	2018-03-29	3/29/18 12:09

IC-2

3-12-18 AK

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.0326208 \cdot A + 0.253285$
 RSD: 1.183 %
 Correlation coefficient: 0.999943

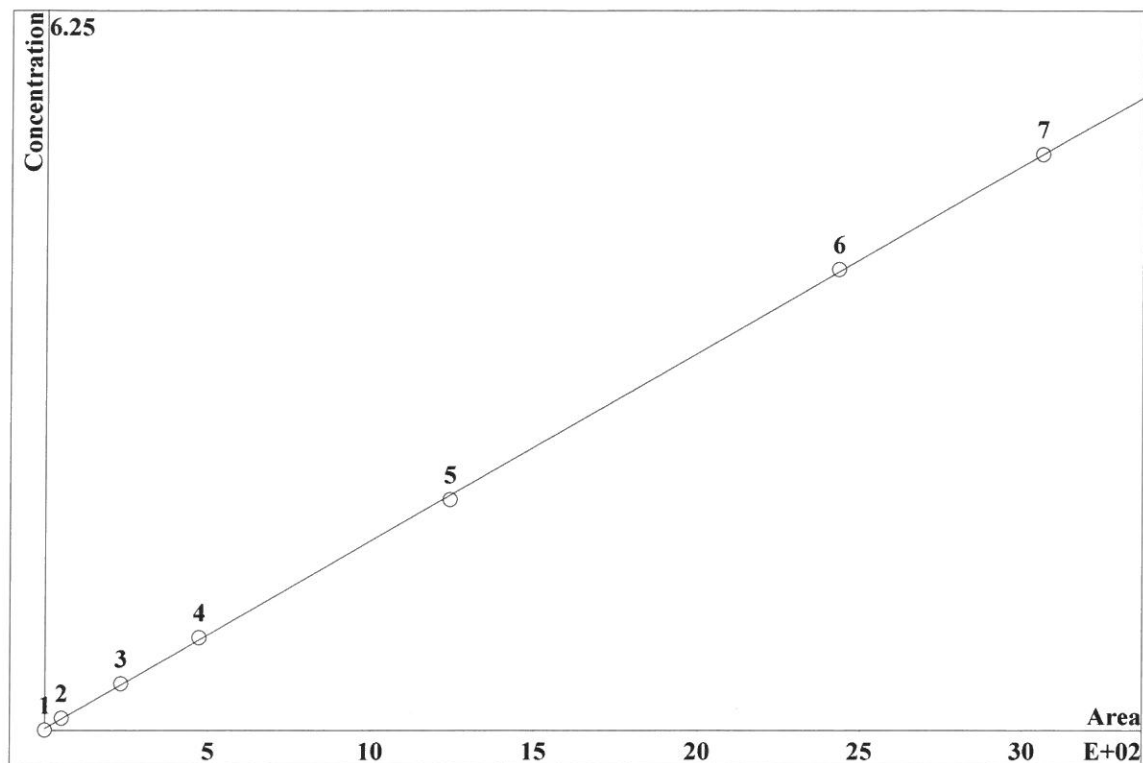

K3 = 0 K2 = 0 K1 = 0.0326208 K0 = 0.253285

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	3.69	52.63	0.1	20	5.099		
3	15.34	233.2	0.4	20	5.099		
4	31.64	473.3	0.8	20	5.099		
5	84.72	1244	2	20	5.099		
6	162.6	2433	4	20	5.099		
7	204.1	3058	5	20	5.099		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.0497015 \cdot A + 0.332296$
 RSD: 1.834 %
 Correlation coefficient: 0.999863

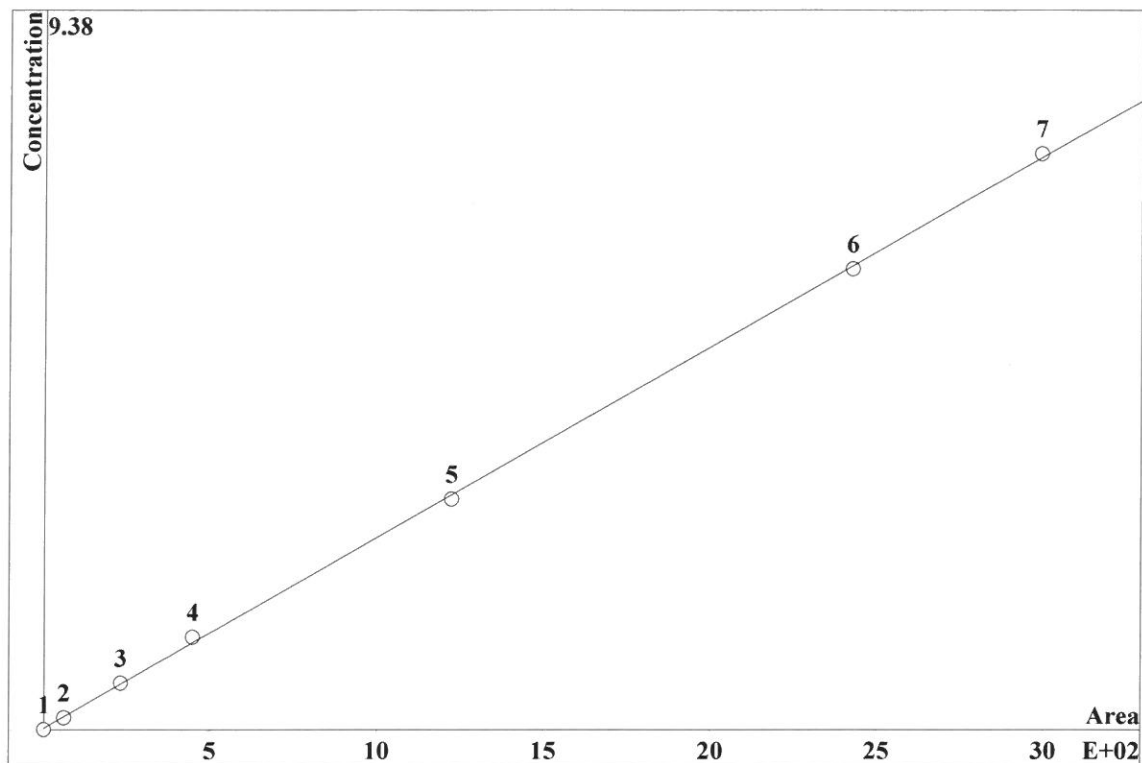

K3 = 0 K2 = 0 K1 = 0.0497015 K0 = 0.332296

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.212	61.67	0.15	20	8.753		
3	15.96	231.8	0.6	20	8.753		
4	30.65	449.6	1.2	20	8.753		
5	84.5	1224	3	20	8.753		
6	169	2425	6	20	8.753		
7	207.6	2991	7.5	20	8.753		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.0206268 \cdot A + 1.27253$
 RSD: 1.661 %
 Correlation coefficient: 0.999887

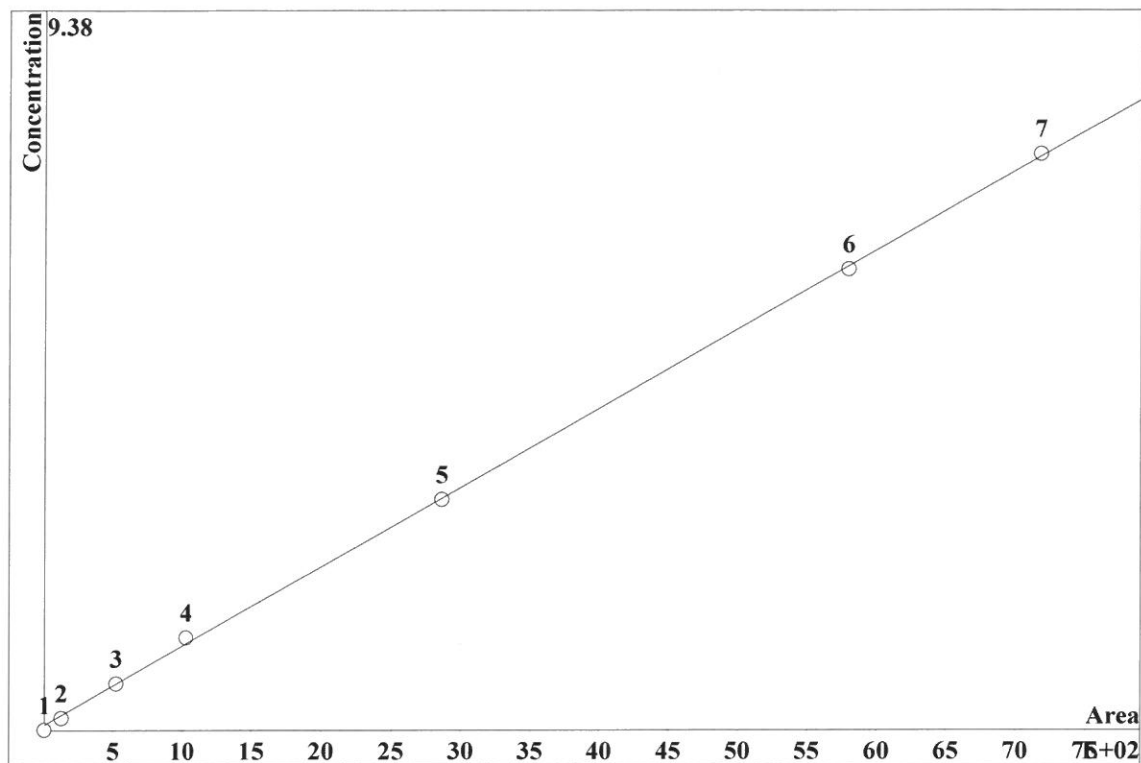

K3 = 0 K2 = 0 K1 = 0.0206268 K0 = 1.27253

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.466	124.7	0.15	20	11.21		
3	30.77	523.1	0.6	20	11.21		
4	60.82	1030	1.2	20	11.21		
5	170.2	2864	3	20	11.21		
6	342.3	5798	6	20	11.21		
7	425.3	7179	7.5	20	11.21		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.112224 \cdot A + 1.31848$
 RSD: 1.932 %
 Correlation coefficient: 0.999848

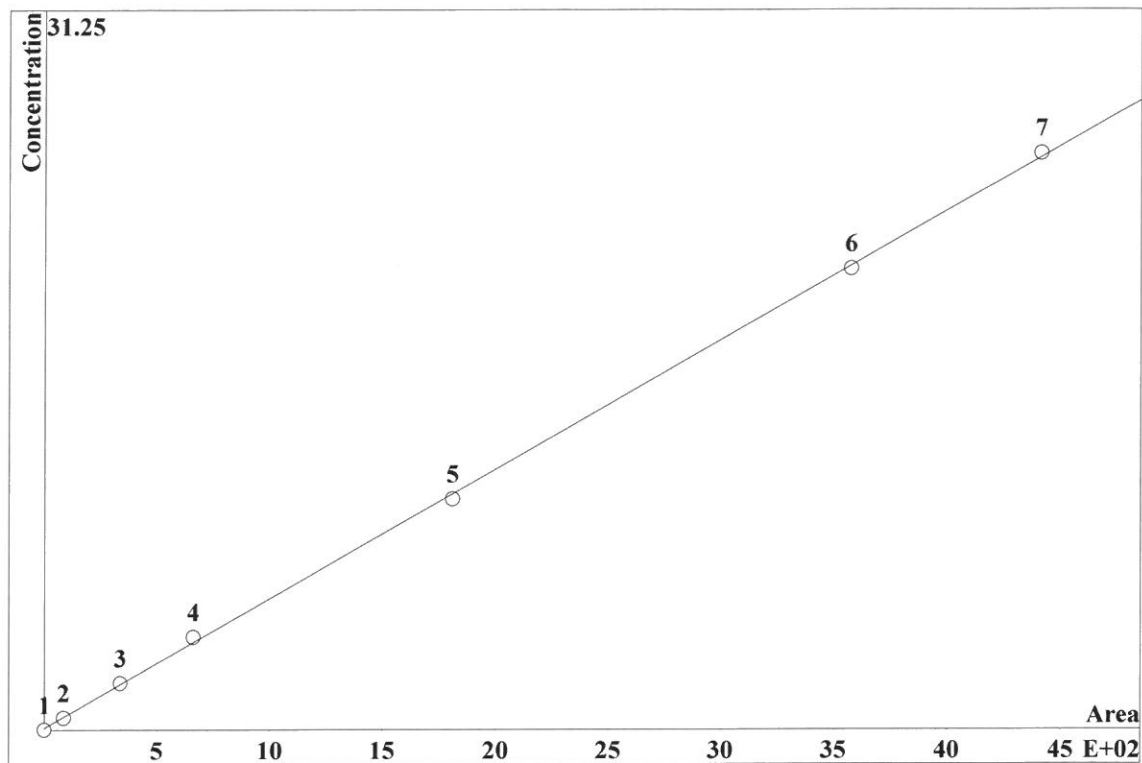


K3 = 0 K2 = 0 K1 = 0.112224 K0 = 1.31848
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	3.607	87.1	0.5	20	14.51		
3	14.28	338.6	2	20	14.51		
4	27.68	662.1	4	20	14.51		
5	75.39	1812	10	20	14.51		
6	148.6	3578	20	20	14.51		
7	181.8	4412	25	20	14.51		

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.020582 \cdot A + 0.358059$
 RSD: 2.151 %
 Correlation coefficient: 0.999811

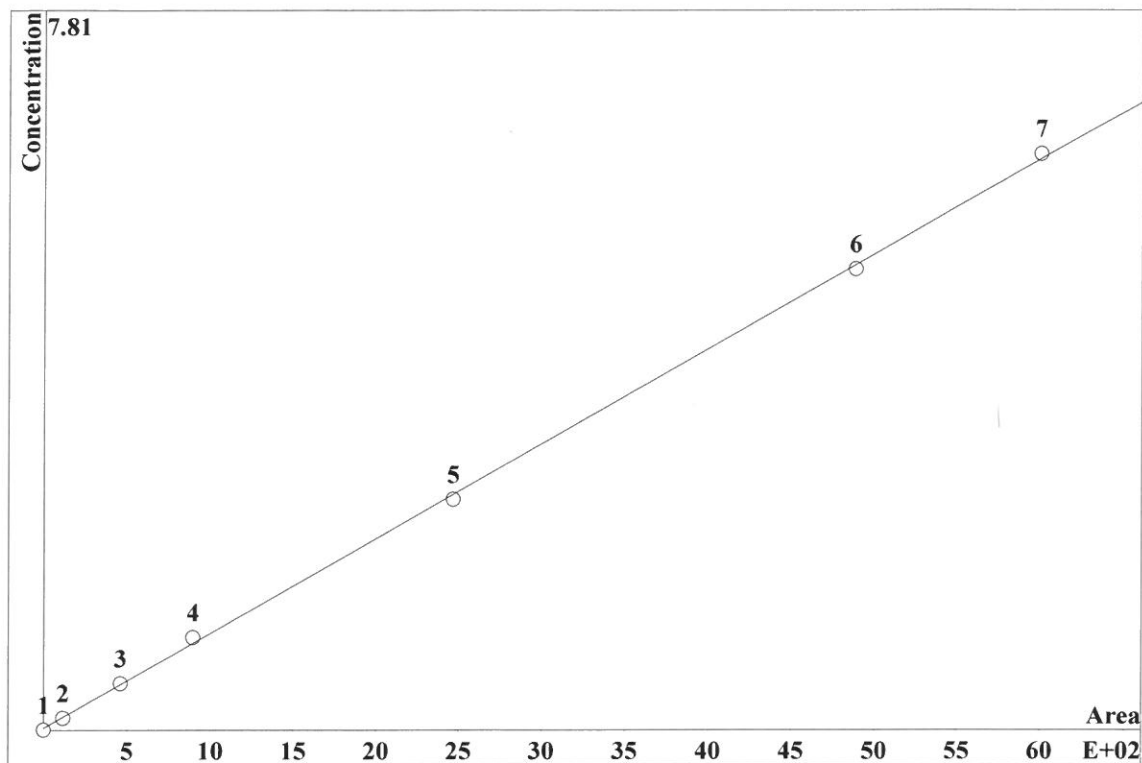


K3 = 0 K2 = 0 K1 = 0.020582 K0 = 0.358059
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.168	118.6	0.125	20	17.18		
3	16.3	462.8	0.5	20	17.18		
4	31.02	895.4	1	20	17.18		
5	83.09	2467	2.5	20	17.18		
6	158.8	4887	5	20	17.18		
7	191	6005	6.25	20	17.18		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.0540131 \cdot A - 9.81679$
 RSD: 5.375 %
 Correlation coefficient: 0.998820

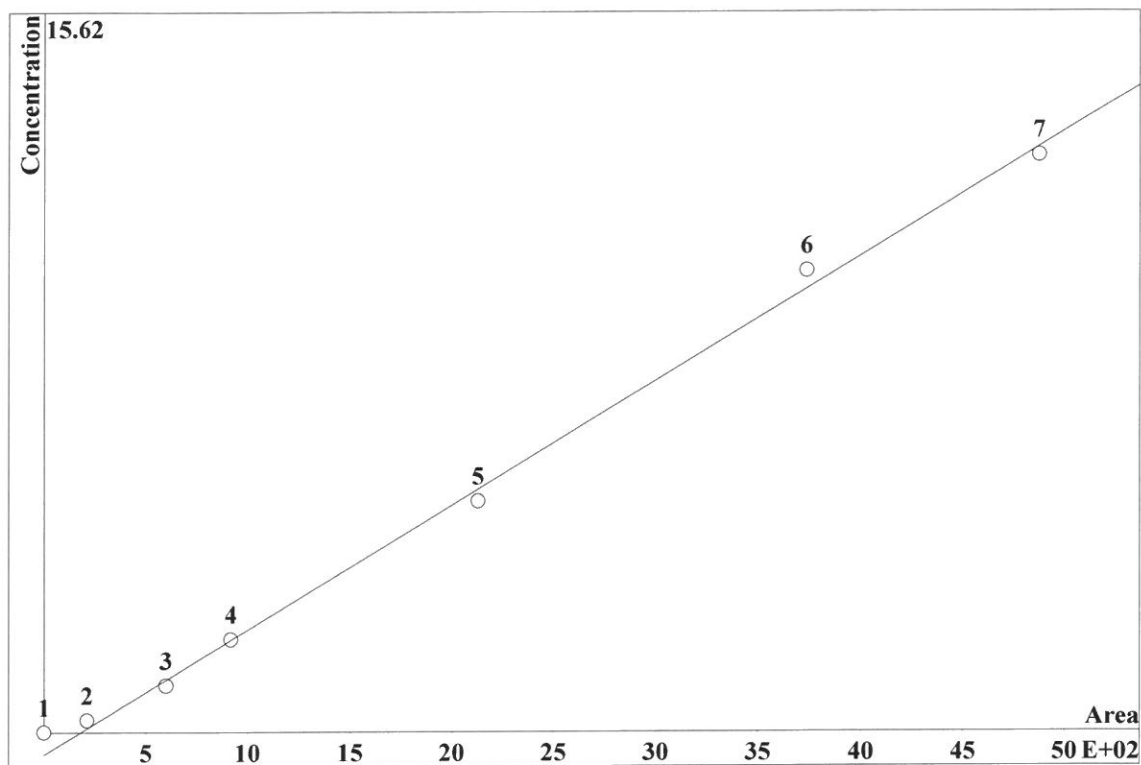


K3 = 0 K2 = 0 K1 = 0.0540131 K0 = -9.81679
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.678	211.5	0.25	20	23.13		
3	13.9	600.4	1	20	23.13		
4	21.89	919	2	20	23.13		
5	53.45	2130	5	20	23.13		
6	96.42	3738	10	20	23.13		
7	111.5	4878	12.5	20	23.13		

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.0653755 \cdot A + 3.57615$
 RSD: 1.648 %
 Correlation coefficient: 0.999889

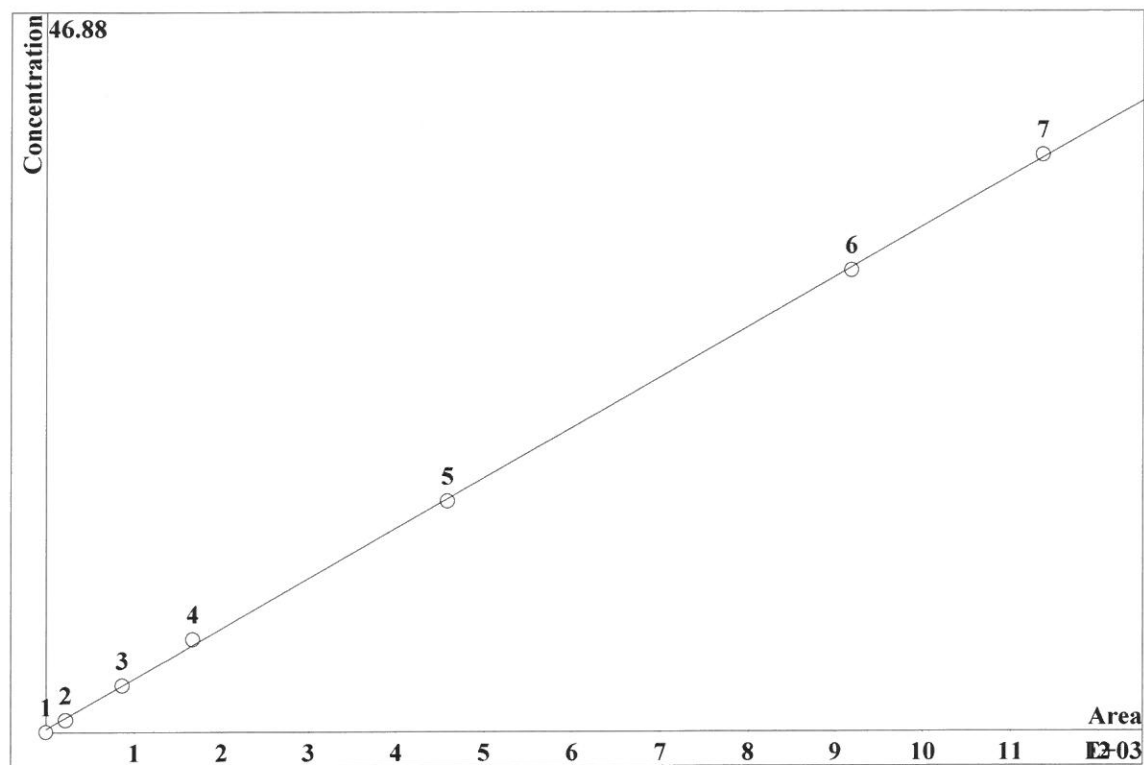

K3 = 0 K2 = 0 K1 = 0.0653755 K0 = 3.57615
 Base: Area
 Ref.channel: chl
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.231	225.4	0.75	20	25.36		
3	24.05	865.8	3	20	25.36		
4	46.34	1671	6	20	25.36		
5	127.1	4583	15	20	25.36		
6	253.6	9186	30	20	25.36		
7	310.5	1.136e+04	37.5	20	25.36		

Report date: 3/15/2018 9:22:39 AM
Printed by: wet


Ident: STD1
Analysis from: 3/12/2018 2:48:21 PM
File: _2018-03-12_

Last save: 3/12/2018 3:16:21 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16713

Last save: 3/12/2018 1:40:

SAMPLE:
:
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

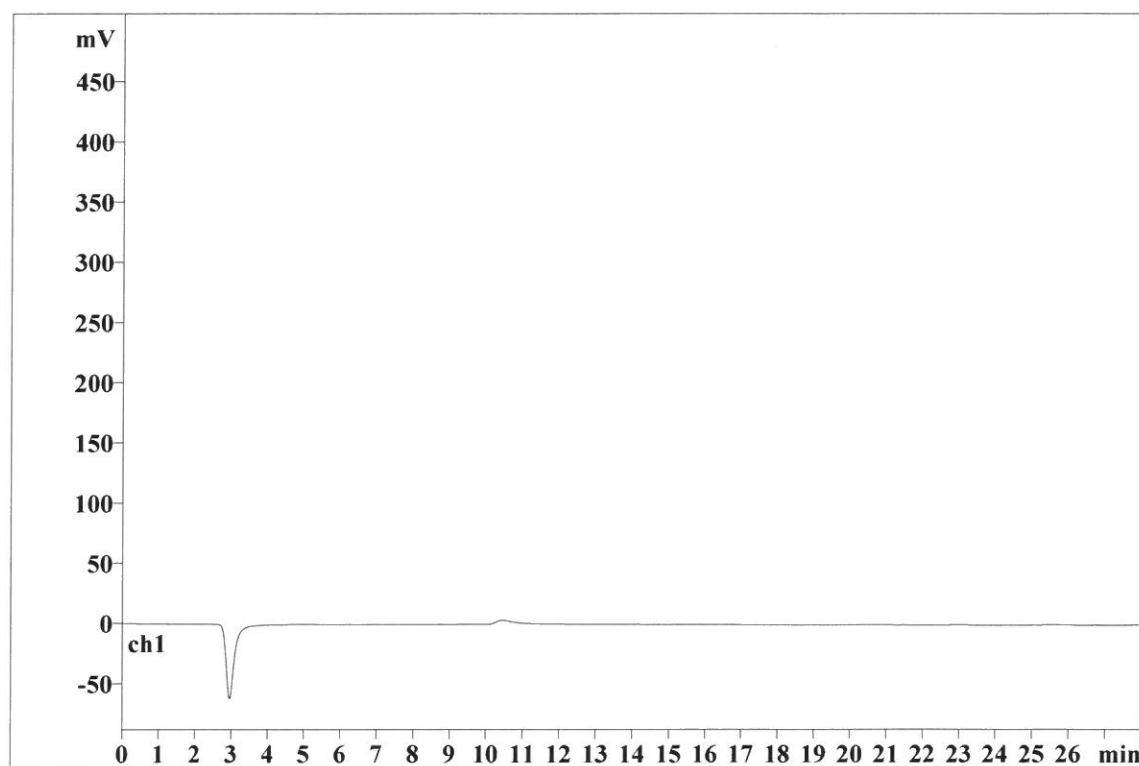

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:27:52 AM
Printed by: wet


Ident: STD2
Analysis from: 3/12/2018 3:19:16 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16714

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

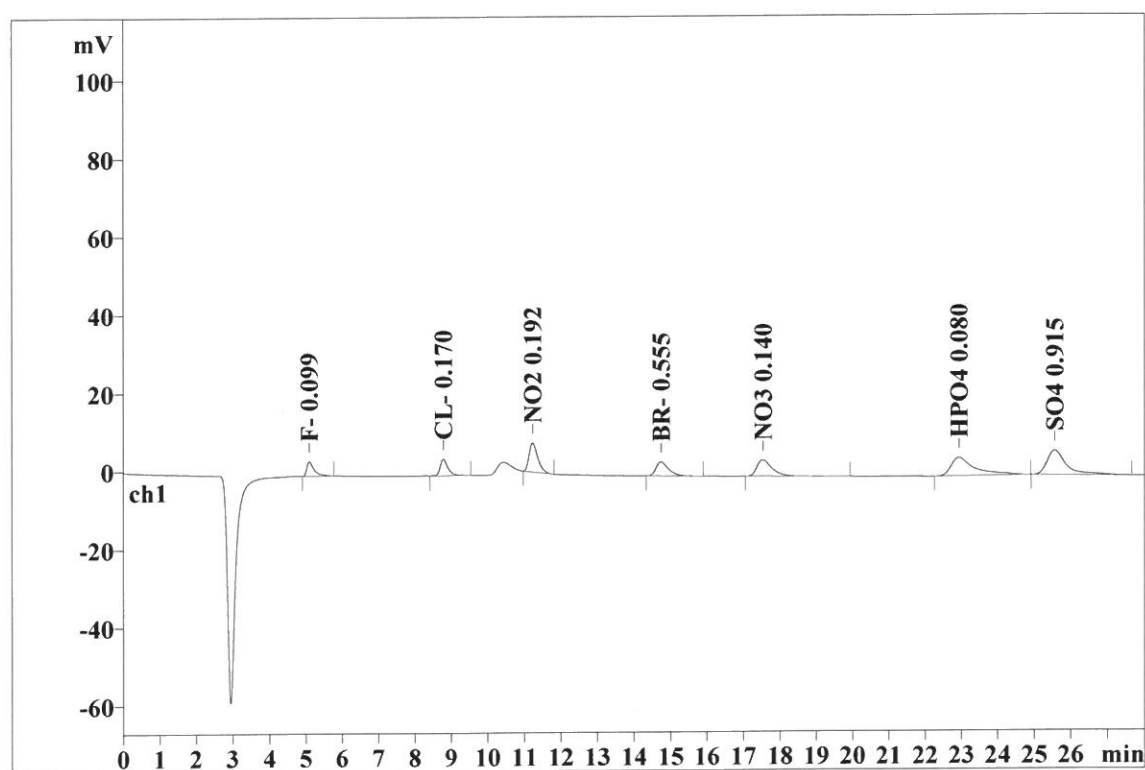

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.10	0.199	3.69	10.83	52.635	5.97
2	8.79	0.216	4.21	12.37	61.667	6.99
3	11.24	0.254	7.46	21.92	124.683	14.14
4	14.74	0.357	3.61	10.59	87.097	9.88
5	17.54	0.422	4.17	12.24	118.598	13.45
6	22.94	0.580	4.68	13.73	211.548	24.00
7	25.57	0.494	6.23	18.29	225.363	25.56
7	28.00	0.360	34.04	99.98	881.591	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:28:14 AM
Printed by: wet


Ident: STD3
Analysis from: 3/12/2018 3:50:12 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16715

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

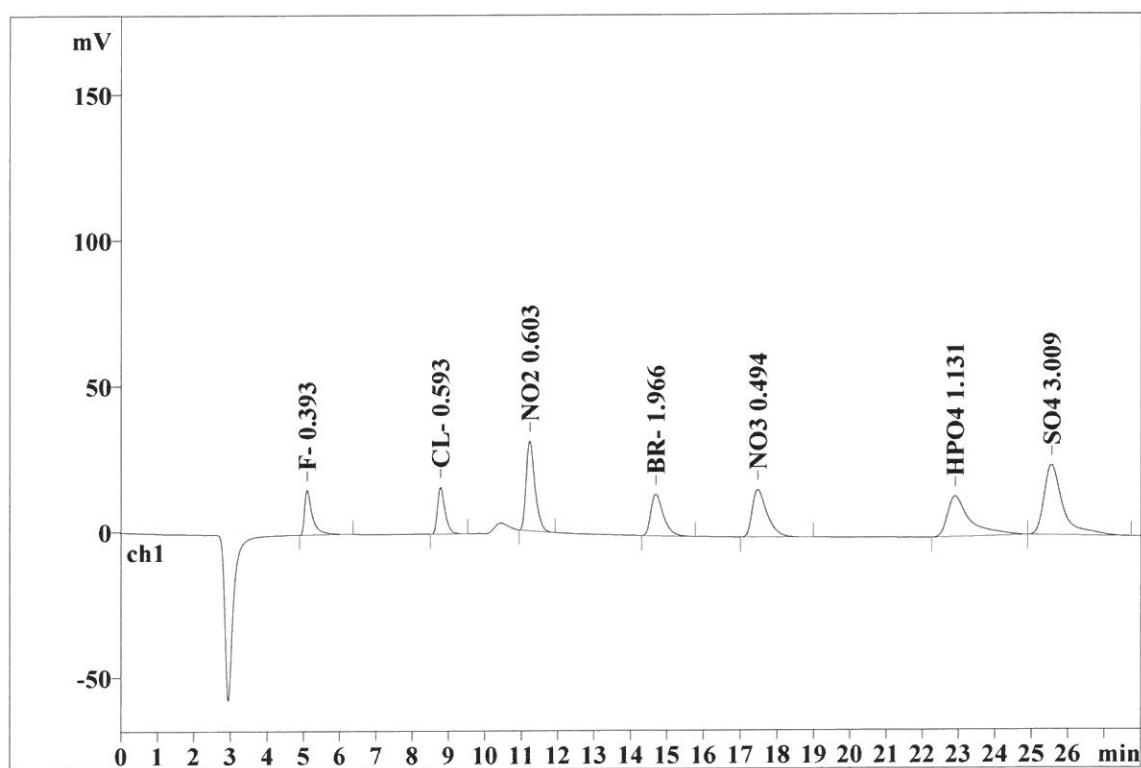

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.201	15.34	11.75	233.152	7.16
2	8.78	0.215	15.96	12.22	231.849	7.12
3	11.23	0.255	30.76	23.56	523.099	16.07
4	14.70	0.354	14.28	10.94	338.575	10.40
5	17.47	0.424	16.30	12.48	462.750	14.21
6	22.91	0.555	13.90	10.64	600.416	18.44
7	25.55	0.493	24.05	18.41	865.815	26.59
7	28.00	0.357	130.59	100.00	3255.658	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:28:24 AM
Printed by: wet


Ident: STD4
Analysis from: 3/12/2018 4:21:07 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16716

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

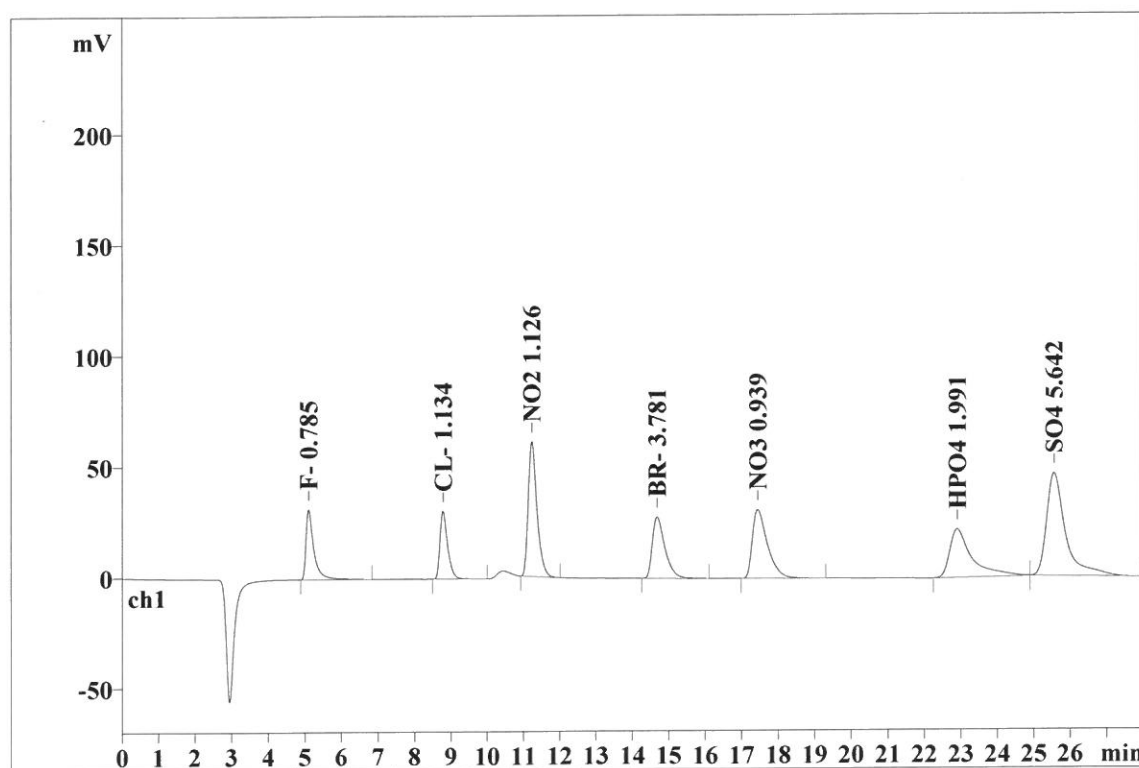

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.10	0.200	31.64	12.65	473.320	7.76
2	8.78	0.215	30.65	12.26	449.624	7.37
3	11.24	0.252	60.82	24.32	1030.197	16.89
4	14.68	0.355	27.68	11.07	662.135	10.85
5	17.44	0.430	31.02	12.41	895.396	14.68
6	22.90	0.543	21.89	8.75	919.000	15.06
7	25.56	0.493	46.34	18.53	1671.278	27.39
7	28.00	0.356	250.03	100.00	6100.950	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:28:37 AM
Printed by: wet


Ident: STD5
Analysis from: 3/12/2018 4:52:03 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16717

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

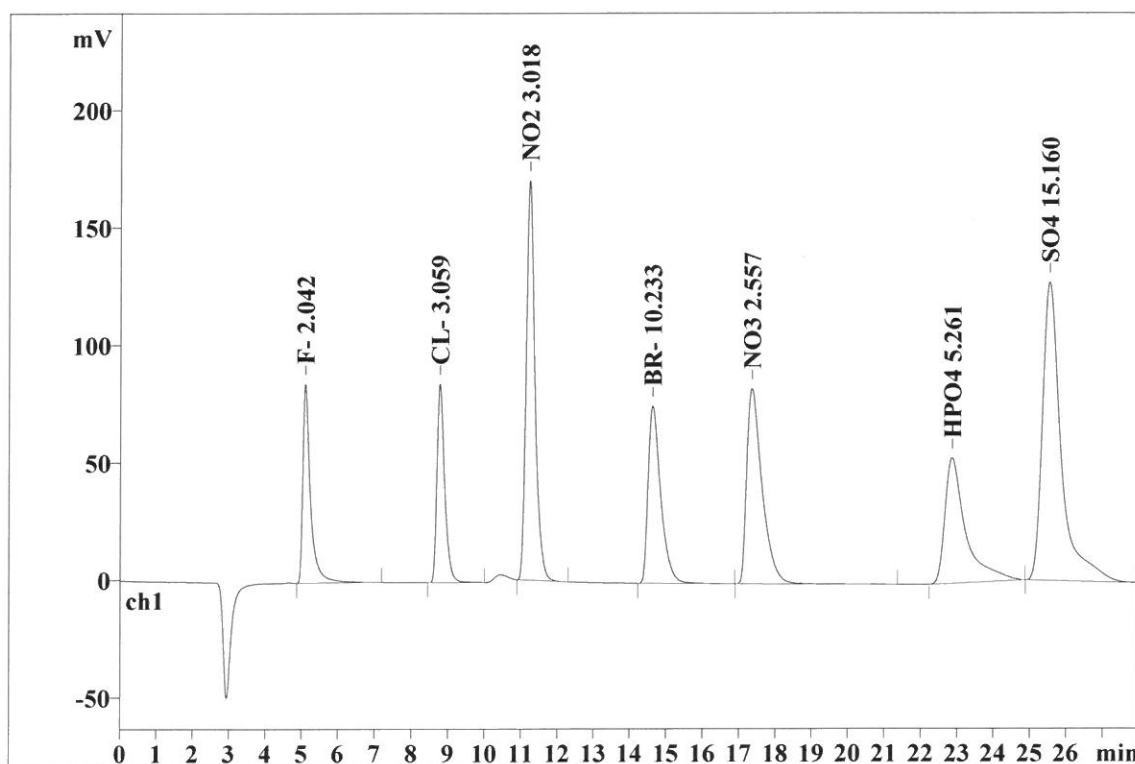

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.10	0.195	84.72	12.49	1243.953	7.62
2	8.78	0.212	84.50	12.45	1224.371	7.50
3	11.24	0.248	170.18	25.09	2864.331	17.55
4	14.63	0.356	75.38	11.11	1811.944	11.10
5	17.35	0.444	83.08	12.25	2467.367	15.11
6	22.85	0.520	53.44	7.88	2129.894	13.05
7	25.54	0.493	127.10	18.73	4583.220	28.07
7	28.00	0.353	678.41	100.00	16325.081	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:28:50 AM
Printed by: wet


Ident: STD6
Analysis from: 3/12/2018 5:22:59 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16718

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

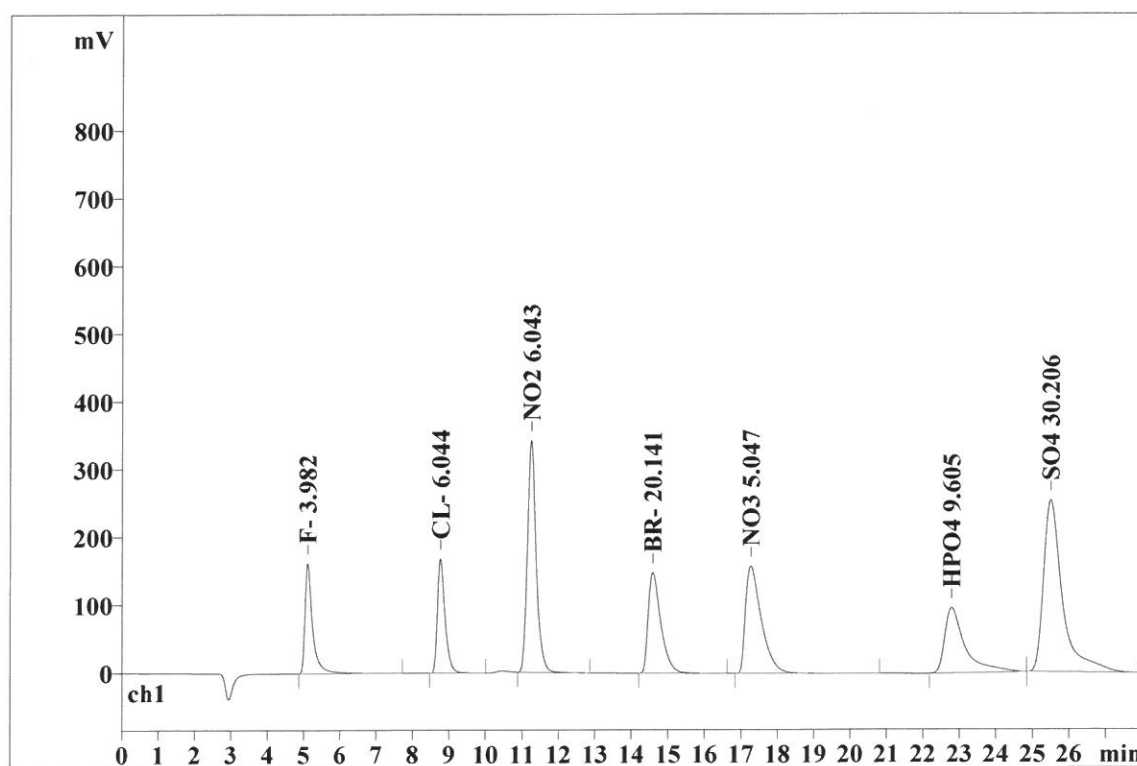

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.11	0.199	162.62	12.21	2433.439	7.59
2	8.77	0.210	169.02	12.69	2425.395	7.57
3	11.26	0.249	342.33	25.71	5797.554	18.09
4	14.58	0.358	148.60	11.16	3577.601	11.16
5	17.26	0.465	158.84	11.93	4886.878	15.25
6	22.78	0.512	96.42	7.24	3738.176	11.67
7	25.49	0.495	253.60	19.05	9185.915	28.67
7	28.00	0.356	1331.44	100.00	32044.959	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:29:03 AM
Printed by: wet


Ident: STD7
Analysis from: 3/12/2018 5:53:54 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16719

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

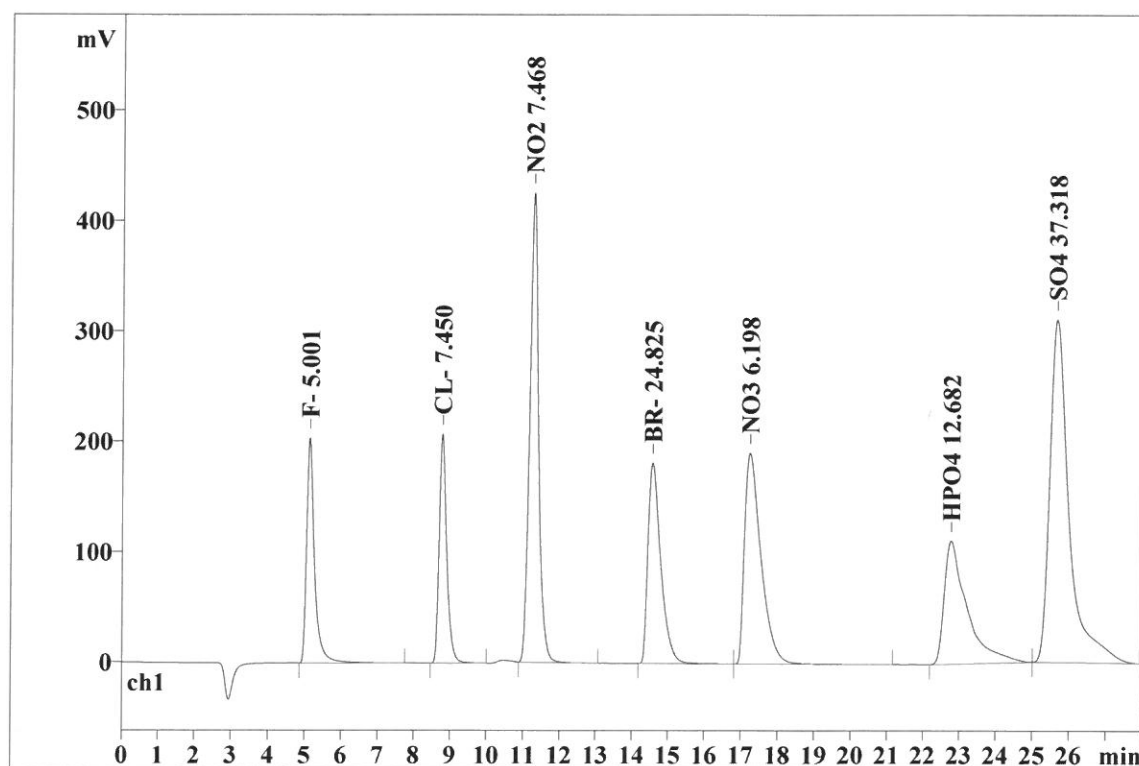

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.12	0.205	204.14	12.51	3058.124	7.67
2	8.77	0.211	207.64	12.72	2991.295	7.50
3	11.27	0.248	425.32	26.06	7179.305	18.00
4	14.57	0.361	181.84	11.14	4412.390	11.06
5	17.23	0.476	191.01	11.70	6004.853	15.06
6	22.77	0.617	111.54	6.83	4877.587	12.23
7	25.65	0.501	310.48	19.02	11361.773	28.49
7	28.00	0.374	1631.96	100.00	39885.328	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:32:31 AM
Printed by: wet


Ident: ICV
Analysis from: 3/12/2018 7:26:41 PM
File: _2018-03-12_

Last save: 3/12/2018 7:54:41 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16722

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

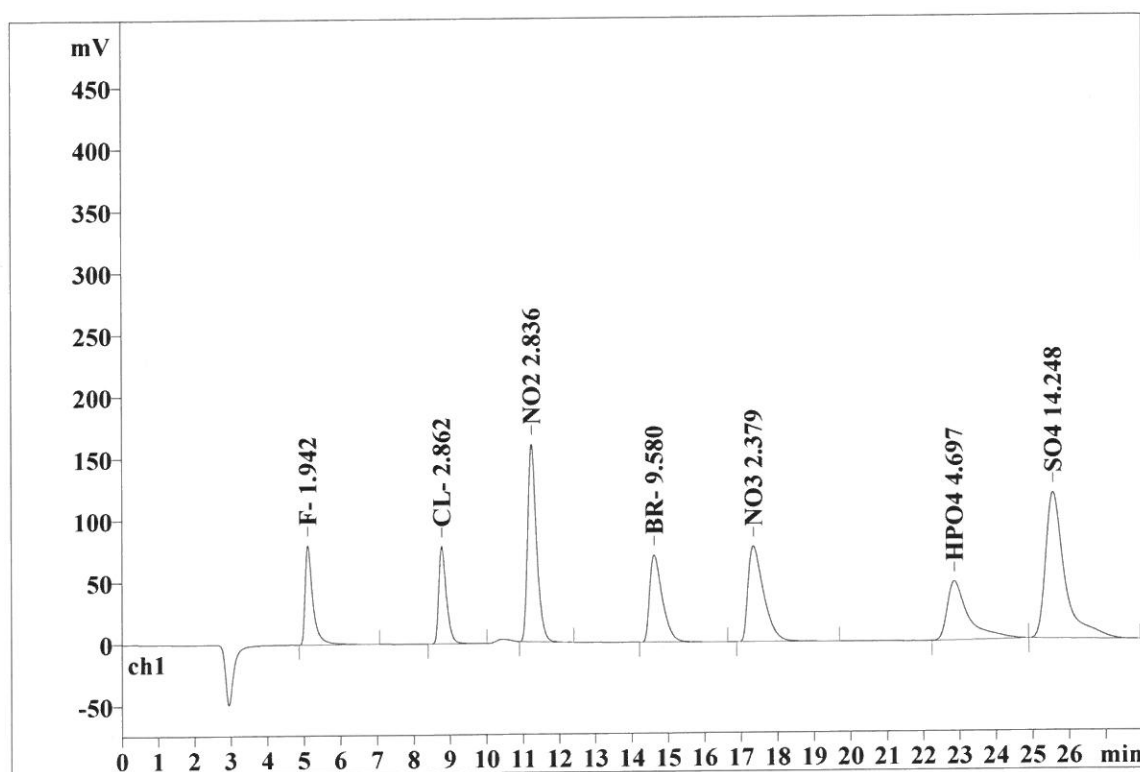

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.11	0.199	80.26	12.69	1182.971	7.77
2	8.78	0.215	78.76	12.45	1145.119	7.52
3	11.24	0.250	159.65	25.24	2688.082	17.65
4	14.62	0.360	70.56	11.16	1695.607	11.13
5	17.34	0.449	77.35	12.23	2294.187	15.06
6	22.85	0.525	47.60	7.53	1920.950	12.61
7	25.56	0.496	118.25	18.70	4304.268	28.26
7	28.00	0.356	632.44	100.00	15231.184	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:32:41 AM
Printed by: wet


Ident: ICB
Analysis from: 3/12/2018 7:57:37 PM
File: _2018-03-12_

Last save: 3/12/2018 8:25:37 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16723

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

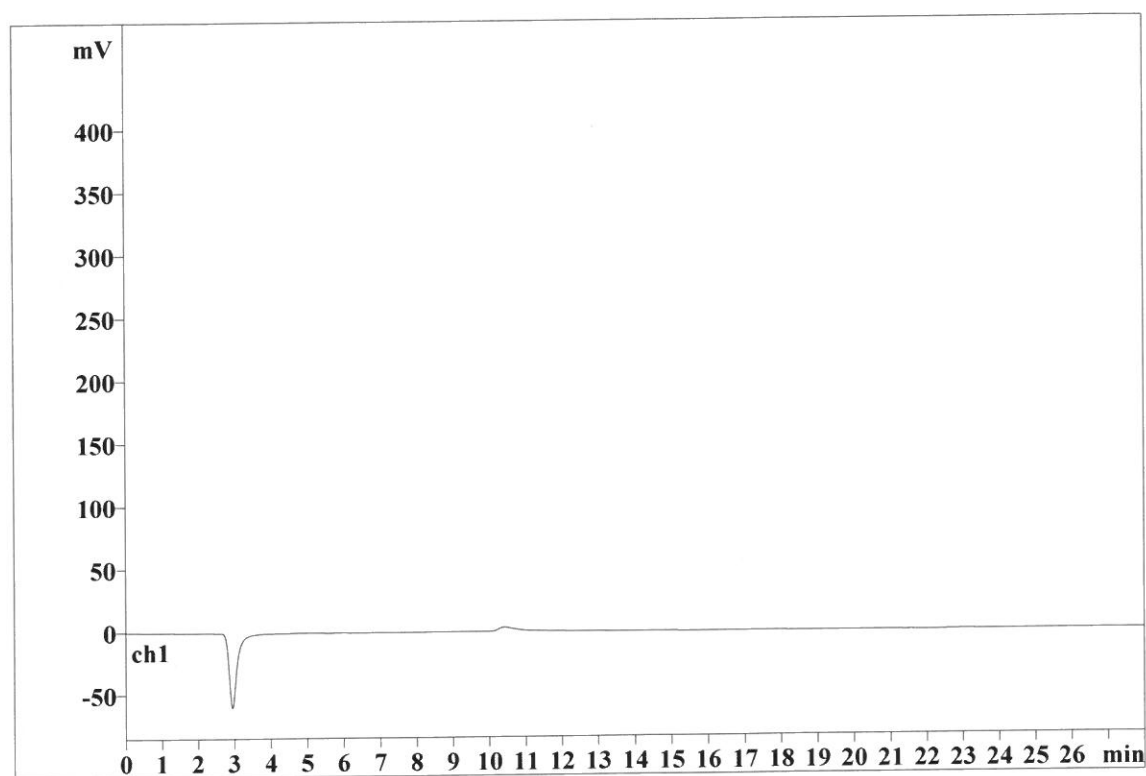

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 1:54:03 PM
Printed by: wet


Ident: CCV
Analysis from: 3/28/2018 9:38:32 AM
File: _2018-03-28_

Last save: 3/29/2018 1:52:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16921

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

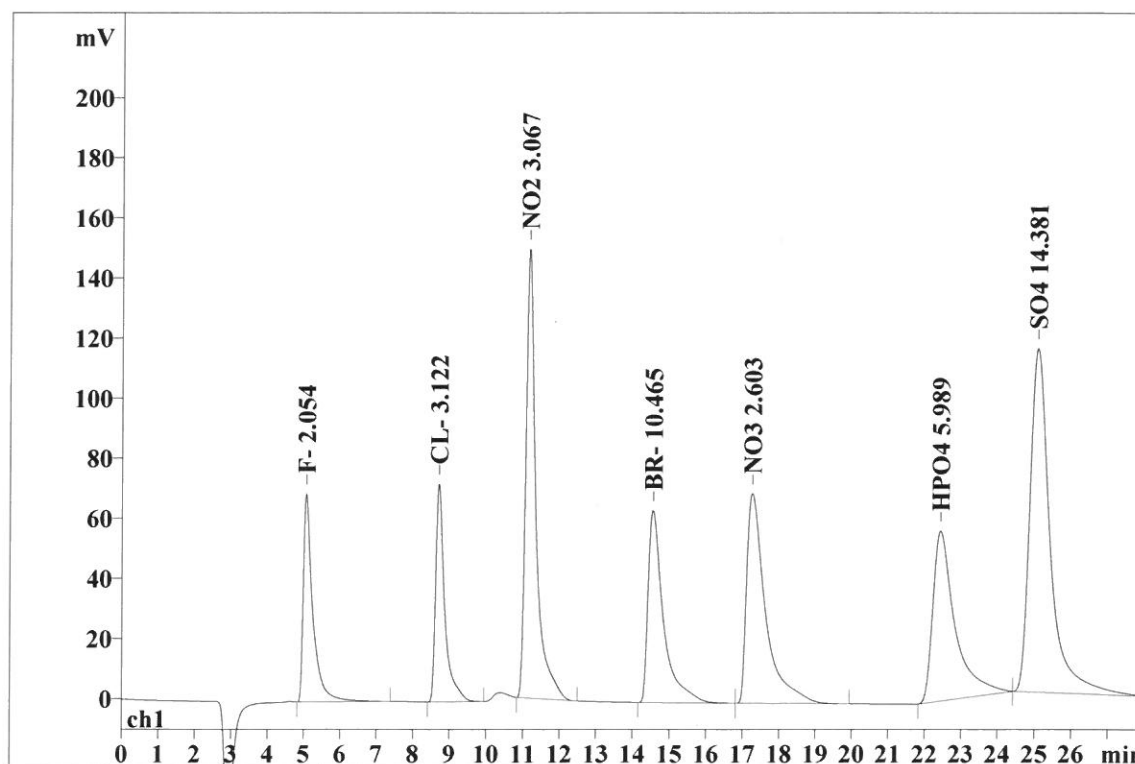

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.07	0.236	69.30	11.62	1251.525	7.57
2	8.71	0.233	72.59	12.17	1249.578	7.56
3	11.17	0.261	149.58	25.08	2912.492	17.63
4	14.55	0.389	63.95	10.72	1853.336	11.22
5	17.26	0.489	69.82	11.71	2512.373	15.20
6	22.43	0.573	56.62	9.50	2399.376	14.52
7	25.08	0.525	114.42	19.19	4344.921	26.30
7	28.00	0.387	596.28	100.00	16523.600	100.00

Report date: 3/29/2018 1:54:28 PM
Printed by: wet


Ident: CCB
Analysis from: 3/28/2018 10:09:29 AM
File: _2018-03-28_

Last save: 3/29/2018 1:52:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16922

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

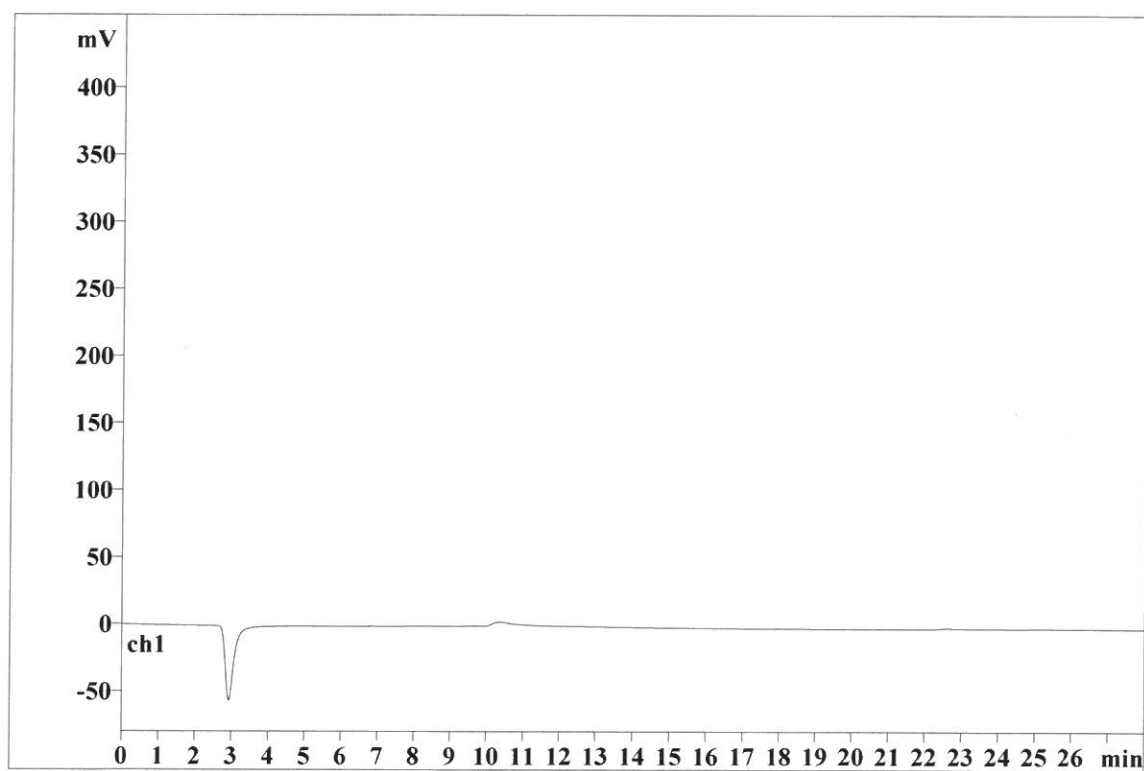

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 1:54:38 PM
Printed by: wet


Ident: LB94228BLW
Analysis from: 3/28/2018 10:40:27 AM
File: _2018-03-28_

Last save: 3/29/2018 1:52:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16923

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

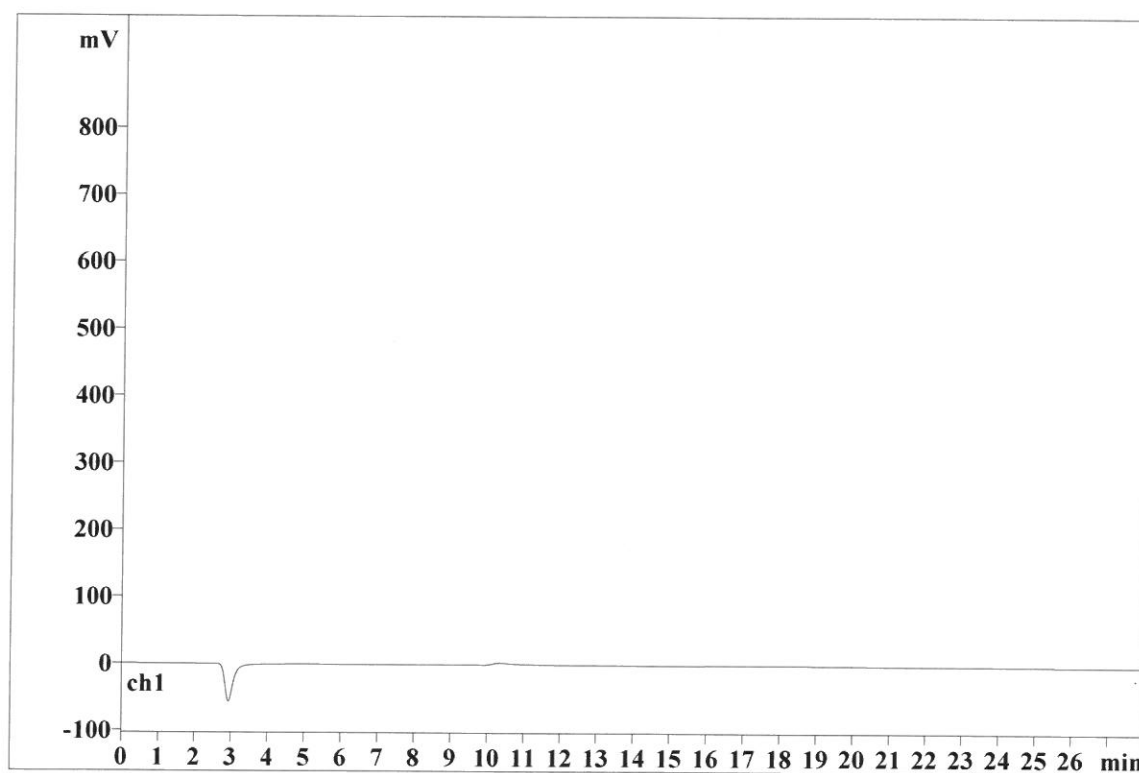

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 1:54:45 PM
Printed by: wet


Ident: LB94228BSW
Analysis from: 3/28/2018 11:11:25 AM
File: _2018-03-28_

Last save: 3/29/2018 1:52:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16924

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

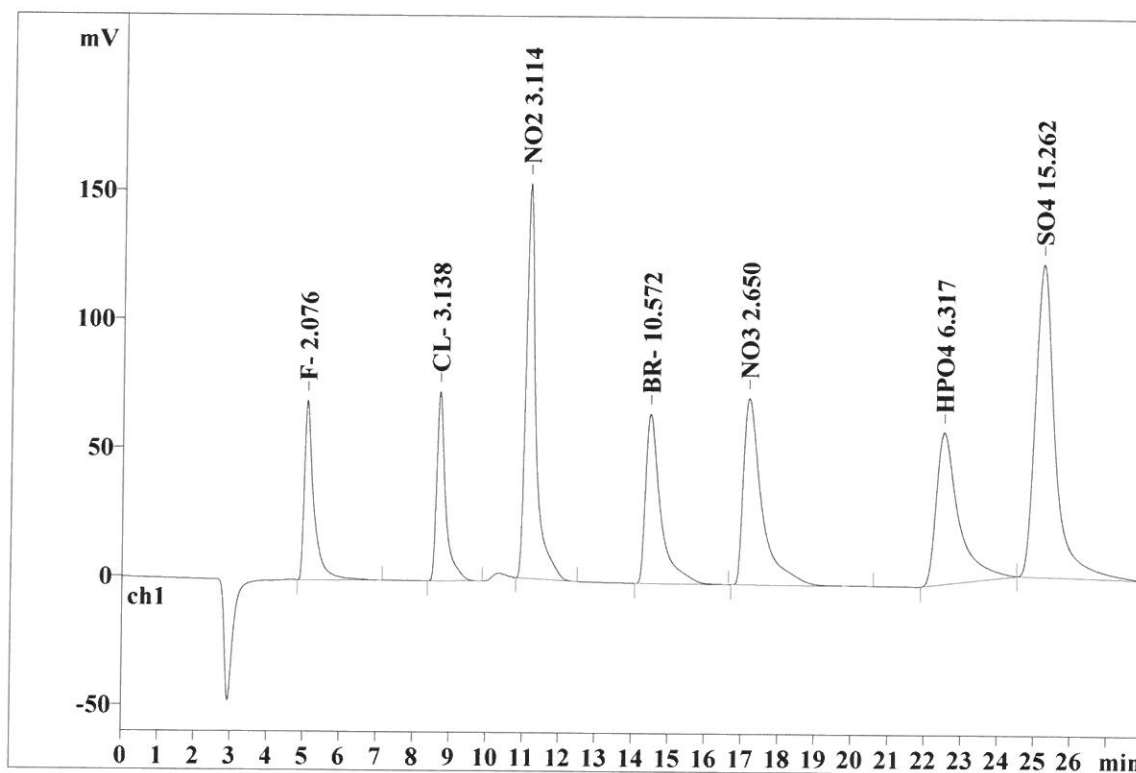

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.07	0.238	69.75	11.32	1264.949	7.42
2	8.69	0.231	73.62	11.95	1255.865	7.37
3	11.13	0.258	153.55	24.93	2958.083	17.36
4	14.47	0.381	65.90	10.70	1872.312	10.99
5	17.15	0.478	72.45	11.76	2557.717	15.01
6	22.49	0.576	59.01	9.58	2520.829	14.79
7	25.18	0.526	121.59	19.74	4614.339	27.07
7	28.00	0.384	615.88	100.00	17044.093	100.00

Report date: 3/29/2018 1:54:56 PM
Printed by: wet


Ident: J2116-01
Analysis from: 3/28/2018 1:37:45 PM
File: _2018-03-28_

Last save: 3/29/2018 1:52:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16926

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

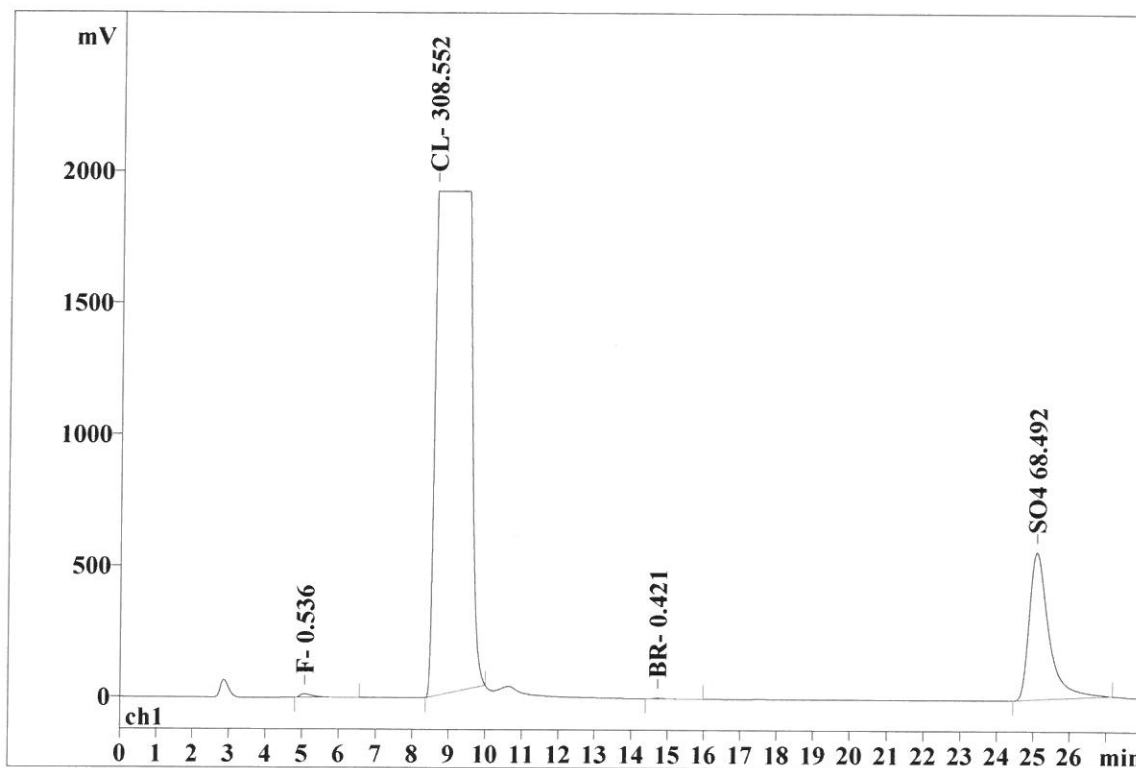

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.07	0.354	12.85	0.52	320.981	0.22
2	8.62	1.056	1925.41	77.20	124155.211	85.37
3	0.00	0.000	0.00	0.00	0.000	0.00
4	14.73	0.362	2.46	0.10	63.222	0.04
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.08	0.526	559.82	22.45	20898.725	14.37
7	28.00	0.328	2500.55	100.26	145438.139	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 1:55:05 PM
Printed by: wet


Ident: J2116-04
Analysis from: 3/28/2018 2:08:43 PM
File: _2018-03-28_

Last save: 3/29/2018 1:52:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16927

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

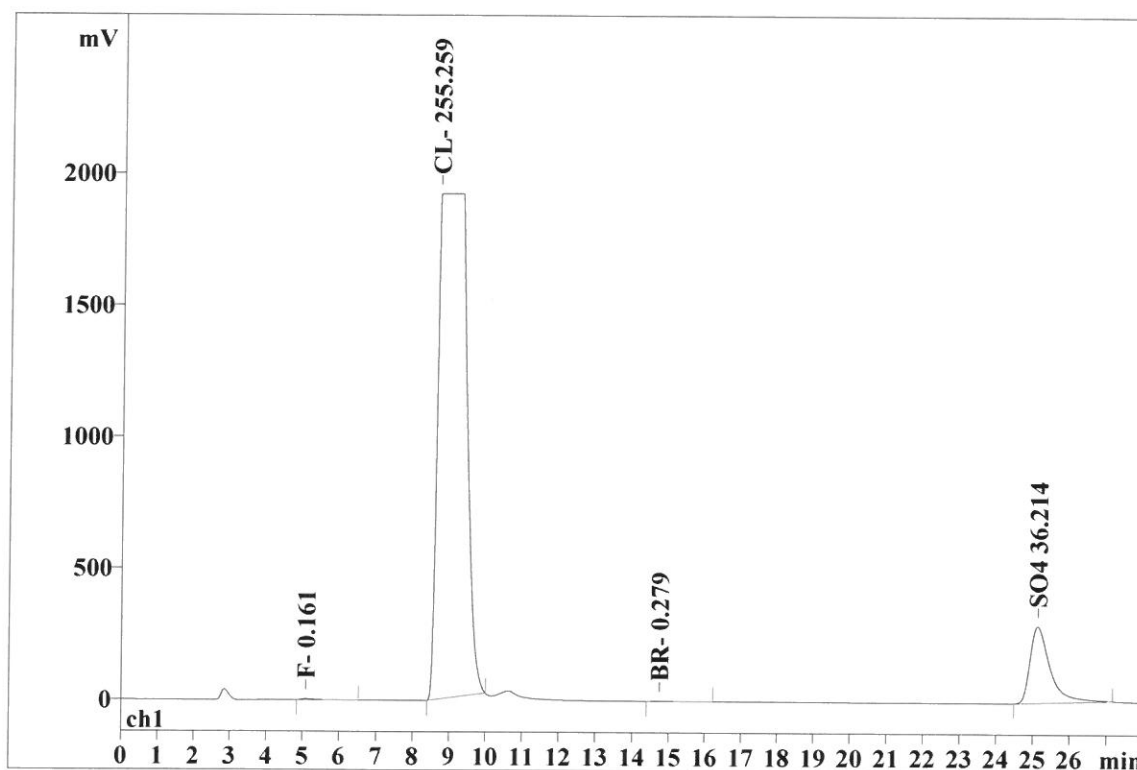

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.354	3.61	0.16	91.041	0.08
2	8.69	0.856	1925.26	86.88	102710.064	90.20
3	0.00	0.000	0.00	0.00	0.000	0.00
4	14.75	0.366	1.37	0.06	38.004	0.03
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.12	0.535	290.44	13.11	11024.036	9.68
7	28.00	0.302	2220.68	100.21	113863.145	100.00

Report date: 3/29/2018 1:55:17 PM
Printed by: wet


Ident: J2116-06
Analysis from: 3/28/2018 2:39:41 PM
File: _2018-03-28_

Last save: 3/29/2018 1:52:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16928

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

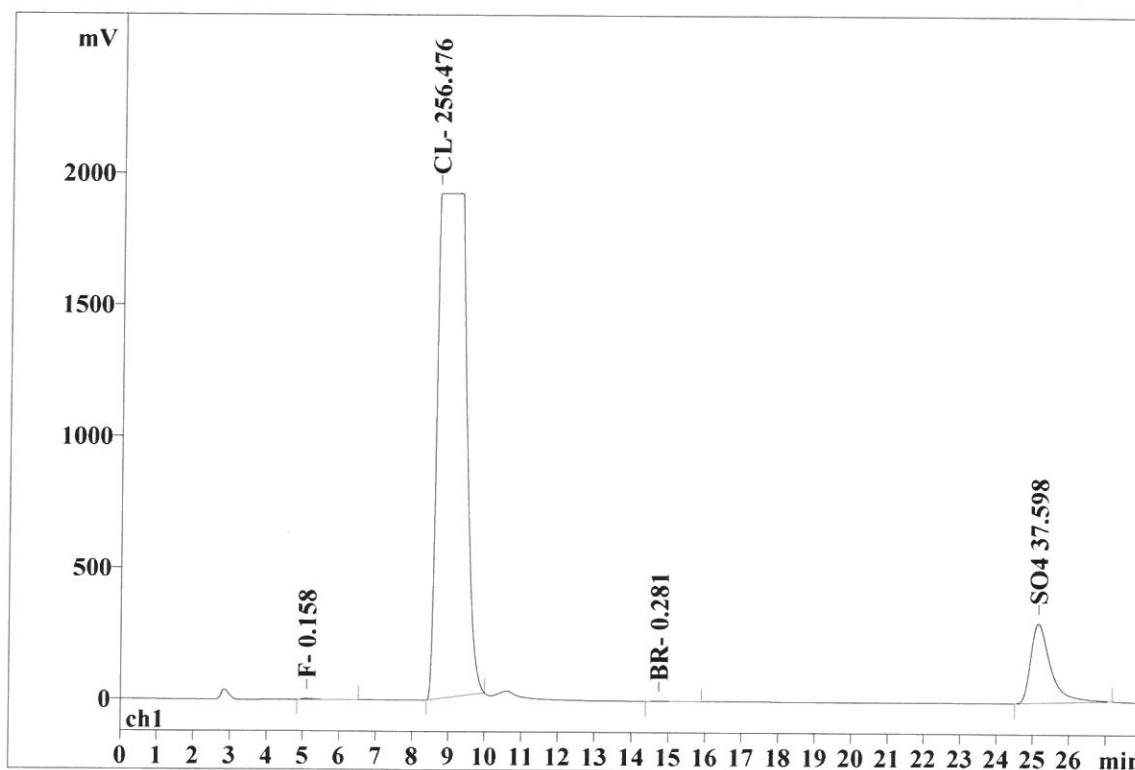

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.10	0.363	3.44	0.15	89.226	0.08
2	8.69	0.860	1924.34	86.41	103199.905	89.92
3	0.00	0.000	0.00	0.00	0.000	0.00
4	14.75	0.366	1.43	0.06	38.383	0.03
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.14	0.537	301.35	13.53	11447.424	9.97
7	28.00	0.304	2230.57	100.16	114774.939	100.00

Report date: 3/29/2018 1:55:26 PM
Printed by: wet


Ident: J2116-05
Analysis from: 3/28/2018 3:10:39 PM
File: _2018-03-28_

Last save: 3/29/2018 1:52:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16929

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

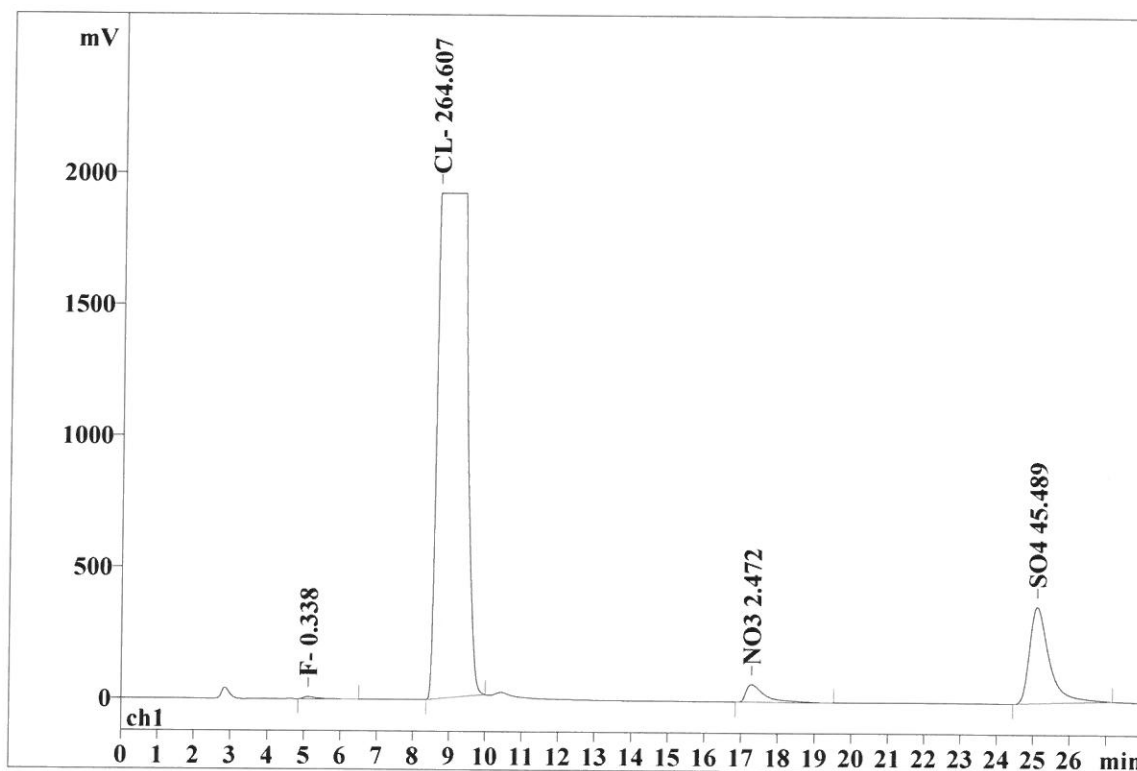

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.11	0.324	8.52	0.36	199.343	0.16
2	8.66	0.884	1928.44	81.52	106471.544	86.62
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.28	0.479	66.83	2.83	2384.570	1.94
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.10	0.534	367.01	15.51	13861.651	11.28
7	28.00	0.317	2370.79	100.22	122917.107	100.00

Report date: 3/29/2018 1:55:34 PM
Printed by: wet


Ident: J2116-07
Analysis from: 3/28/2018 3:41:41 PM
File: _2018-03-28_

Last save: 3/29/2018 1:52:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16930

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

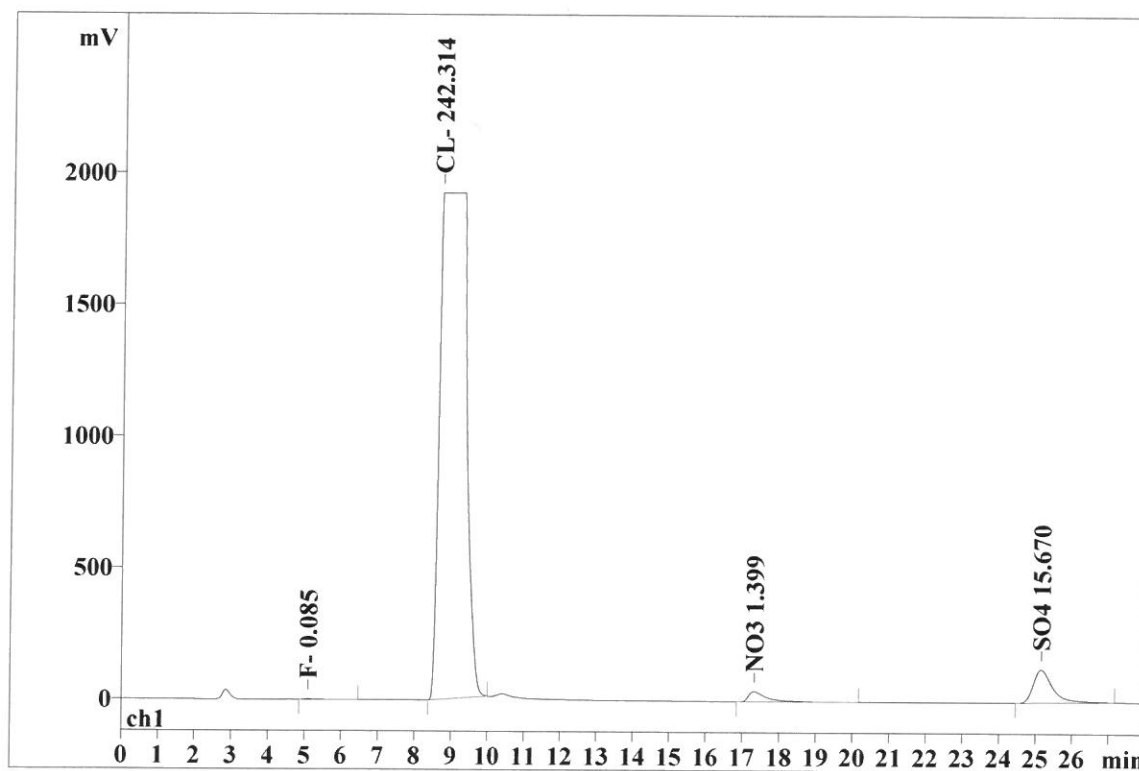

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.338	1.78	0.09	44.284	0.04
2	8.70	0.794	1926.99	92.22	97500.878	94.09
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.32	0.472	37.98	1.82	1342.329	1.30
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.15	0.533	125.68	6.01	4739.115	4.57
7	28.00	0.305	2092.44	100.14	103626.606	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 1:55:51 PM
Printed by: wet


Ident: J2116-01DUP
Analysis from: 3/28/2018 4:12:49 PM
File: _2018-03-28_

Last save: 3/29/2018 1:52:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16931

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

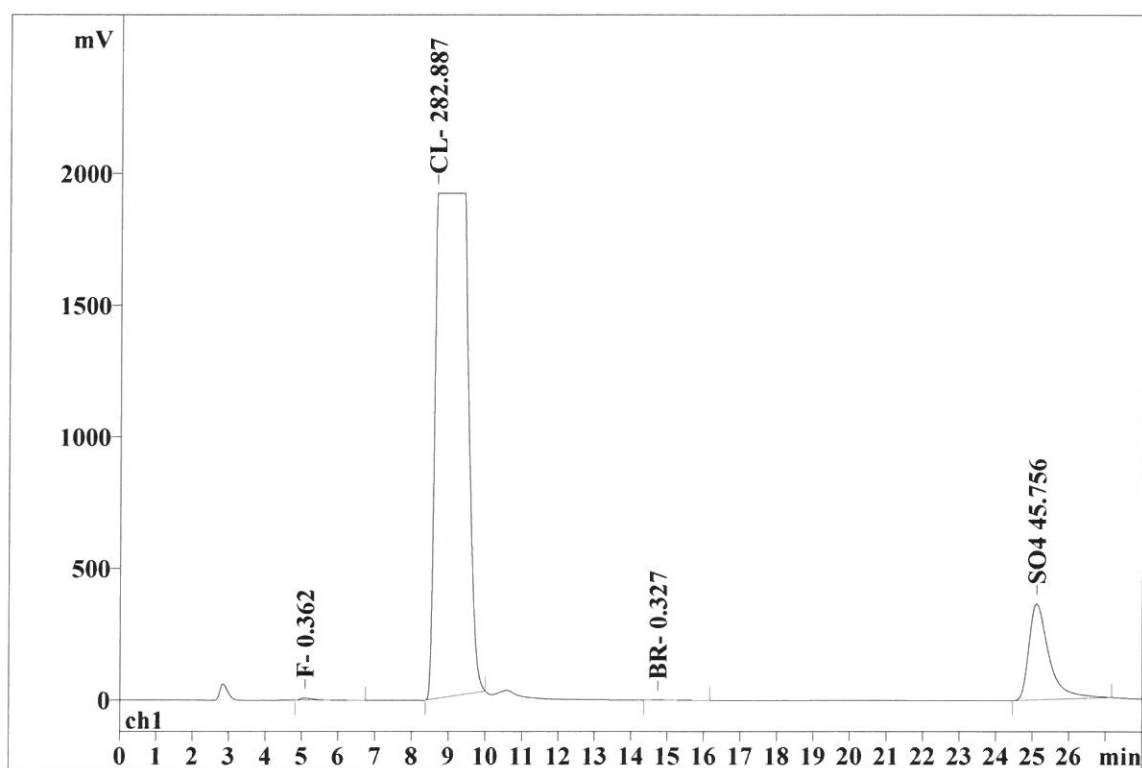

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.362	8.23	0.36	214.324	0.17
2	8.67	0.960	1924.59	83.85	113827.451	88.91
3	0.00	0.000	0.00	0.00	0.000	0.00
4	14.74	0.366	1.73	0.08	46.614	0.04
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.11	0.540	365.34	15.92	13943.119	10.89
7	28.00	0.318	2299.88	100.20	128031.508	100.00

Report date: 3/29/2018 1:57:45 PM
Printed by: wet


Ident: J2116-02MS
Analysis from: 3/28/2018 4:43:51 PM
File: _2018-03-28_

Last save: 3/29/2018 1:57:43 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16932

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 12
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

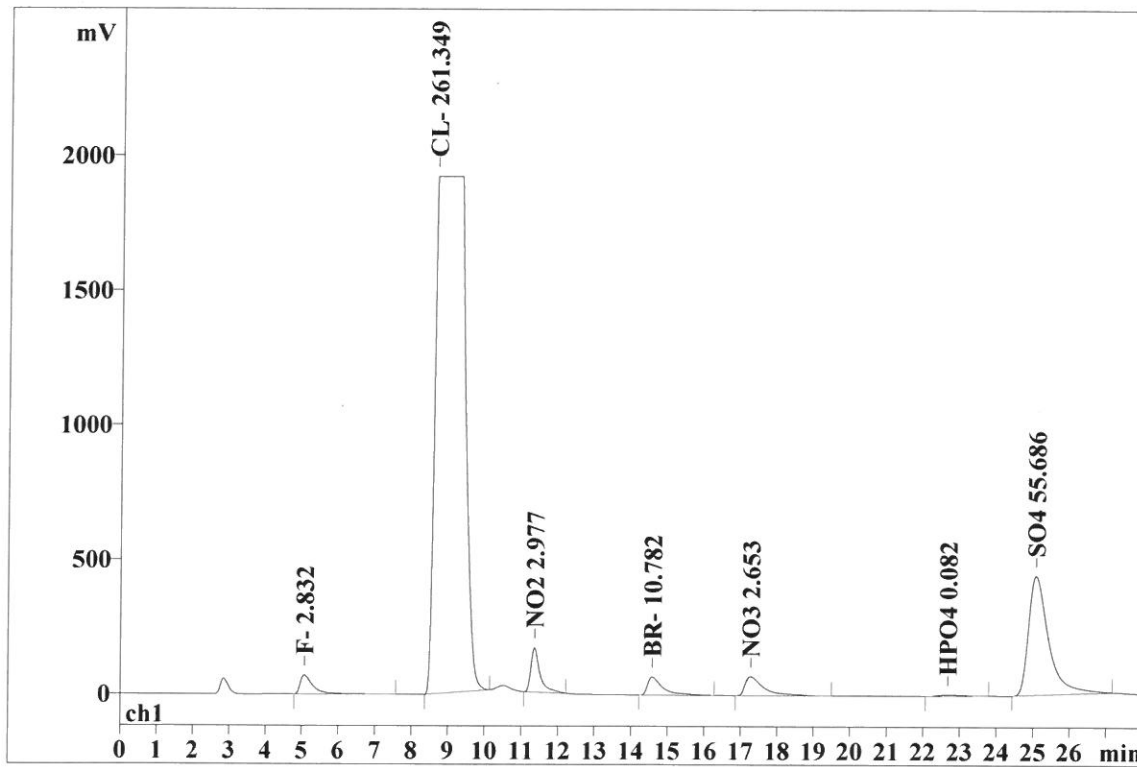

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.08	0.336	70.85	2.58	1728.252	1.32
2	8.67	0.875	1927.18	70.26	105160.473	80.04
3	11.36	0.230	164.90	6.01	2824.873	2.15
4	14.59	0.380	66.89	2.44	1909.853	1.45
5	17.27	0.487	70.52	2.57	2560.825	1.95
6	22.66	0.729	4.54	0.17	212.180	0.16
7	25.07	0.544	442.57	16.14	16981.032	12.93
7	28.00	0.512	2747.45	100.17	131377.488	100.00

Report date: 3/29/2018 1:58:21 PM
Printed by: wet


Ident: J2116-03MSD
Analysis from: 3/28/2018 5:14:49 PM
File: _2018-03-28_

Last save: 3/29/2018 1:58:20 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16933

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 13
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

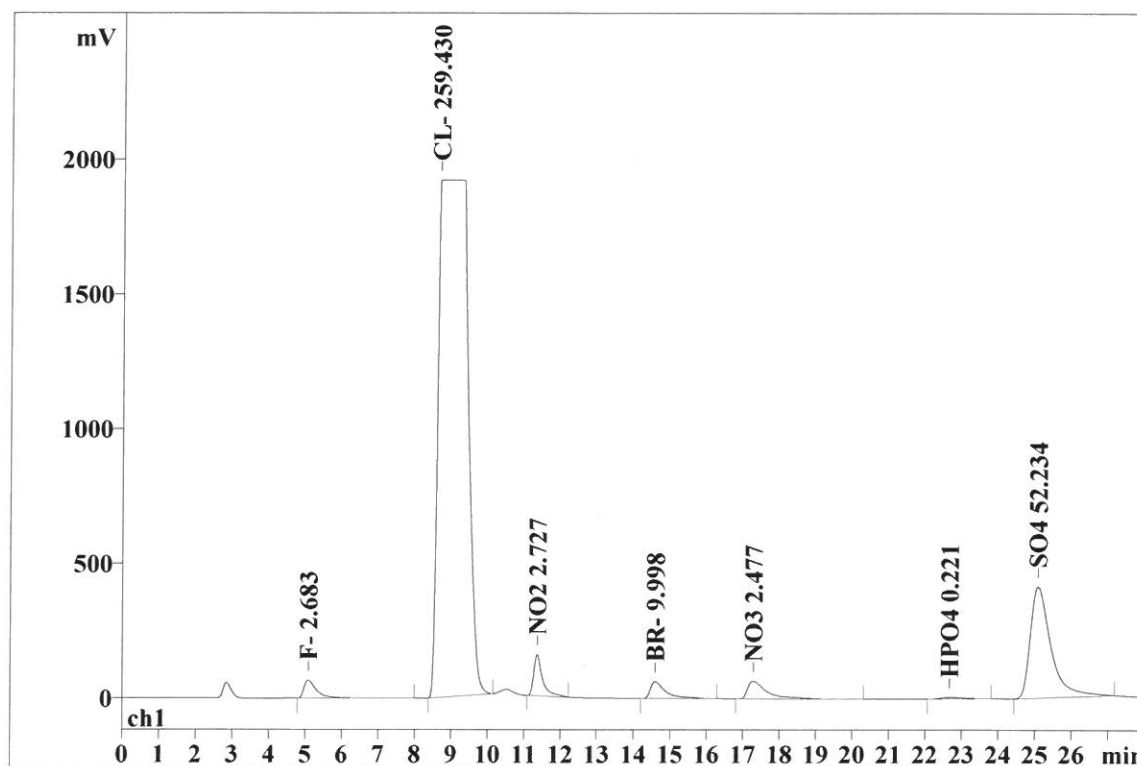

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.08	0.339	67.26	2.50	1637.321	1.27
2	8.68	0.868	1924.00	71.61	104388.298	80.95
3	11.37	0.227	153.25	5.70	2582.783	2.00
4	14.60	0.379	61.85	2.30	1769.993	1.37
5	17.28	0.487	65.02	2.42	2389.748	1.85
6	22.66	0.723	5.63	0.21	263.751	0.20
7	25.08	0.548	412.64	15.36	15924.896	12.35
7	28.00	0.510	2689.64	100.11	128956.788	100.00

Report date: 3/29/2018 1:58:55 PM
Printed by: wet


Ident: CCV
Analysis from: 3/28/2018 5:45:53 PM
File: _2018-03-28_

Last save: 3/29/2018 1:53:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16934

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

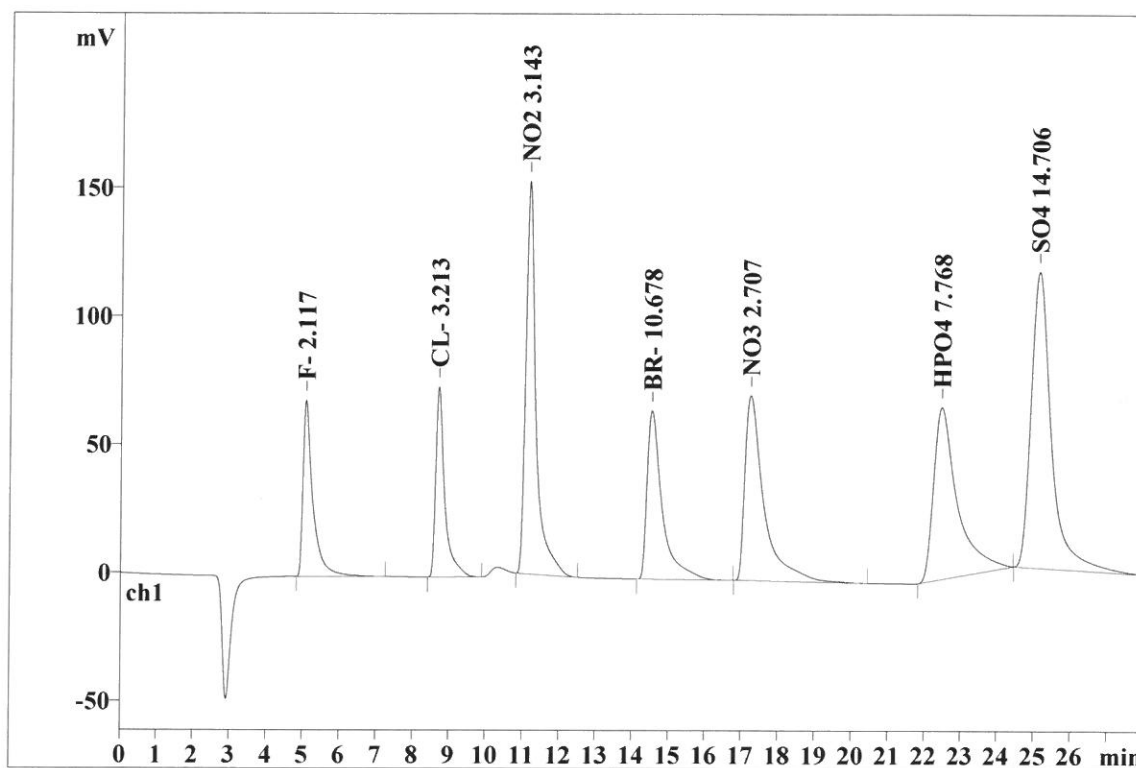

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.08	0.244	68.77	11.15	1290.086	7.34
2	8.71	0.234	74.15	12.03	1286.057	7.32
3	11.17	0.260	153.24	24.85	2986.214	17.00
4	14.53	0.384	65.70	10.66	1891.313	10.76
5	17.23	0.481	72.10	11.69	2613.328	14.87
6	22.45	0.615	67.06	10.88	3058.245	17.41
7	25.13	0.537	115.53	18.74	4444.265	25.30
7	28.00	0.394	616.55	100.00	17569.508	100.00

Report date: 3/29/2018 1:59:21 PM
Printed by: wet


Ident: CCB
Analysis from: 3/28/2018 6:16:51 PM
File: _2018-03-28_

Last save: 3/29/2018 1:59:18 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16935

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

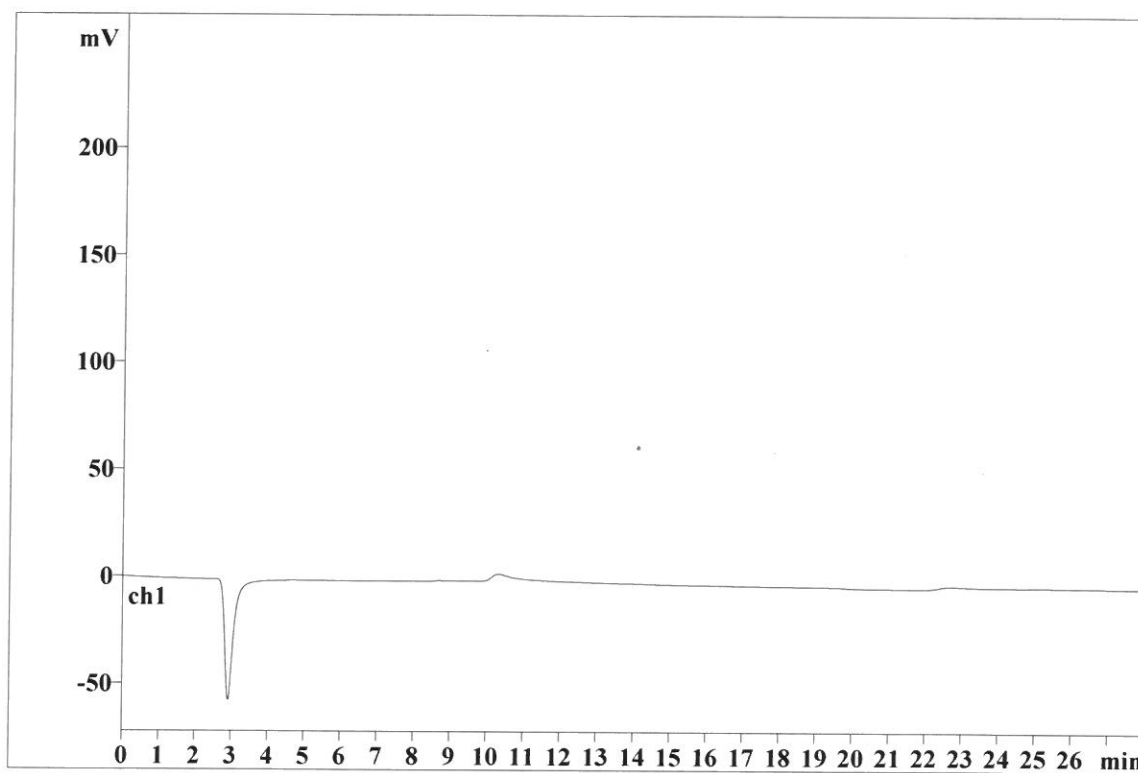

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 2:01:39 PM
Printed by: wet


Ident: J2116-01DLX5
Analysis from: 3/28/2018 6:47:53 PM
File: _2018-03-28_

Last save: 3/29/2018 2:01:39 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16936

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 14
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

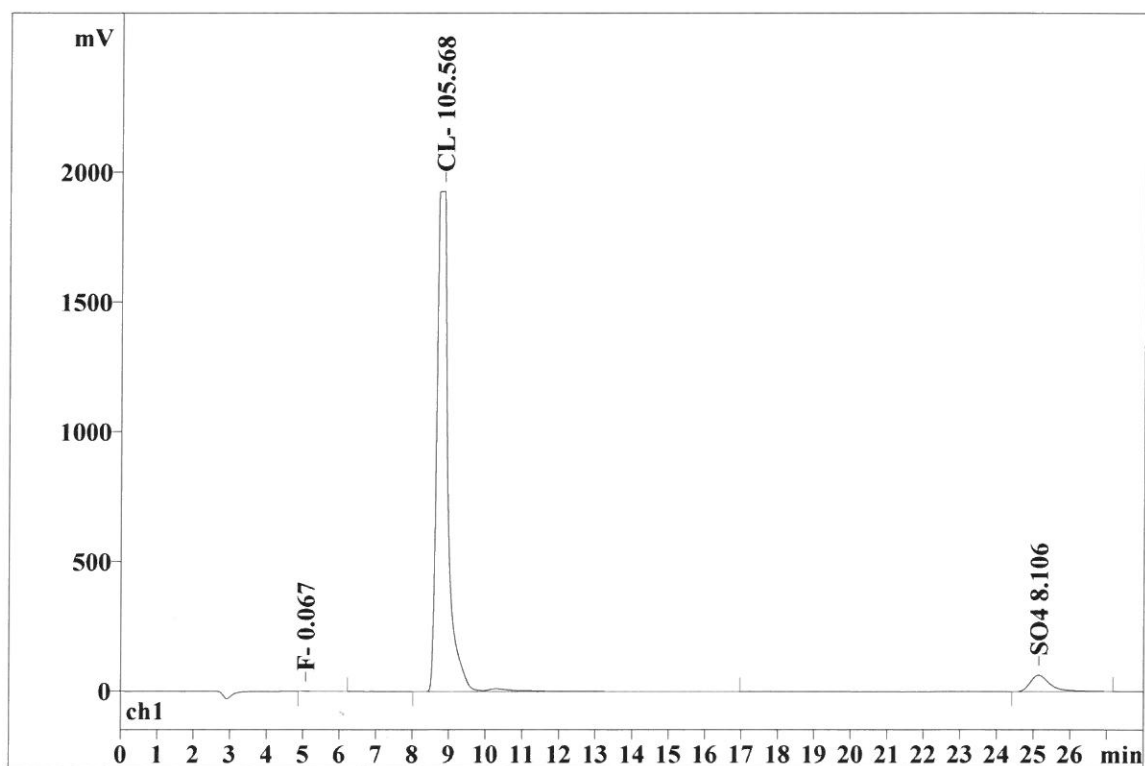

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.07	0.275	1.68	0.08	33.184	0.07
2	8.84	0.298	1934.11	97.04	42474.033	94.53
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.14	0.540	63.66	3.19	2425.055	5.40
7	28.00	0.159	1999.45	100.32	44932.272	100.00

Report date: 3/29/2018 2:02:32 PM
Printed by: wet


Ident: J2116-01DL2X100
Analysis from: 3/28/2018 7:18:51 PM
File: _2018-03-28_

Last save: 3/29/2018 1:53:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16937

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 15
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

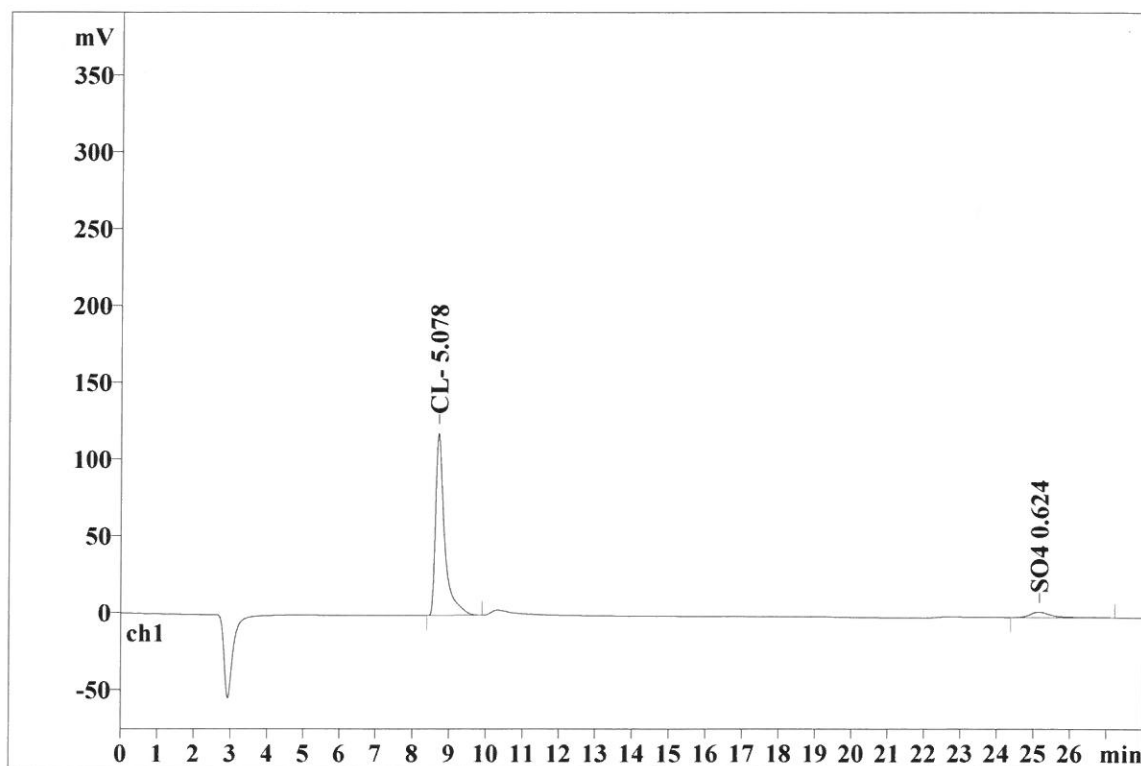

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.71	0.231	118.53	97.12	2036.525	93.73
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.15	0.546	3.51	2.88	136.200	6.27
7	28.00	0.111	122.04	99.99	2172.724	100.00

Report date: 3/29/2018 2:04:08 PM
Printed by: wet


Ident: J2116-04DLX50
Analysis from: 3/28/2018 7:49:49 PM
File: _2018-03-28_

Last save: 3/29/2018 1:53:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16938

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 16
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

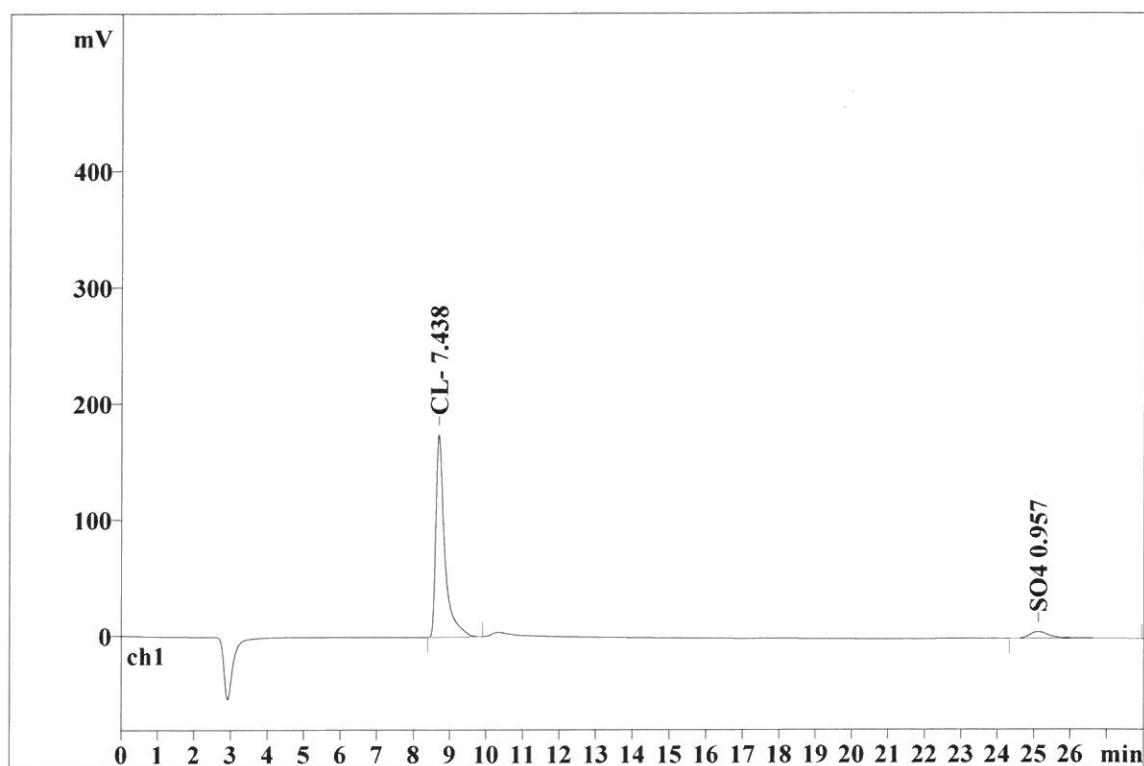

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.70	0.230	174.51	96.70	2986.564	92.62
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.12	0.547	5.94	3.29	238.110	7.38
7	28.00	0.111	180.45	100.00	3224.674	100.00

Report date: 3/29/2018 2:05:01 PM
Printed by: wet


Ident: J2116-06DLX2
Analysis from: 3/28/2018 8:20:48 PM
File: _2018-03-28_

Last save: 3/29/2018 2:04:43 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16939

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 17
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

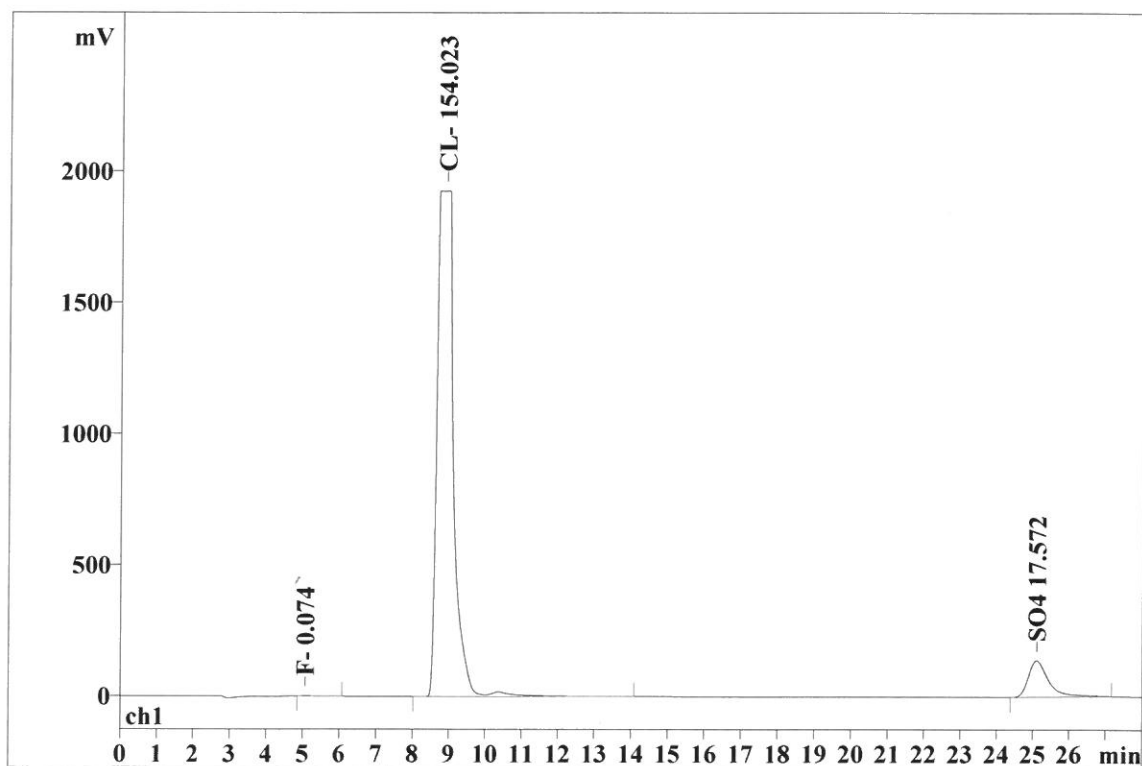

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.07	0.298	1.80	0.09	37.607	0.06
2	8.91	0.457	1926.32	93.21	61972.354	92.04
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.11	0.544	138.37	6.69	5321.035	7.90
7	28.00	0.186	2066.48	99.99	67330.996	100.00

Report date: 3/29/2018 2:05:53 PM
Printed by: wet


Ident: J2116-06DL2X50
Analysis from: 3/28/2018 8:51:45 PM
File: _2018-03-28_

Last save: 3/29/2018 1:53:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16940

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 18
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

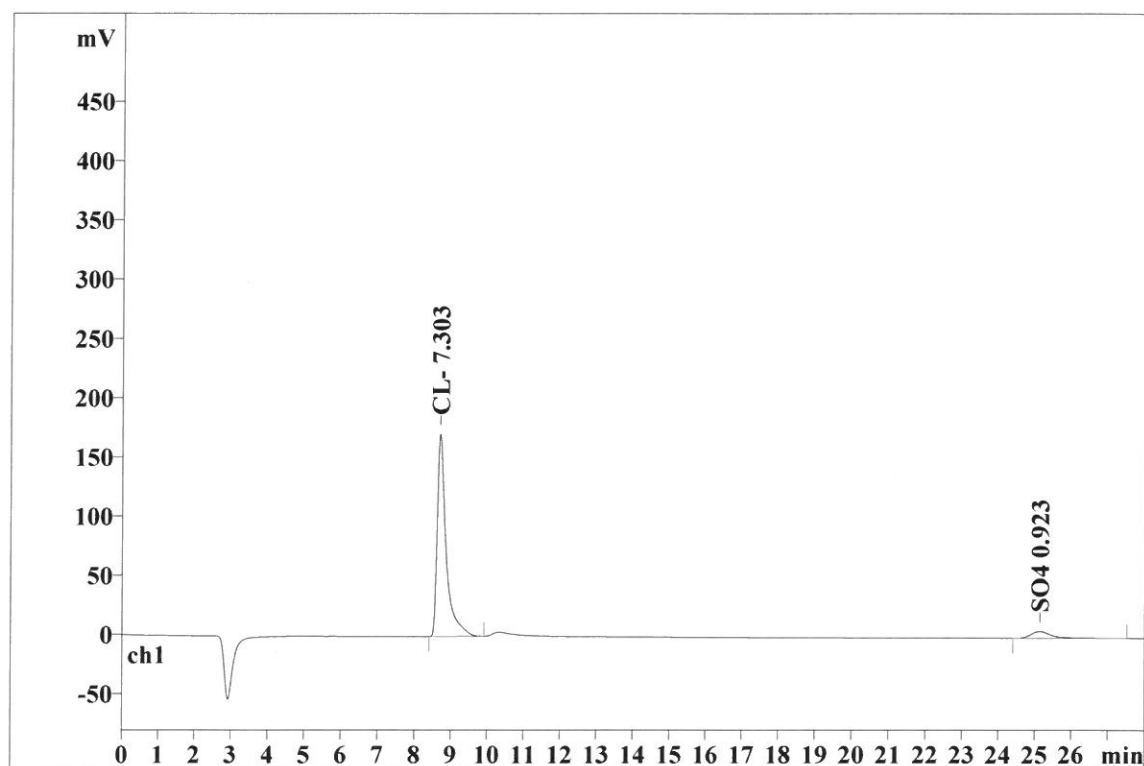

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.71	0.230	170.66	96.70	2931.973	92.79
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.14	0.550	5.82	3.30	227.807	7.21
7	28.00	0.111	176.48	100.00	3159.779	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 2:06:55 PM
Printed by: wet


Ident: J2116-05DLX2
Analysis from: 3/28/2018 9:22:44 PM
File: _2018-03-28_

Last save: 3/29/2018 2:06:30 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16941

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 19
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

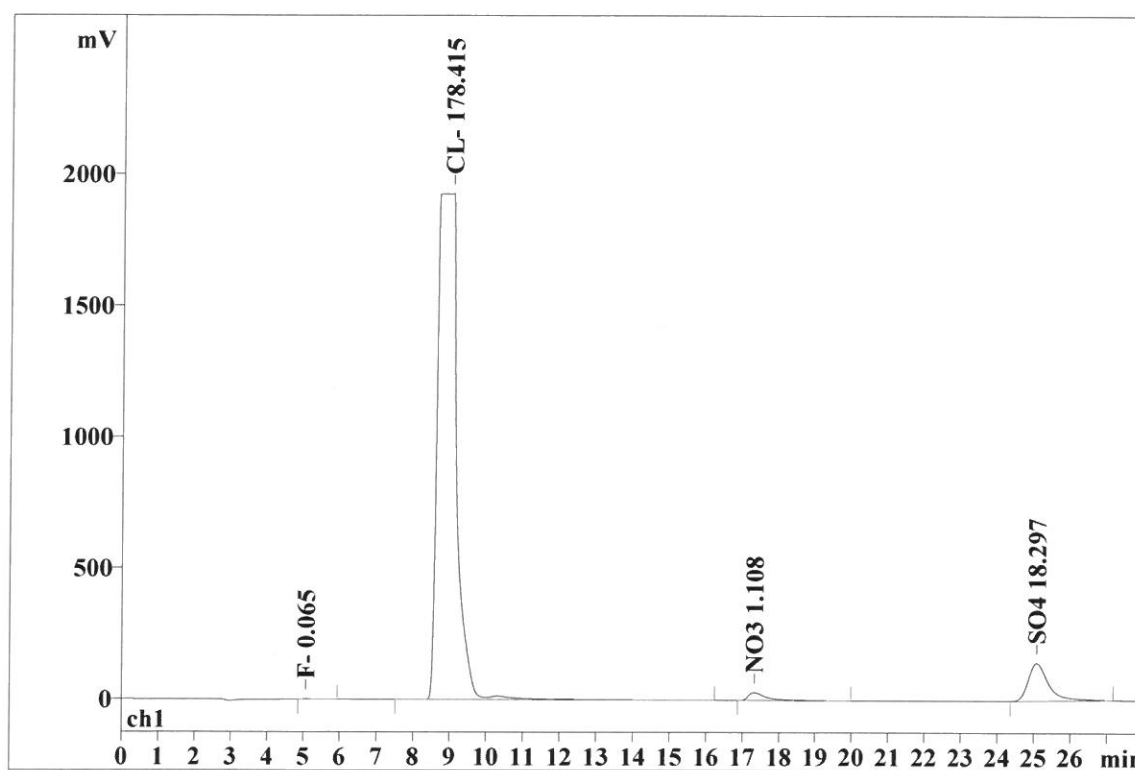

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.07	0.302	1.53	0.07	32.078	0.04
2	9.05	0.534	1930.35	91.81	71787.936	91.54
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	17.32	0.467	30.10	1.43	1058.904	1.35
6	0.00	0.000	0.00	0.00	0.000	0.00
7	25.08	0.547	143.65	6.83	5542.721	7.07
7	28.00	0.264	2105.64	100.15	78421.639	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 2:08:41 PM
Printed by: wet


Ident: CCV
Analysis from: 3/28/2018 10:55:44 PM
File: _2018-03-28_

Last save: 3/29/2018 1:53:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16944

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

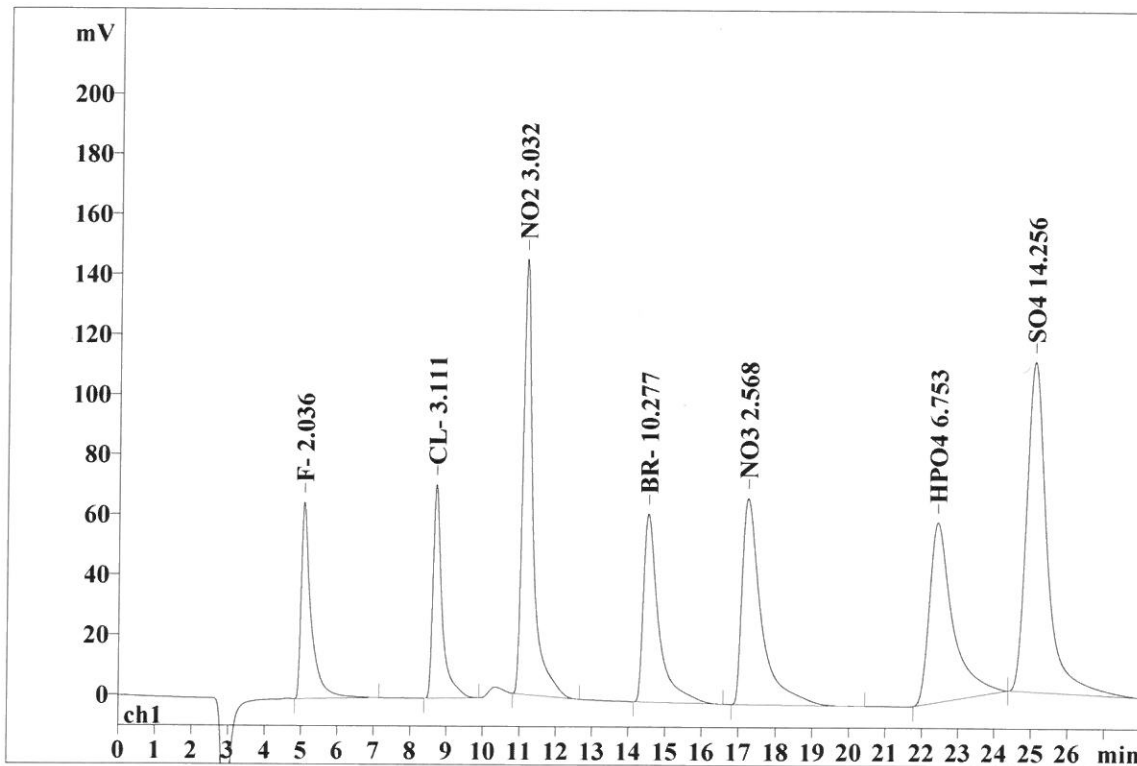

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.07	0.244	65.43	11.22	1240.580	7.45
2	8.70	0.234	71.21	12.22	1245.284	7.48
3	11.16	0.264	145.03	24.88	2878.040	17.28
4	14.52	0.386	62.71	10.76	1819.688	10.93
5	17.23	0.484	68.67	11.78	2478.127	14.88
6	22.41	0.609	59.90	10.28	2682.269	16.11
7	25.07	0.546	109.96	18.86	4306.544	25.86
7	28.00	0.395	582.90	100.00	16650.532	100.00

Report date: 3/29/2018 2:09:03 PM
Printed by: wet


Ident: CCB
Analysis from: 3/28/2018 11:26:42 PM
File: _2018-03-28_

Last save: 3/29/2018 2:08:59 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16945

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

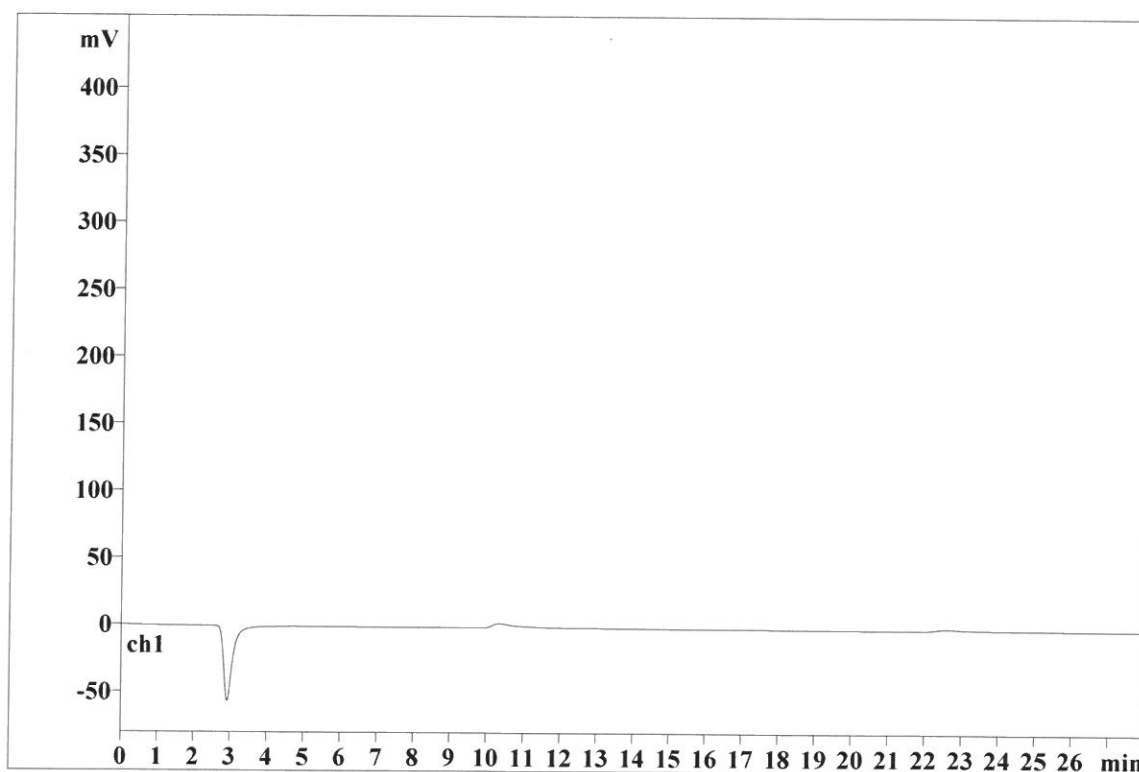

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 2:09:34 PM
Printed by: wet


Ident: CCV
Analysis from: 3/29/2018 8:30:04 AM
File: _2018-03-29_

Last save: 3/29/2018 1:53:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16948

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

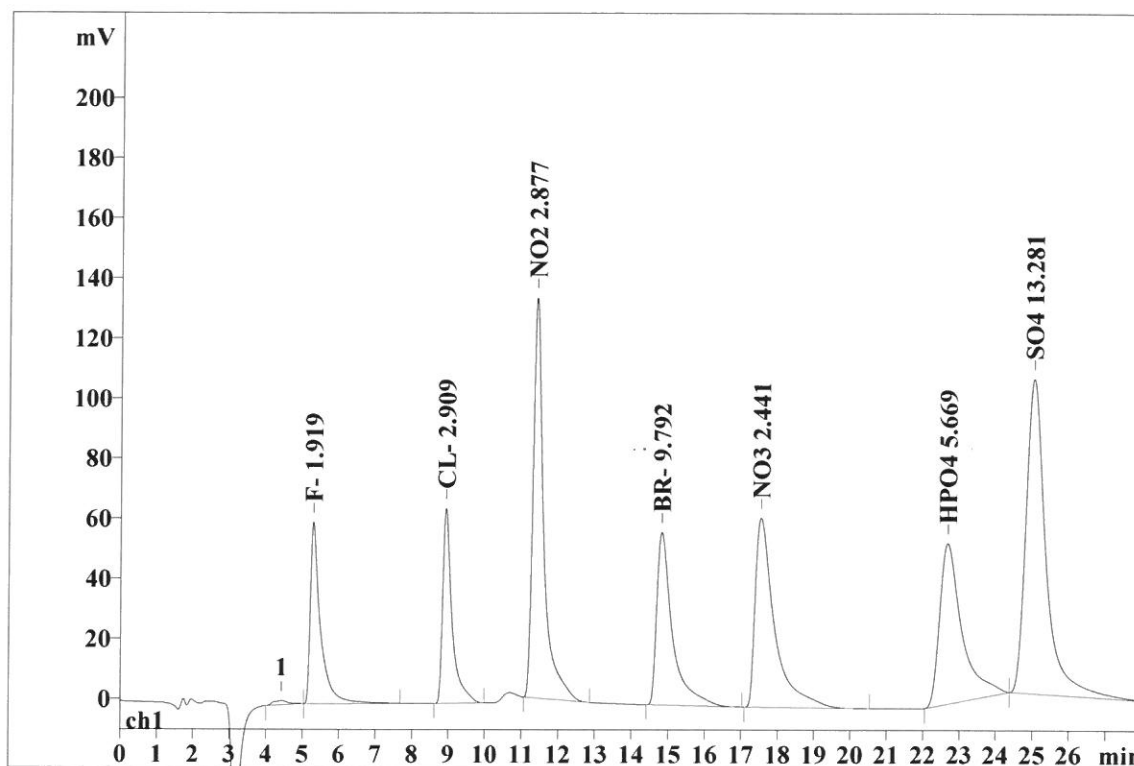

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.28	0.248	60.47	11.22	1169.017	7.55
2	8.93	0.240	64.95	12.05	1163.801	7.52
3	11.40	0.272	133.37	24.74	2727.514	17.62
4	14.81	0.403	57.48	10.66	1733.306	11.20
5	17.53	0.503	63.01	11.69	2354.400	15.21
6	22.66	0.585	53.54	9.93	2280.890	14.74
7	25.03	0.532	104.82	19.45	4008.182	25.90
7	28.00	0.397	537.63	99.74	15437.111	99.75

Report date: 3/29/2018 2:09:47 PM
Printed by: wet


Ident: CCB
Analysis from: 3/29/2018 9:03:21 AM
File: _2018-03-29_

Last save: 3/29/2018 1:53:46 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16949

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

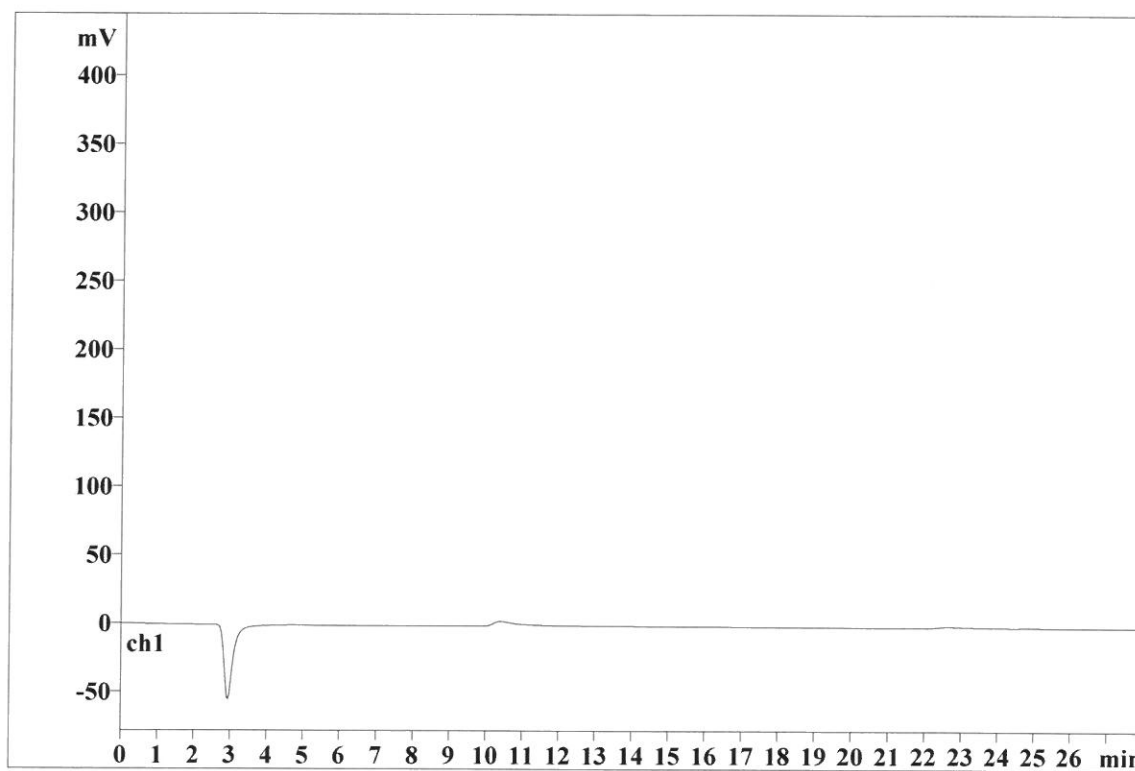

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 2:09:58 PM
Printed by: wet


Ident: LB94228BLW2
Analysis from: 3/29/2018 9:34:19 AM
File: _2018-03-29_

Last save: 3/29/2018 1:53:47 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16950

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

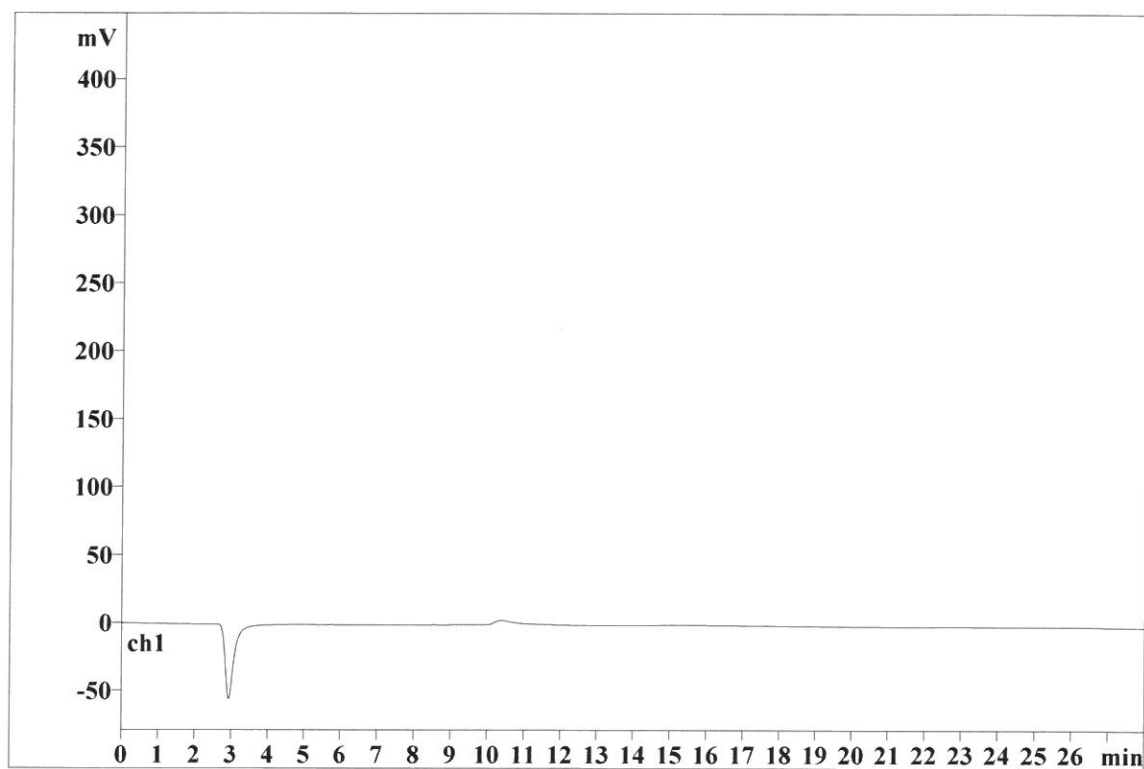

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 2:10:12 PM
Printed by: wet


Ident: LB94228BSW2
Analysis from: 3/29/2018 10:05:17 AM
File: _2018-03-29_

Last save: 3/29/2018 1:53:47 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16951

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

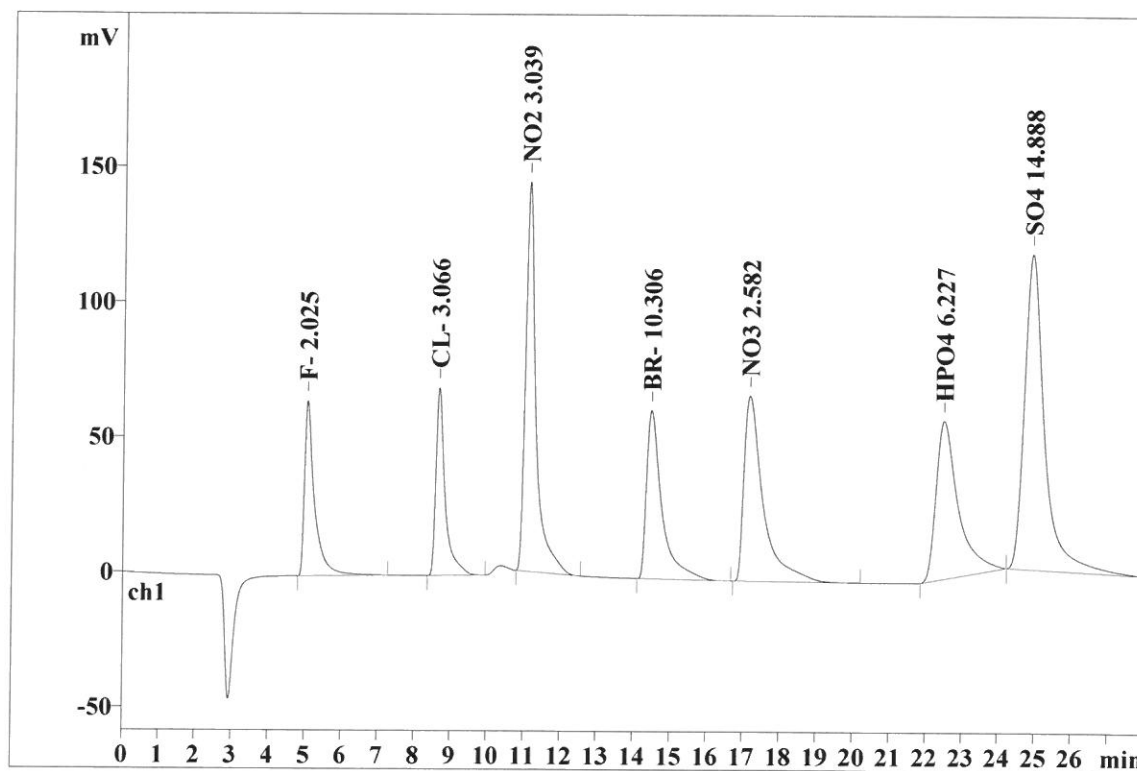

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.05	0.245	64.76	11.08	1233.916	7.41
2	8.67	0.236	69.50	11.89	1227.034	7.37
3	11.12	0.267	144.15	24.67	2885.160	17.33
4	14.47	0.391	62.26	10.65	1825.009	10.96
5	17.17	0.489	68.48	11.72	2491.421	14.96
6	22.48	0.589	58.52	10.01	2487.412	14.94
7	24.90	0.533	116.66	19.96	4499.782	27.03
7	28.00	0.393	584.34	100.00	16649.735	100.00

Report date: 3/29/2018 2:12:55 PM
 Printed by: wet
 Ident: J2116-05DLX100
 Analysis from: 3/29/2018 10:36:21 AM
 File: _2018-03-29_


AK
3/30/18

Last save: 3/29/2018 2:12:52 PM

Method: AnionsIC2-031218.mtw
 Run operator: wet
 Analysis number: 16952

Last save: 3/12/2018 6:21:

SAMPLE:
 : AK/AP
 Vial number: 22
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

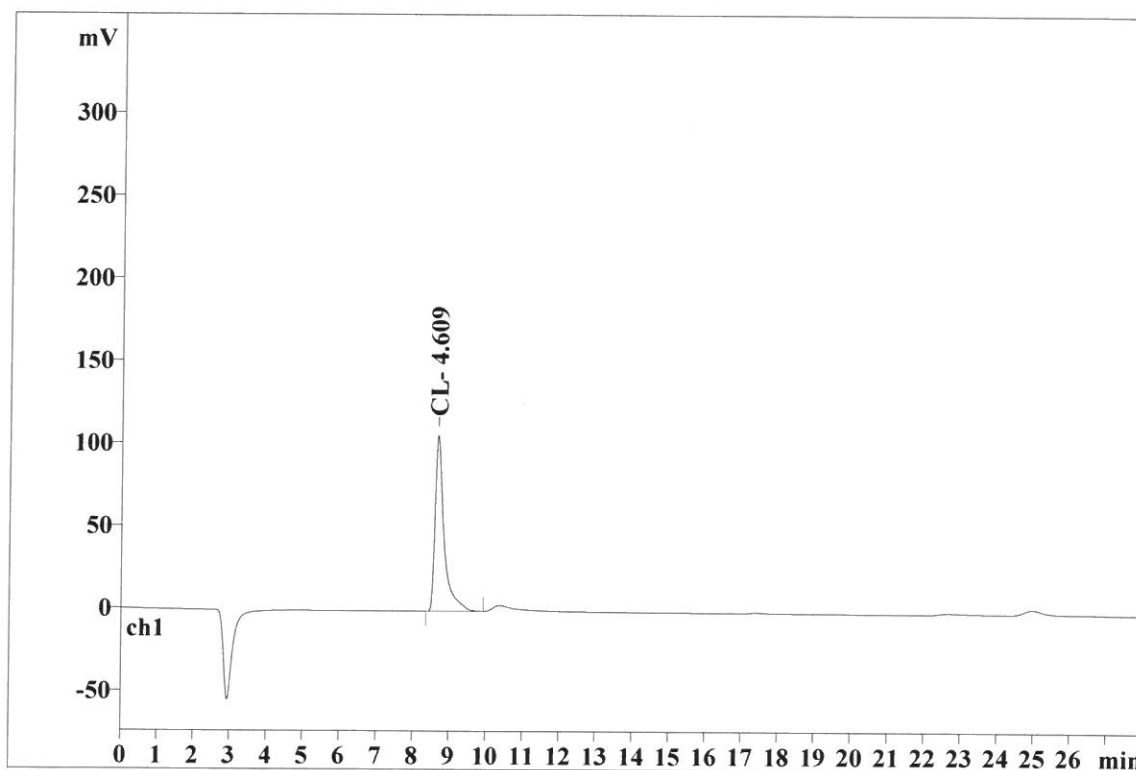

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.68	0.231	106.52	100.00	1848.013	100.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.033	106.52	100.00	1848.013	100.00

Report date: 3/29/2018 2:13:18 PM
Printed by: wet


Ident: J2116-07DLX100
Analysis from: 3/29/2018 11:07:19 AM
File: _2018-03-29_

Last save: 3/29/2018 2:13:14 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16953

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 23
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

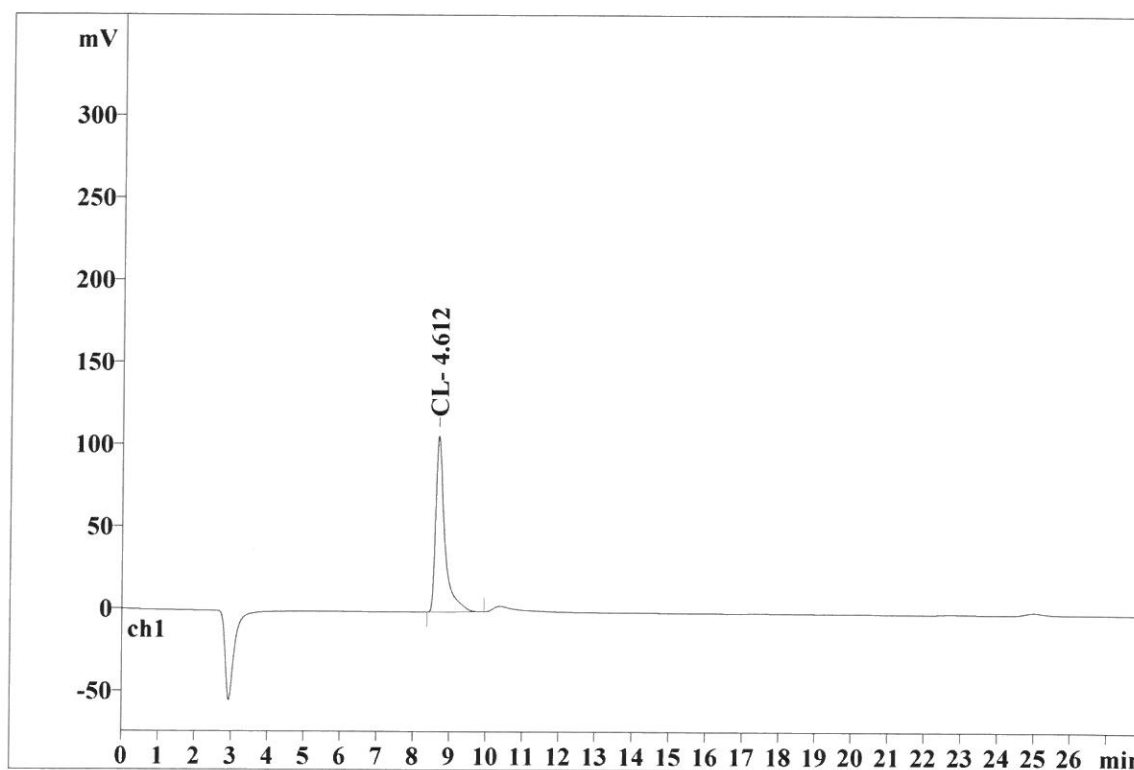

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	0.00	0.000	0.00	0.00	0.000	0.00
2	8.68	0.231	106.96	100.00	1849.387	100.00
3	0.00	0.000	0.00	0.00	0.000	0.00
4	0.00	0.000	0.00	0.00	0.000	0.00
5	0.00	0.000	0.00	0.00	0.000	0.00
6	0.00	0.000	0.00	0.00	0.000	0.00
7	0.00	0.000	0.00	0.00	0.000	0.00
7	28.00	0.033	106.96	100.00	1849.387	100.00

Report date: 3/29/2018 2:13:35 PM
Printed by: wet


Ident: CCV
Analysis from: 3/29/2018 11:38:25 AM
File: _2018-03-29_

Last save: 3/29/2018 1:53:47 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16954

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

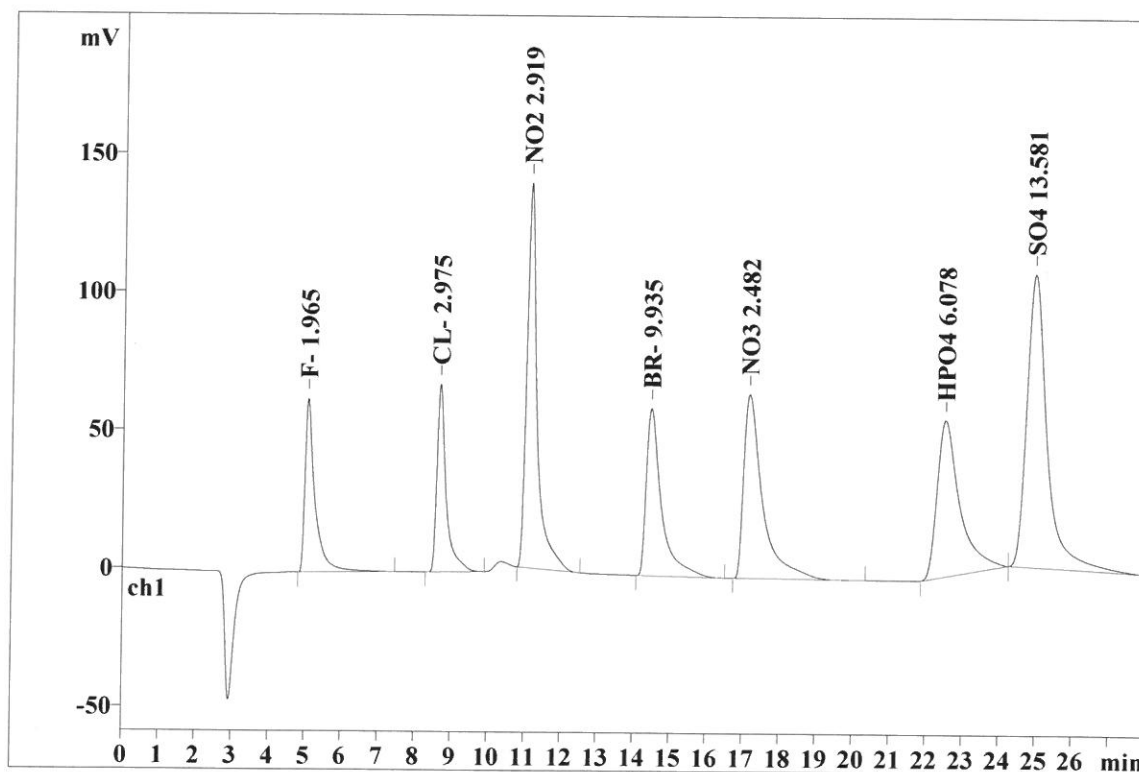

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.06	0.245	62.69	11.21	1197.219	7.56
2	8.67	0.235	67.82	12.13	1190.653	7.52
3	11.12	0.265	139.17	24.89	2768.563	17.48
4	14.46	0.387	60.51	10.82	1758.770	11.10
5	17.15	0.483	66.43	11.88	2394.252	15.11
6	22.50	0.596	56.55	10.11	2432.209	15.35
7	24.93	0.537	105.92	18.95	4099.975	25.88
7	28.00	0.393	559.08	100.00	15841.643	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/29/2018 2:13:46 PM
Printed by: wet


Ident: CCB
Analysis from: 3/29/2018 12:09:23 PM
File: _2018-03-29_

Last save: 3/29/2018 1:53:47 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16955

Last save: 3/12/2018 6:21:

SAMPLE:
:
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

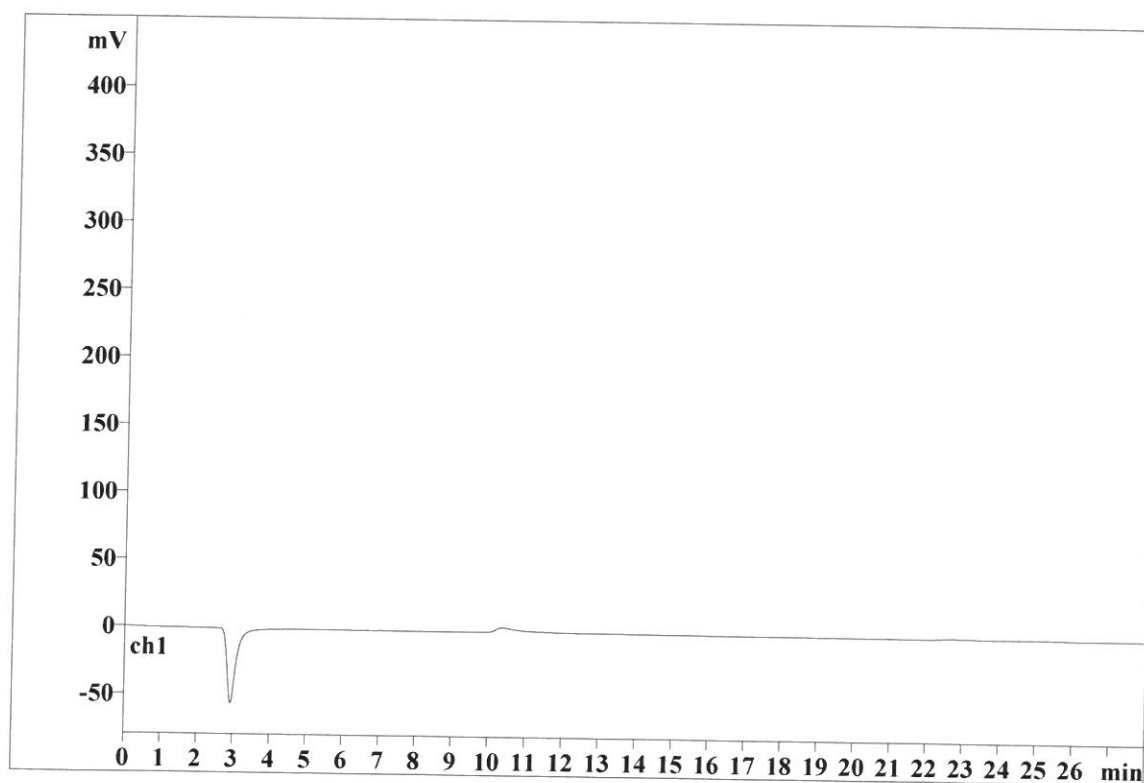

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD