

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

3/29/2018 14:17

Test: ^{Reactive} ~~Total~~ CN ^{Mg/d}

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.677	0.0	0.095	
ICB1	-0.682	0.0	0.003	
CCV1	239.583	0.0	0.234	
CCB1	-0.220	0.0	0.004	
PB107791BL	-0.326	0.0	0.004	
J1749-08	-0.423	0.0	0.004	
J1749-08DUP	-0.255	0.0	0.004	
J1755-06	-0.251	0.0	0.004	
J1761-04	-0.342	0.0	0.004	
J2103-04	-0.468	0.0	0.003	
J2103-08	-0.375	0.0	0.004	
J2103-10	-0.403	0.0	0.004	
J2103-10DUP	-0.399	0.0	0.004	
PB107792BL	-0.599	0.0	0.003	
CCV2	258.599	0.0	0.252	
CCB2	-0.216	0.0	0.004	

N	16
Mean	36.744
SD	86.2700
CV%	234.79

AS

Aquakem v. 7.2AQ1

Results from time period:

Thu Mar 29 13:55:53 2018

Thu Mar 29 14:16:20 2018

Sample Id	Sam/Ctr/c	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.0611	µg/l	3/29/2018 11:24:47	
5.OPPBCN	A	Reactive CN	P	4.5457	µg/l	3/29/2018 11:24:48	
10PPBCN	A	Reactive CN	P	9.5031	µg/l	3/29/2018 11:24:49	
50PPBCN	A	Reactive CN	P	50.321	µg/l	3/29/2018 11:24:50	
100PPBCN	A	Reactive CN	P	100.3069	µg/l	3/29/2018 11:24:51	
250PPBCN	A	Reactive CN	P	250.6823	µg/l	3/29/2018 11:24:52	
500PPBCN	A	Reactive CN	P	499.5798	µg/l	3/29/2018 11:24:53	
ICV1	S	Reactive CN	P	94.6767	µg/l	3/29/2018 13:55:53	
ICB1	S	Reactive CN	P	-0.6819	µg/l	3/29/2018 13:55:54	
CCV1	S	Reactive CN	P	239.5828	µg/l	3/29/2018 13:55:55	
CCB1	S	Reactive CN	P	-0.2203	µg/l	3/29/2018 13:55:56	
PB107791BL	S	Reactive CN	P	-0.3263	µg/l	3/29/2018 13:55:57	
J1749-08	S	Reactive CN	P	-0.4226	µg/l	3/29/2018 13:55:58	
J1749-08DUP	S	Reactive CN	P	-0.2551	µg/l	3/29/2018 13:55:59	
J1755-06	S	Reactive CN	P	-0.2512	µg/l	3/29/2018 13:56:00	
J1761-04	S	Reactive CN	P	-0.3423	µg/l	3/29/2018 13:56:01	
J2103-04	S	Reactive CN	P	-0.4681	µg/l	3/29/2018 13:56:02	
J2103-08	S	Reactive CN	P	-0.3754	µg/l	3/29/2018 13:56:03	
J2103-10	S	Reactive CN	P	-0.4033	µg/l	3/29/2018 14:00:41	
J2103-10DUP	S	Reactive CN	P	-0.399	µg/l	3/29/2018 14:00:42	
PB107792BL	S	Reactive CN	P	-0.5991	µg/l	3/29/2018 14:16:18	
CCV2	S	Reactive CN	P	258.5988	µg/l	3/29/2018 14:16:19	
CCB2	S	Reactive CN	P	-0.2163	µg/l	3/29/2018 14:16:20	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

3/29/2018 15:30


Test Total CN

Accepted 3/29/2018 11:25

Factor 1042
Bias 0.004

Coeff. of det. 0.999994

Errors

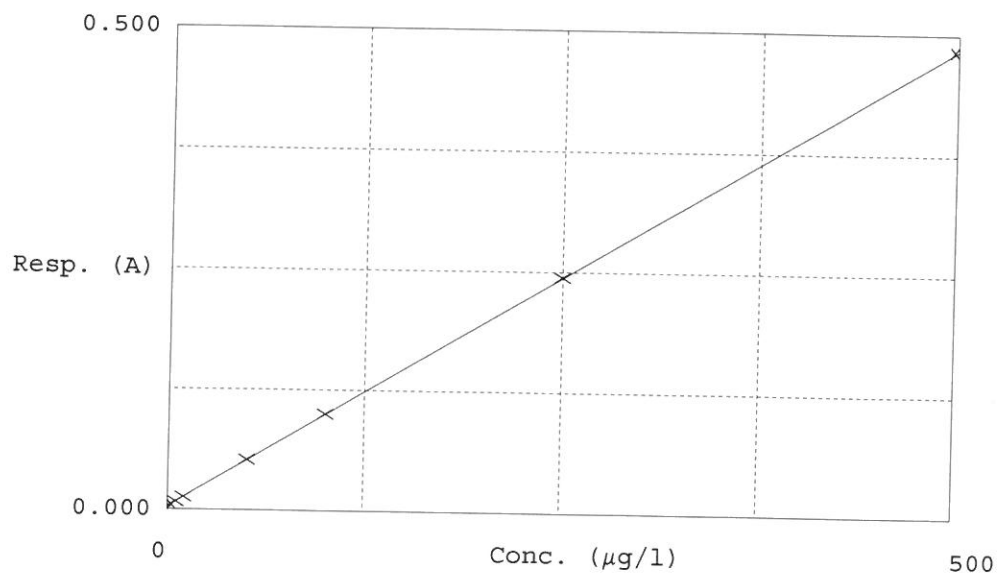

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.004	0.0611	0.0000	
2	5.0PPBCN	0.008	4.5457	5.0000	
3	10PPBCN	0.013	9.5031	10.0000	
4	50PPBCN	0.052	50.3210	50.0000	
5	100PPBCN	0.100	100.3069	100.0000	
6	250PPBCN	0.244	250.6823	250.0000	
7	500PPBCN	0.483	499.5798	500.0000	