

2B94273

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AS

3/30/2018 13:42

Test: ^{Reactive}
Total CN Ng/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.420	0.0	0.091	
ICB1	0.617	0.0	0.004	
CCV1	241.570	0.0	0.227	
CCB1	0.521	0.0	0.004	
PB107828BL	0.266	0.0	0.003	
J1752-04	0.299	0.0	0.004	
J1752-04DUP	0.302	0.0	0.004	
J1752-06	0.455	0.0	0.004	
J1752-08	0.320	0.0	0.004	
J1760-10	0.363	0.0	0.004	
J2137-01	0.357	0.0	0.004	
J2142-02	0.381	0.0	0.004	
J2142-04	0.411	0.0	0.004	
J2142-06	0.659	0.0	0.004	
CCV2	242.382	0.0	0.227	
CCB2	0.554	0.0	0.004	
J2142-08	0.279	0.0	0.003	
J2142-10	0.245	0.0	0.003	
J2146-02	0.256	0.0	0.003	
J2146-04	0.399	0.0	0.004	
CCV3	243.564	0.0	0.228	
CCB3	0.635	0.0	0.004	

N	22
Mean	37.693
SD	85.6597
CV%	227.25

AS

Aquakem v. 7.2AQ1

Results from time period:

Fri Mar 30 13:34:39 2018

Fri Mar 30 13:42:24 2018

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.2108	µg/l	3/30/2018 11:35:24	
5.OPPBCN	A	Reactive CN	P	5.0657	µg/l	3/30/2018 11:35:25	
10PPBCN	A	Reactive CN	P	10.4898	µg/l	3/30/2018 11:35:26	
50PPBCN	A	Reactive CN	P	51.9735	µg/l	3/30/2018 11:35:27	
100PPBCN	A	Reactive CN	P	100.3265	µg/l	3/30/2018 11:35:28	
250PPBCN	A	Reactive CN	P	244.4134	µg/l	3/30/2018 11:35:29	
500PPBCN	A	Reactive CN	P	502.5202	µg/l	3/30/2018 11:35:30	
ICV1	S	Reactive CN	P	94.4205	µg/l	3/30/2018 13:34:39	
ICB1	S	Reactive CN	P	0.6172	µg/l	3/30/2018 13:34:40	
CCV1	S	Reactive CN	P	241.5697	µg/l	3/30/2018 13:34:41	
CCB1	S	Reactive CN	P	0.5213	µg/l	3/30/2018 13:34:42	
PB107828BL	S	Reactive CN	P	0.2661	µg/l	3/30/2018 13:34:43	
J1752-04	S	Reactive CN	P	0.2987	µg/l	3/30/2018 13:34:44	
J1752-04DUP	S	Reactive CN	P	0.3023	µg/l	3/30/2018 13:34:45	
J1752-06	S	Reactive CN	P	0.4549	µg/l	3/30/2018 13:34:46	
J1752-08	S	Reactive CN	P	0.3204	µg/l	3/30/2018 13:34:47	
J1760-10	S	Reactive CN	P	0.3632	µg/l	3/30/2018 13:34:48	
J2137-01	S	Reactive CN	P	0.3569	µg/l	3/30/2018 13:34:49	
J2142-02	S	Reactive CN	P	0.3807	µg/l	3/30/2018 13:42:14	
J2142-04	S	Reactive CN	P	0.4113	µg/l	3/30/2018 13:42:15	
J2142-06	S	Reactive CN	P	0.6587	µg/l	3/30/2018 13:42:16	
CCV2	S	Reactive CN	P	242.3816	µg/l	3/30/2018 13:42:17	
CCB2	S	Reactive CN	P	0.5544	µg/l	3/30/2018 13:42:18	
J2142-08	S	Reactive CN	P	0.2785	µg/l	3/30/2018 13:42:19	
J2142-10	S	Reactive CN	P	0.2453	µg/l	3/30/2018 13:42:20	
J2146-02	S	Reactive CN	P	0.2557	µg/l	3/30/2018 13:42:21	
J2146-04	S	Reactive CN	P	0.3993	µg/l	3/30/2018 13:42:22	
CCV3	S	Reactive CN	P	243.5644	µg/l	3/30/2018 13:42:23	
CCB3	S	Reactive CN	P	0.6353	µg/l	3/30/2018 13:42:24	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

3/30/2018 11:37


Test Total CN

Accepted 3/30/2018 11:37

Factor 1082
Bias 0.003

Coeff. of det. 0.999796

Errors

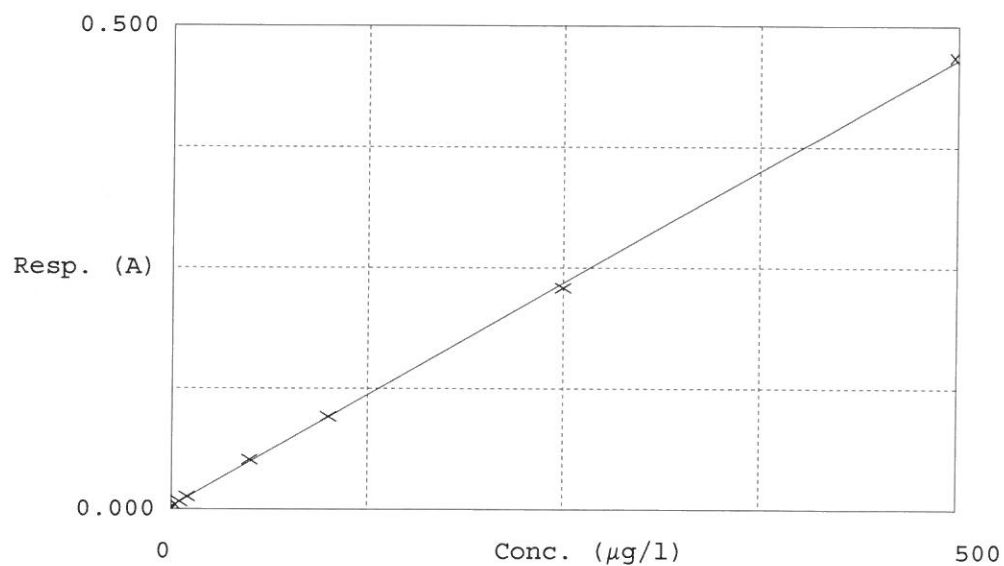

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.2108	0.0000	
2	5.0PPBCN	0.008	5.0657	5.0000	
3	10PPBCN	0.013	10.4898	10.0000	
4	50PPBCN	0.051	51.9735	50.0000	
5	100PPBCN	0.096	100.3265	100.0000	
6	250PPBCN	0.229	244.4134	250.0000	
7	500PPBCN	0.468	502.5202	500.0000	