

Clear table

U-9-18 AR


ident	concentrati on F-	concentrati on CL-	concentrati on NO2	concentrati on BR-	concentrati on NO3	concentrati on HPO4	concentrati on SO4	file name	date time
STD1	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-03-12_	3/12/18 14:48
STD2	0.0990	0.1700	0.1920	0.5550	0.1400	0.0800	0.9150	_2018-03-12_	3/12/18 15:19
STD3	0.3930	0.5930	0.6030	1.9660	0.4940	1.1310	3.0090	_2018-03-12_	3/12/18 15:50
STD4	0.7850	1.1340	1.1260	3.7810	0.9390	1.9910	5.6420	_2018-03-12_	3/12/18 16:21
STD5	2.0420	3.0590	3.0180	10.2330	2.5570	5.2610	15.1600	_2018-03-12_	3/12/18 16:52
STD6	3.9820	6.0440	6.0430	20.1410	5.0470	9.6050	30.2060	_2018-03-12_	3/12/18 17:22
STD7	5.0010	7.4500	7.4680	24.8250	6.1980	12.6820	37.3180	_2018-03-12_	3/12/18 17:53
ICV	1.9420	2.8620	2.8360	9.5800	2.3790	4.6970	14.2480	_2018-03-12_	3/12/18 19:26
ICB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-03-12_	3/12/18 19:57
CCV	2.0330	3.0530	3.0030	10.1690	2.5410	4.8070	14.6140	_2018-03-15_	3/15/18 19:18
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-03-15_	3/15/18 19:49
LB94460BLW	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-03-15_	3/15/18 20:20
LB94460BSW	1.9770	2.9030	2.9030	9.7860	2.4560	4.7430	14.8110	_2018-03-15_	3/15/18 20:51
J1161-07	0.1130	0.1830	0.1960	0.5860	0.1510	0.1300	0.9420	_2018-03-16_	3/16/18 0:58
J1161-09	0.1070	0.1790	0.1930	0.5480	0.1450	0.1080	0.9320	_2018-03-16_	3/16/18 1:29
J1161-08	0.2320	0.3430	0.3610	1.1540	0.3070	0.5580	1.8760	_2018-03-16_	3/16/18 2:31
CCV	2.0480	3.0850	3.0430	10.3030	2.5780	4.8660	14.6430	_2018-03-16_	3/16/18 3:02
CCB	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	0.0000	_2018-03-16_	3/16/18 3:33

IC-2

3-12-18 AK

CALIBRATION OF COMPONENT F-

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.0326208 \cdot A + 0.253285$
 RSD: 1.183 %
 Correlation coefficient: 0.999943

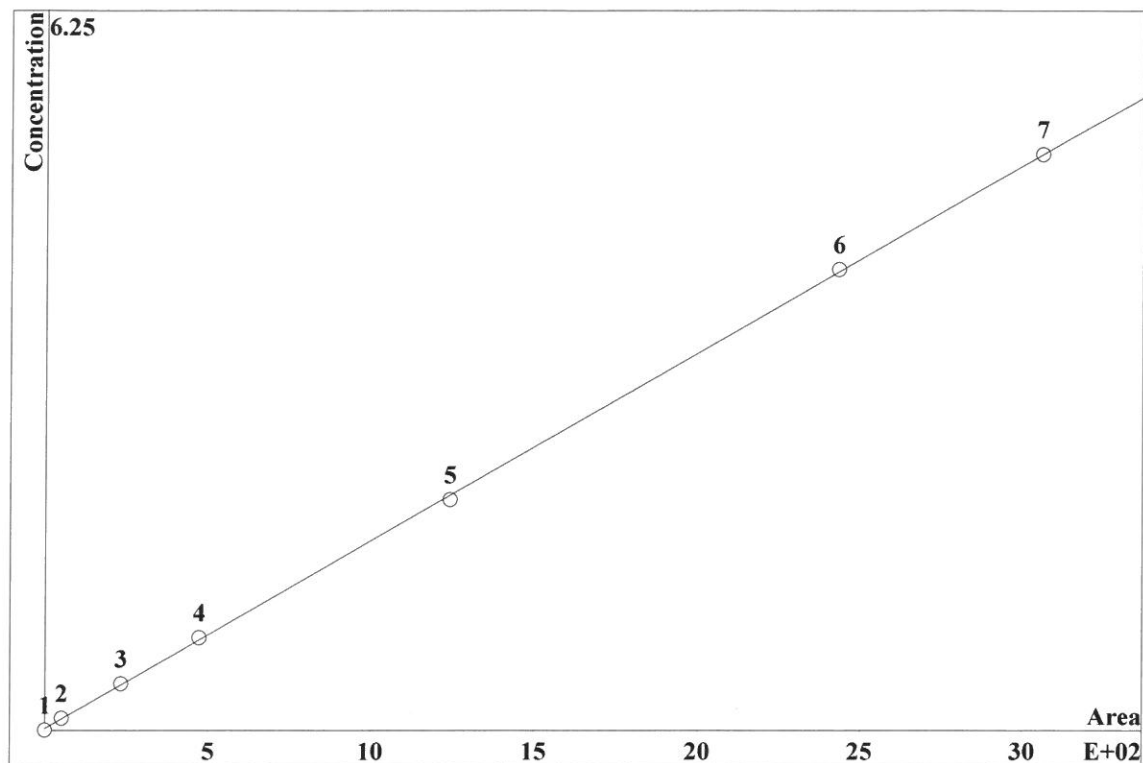

K3 = 0 K2 = 0 K1 = 0.0326208 K0 = 0.253285

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		
2	3.69	52.63	0.1	20	5.099		
3	15.34	233.2	0.4	20	5.099		
4	31.64	473.3	0.8	20	5.099		
5	84.72	1244	2	20	5.099		
6	162.6	2433	4	20	5.099		
7	204.1	3058	5	20	5.099		

CALIBRATION OF COMPONENT CL-

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.0497015 \cdot A + 0.332296$
 RSD: 1.834 %
 Correlation coefficient: 0.999863

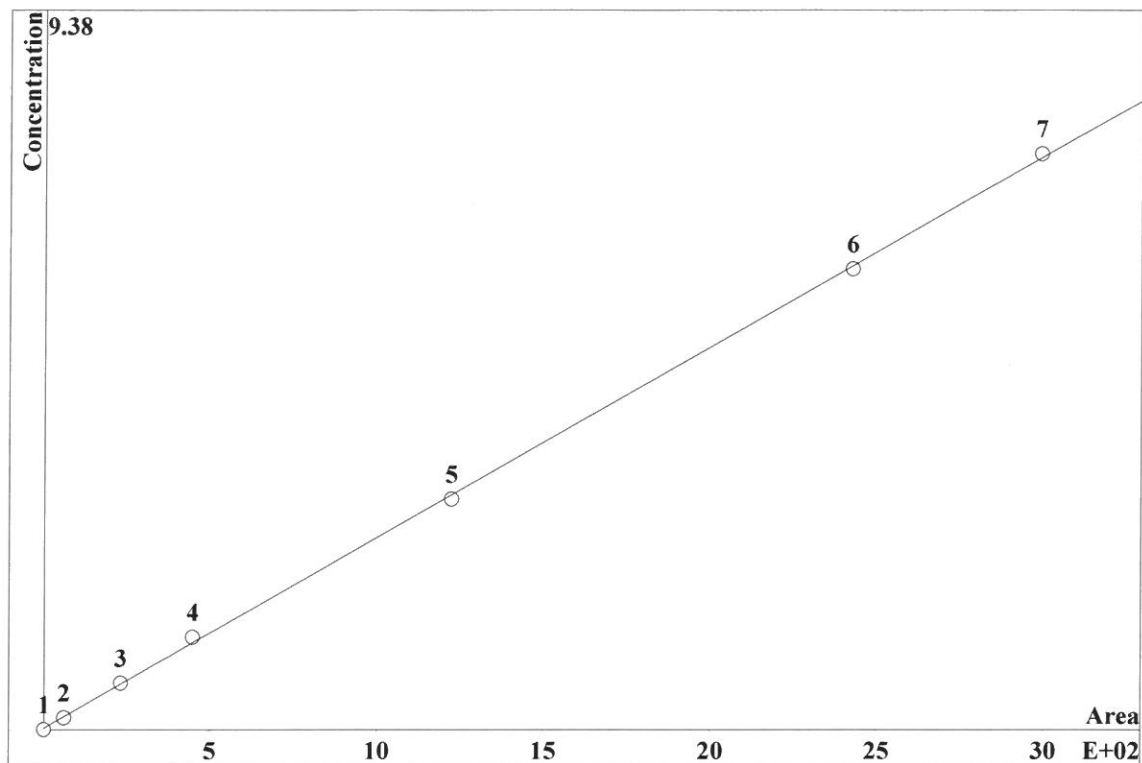

K3 = 0 K2 = 0 K1 = 0.0497015 K0 = 0.332296

Base: Area

Ref.channel: chl

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.212	61.67	0.15	20	8.753		
3	15.96	231.8	0.6	20	8.753		
4	30.65	449.6	1.2	20	8.753		
5	84.5	1224	3	20	8.753		
6	169	2425	6	20	8.753		
7	207.6	2991	7.5	20	8.753		

CALIBRATION OF COMPONENT NO2

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.0206268 \cdot A + 1.27253$
 RSD: 1.661 %
 Correlation coefficient: 0.999887

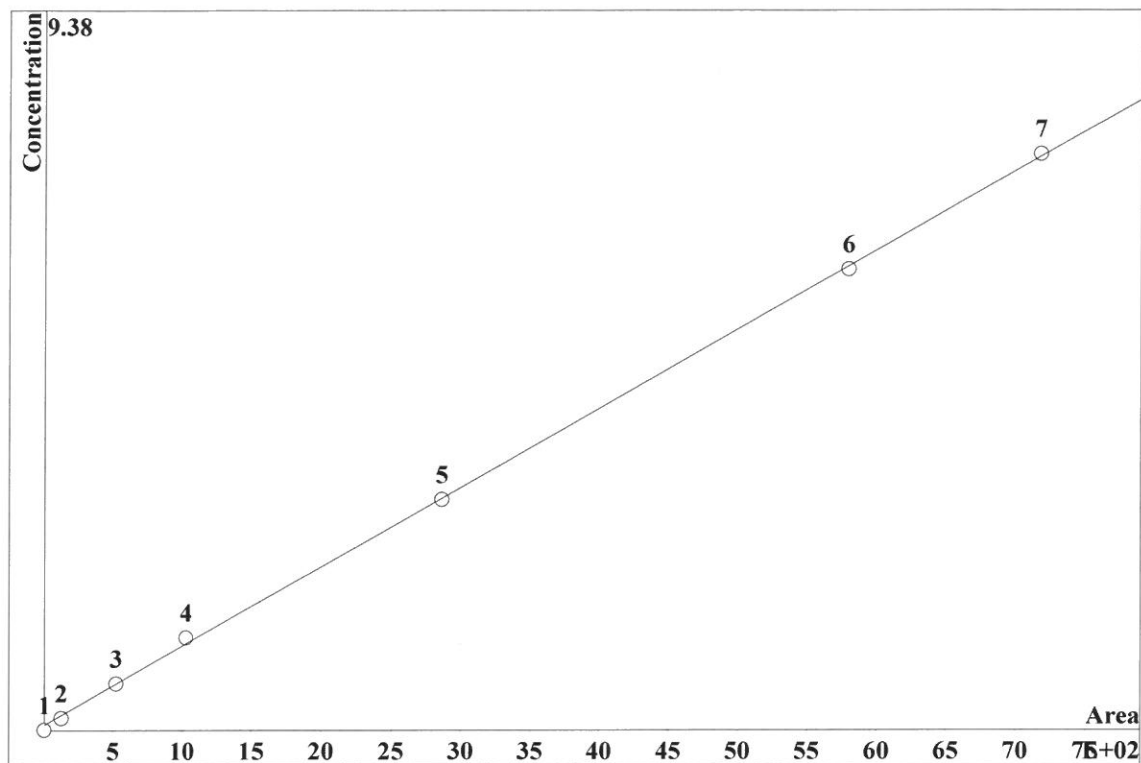

K3 = 0 K2 = 0 K1 = 0.0206268 K0 = 1.27253

Base: Area

Ref.channel: ch1

ISTD:


Formula: Linear

Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	7.466	124.7	0.15	20	11.21		
3	30.77	523.1	0.6	20	11.21		
4	60.82	1030	1.2	20	11.21		
5	170.2	2864	3	20	11.21		
6	342.3	5798	6	20	11.21		
7	425.3	7179	7.5	20	11.21		

CALIBRATION OF COMPONENT BR-

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.112224 \cdot A + 1.31848$
 RSD: 1.932 %
 Correlation coefficient: 0.999848

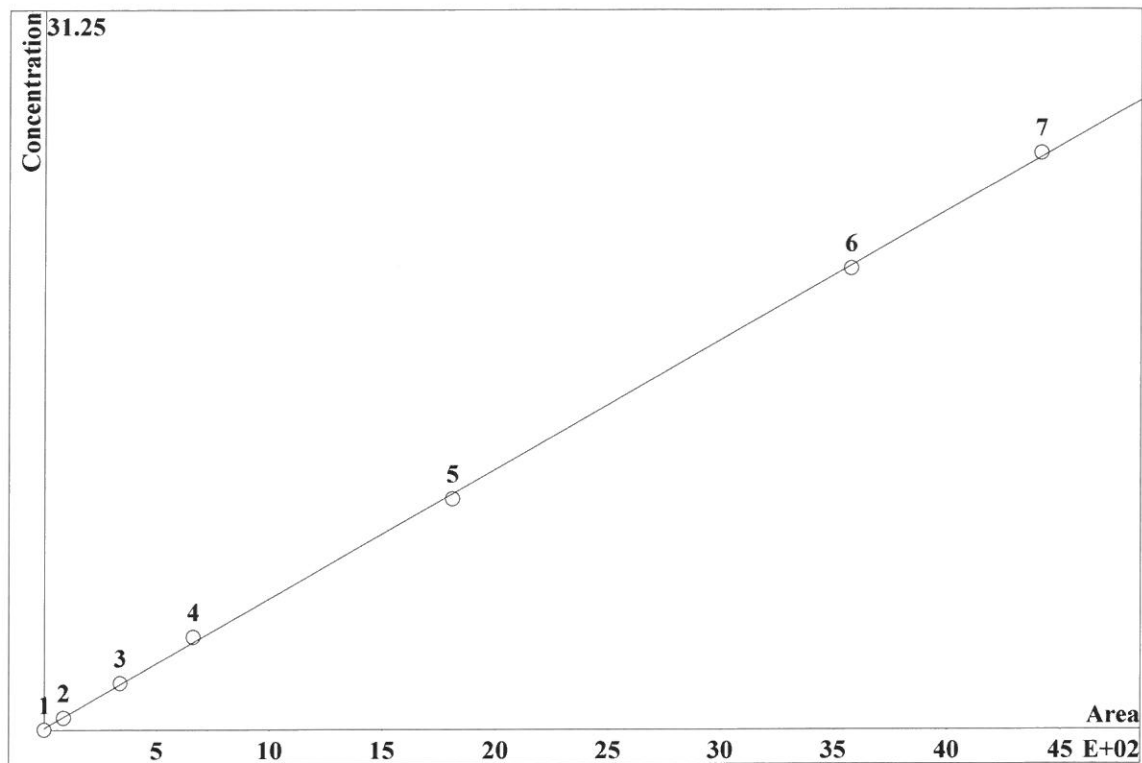


K3 = 0 K2 = 0 K1 = 0.112224 K0 = 1.31848
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	3.607	87.1	0.5	20	14.51		
3	14.28	338.6	2	20	14.51		
4	27.68	662.1	4	20	14.51		
5	75.39	1812	10	20	14.51		
6	148.6	3578	20	20	14.51		
7	181.8	4412	25	20	14.51		

CALIBRATION OF COMPONENT NO3

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.020582 \cdot A + 0.358059$
 RSD: 2.151 %
 Correlation coefficient: 0.999811

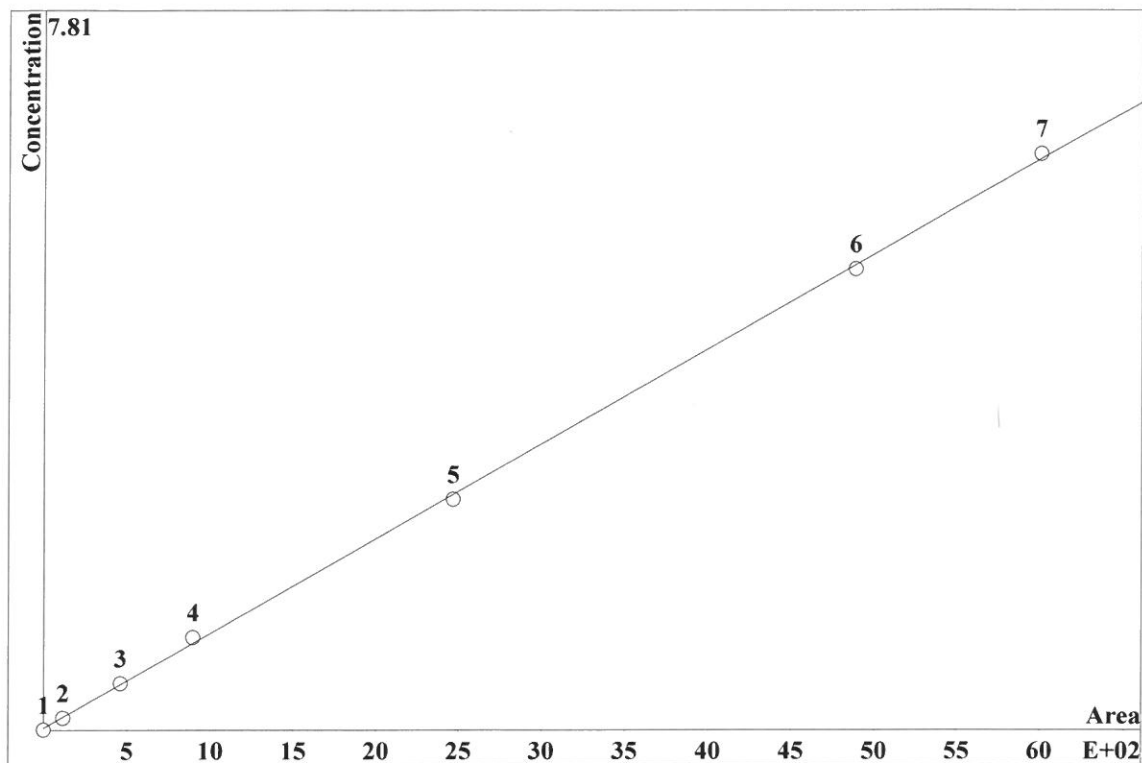


K3 = 0 K2 = 0 K1 = 0.020582 K0 = 0.358059
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	4.168	118.6	0.125	20	17.18		
3	16.3	462.8	0.5	20	17.18		
4	31.02	895.4	1	20	17.18		
5	83.09	2467	2.5	20	17.18		
6	158.8	4887	5	20	17.18		
7	191	6005	6.25	20	17.18		

CALIBRATION OF COMPONENT HPO4

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.0540131 \cdot A - 9.81679$
 RSD: 5.375 %
 Correlation coefficient: 0.998820

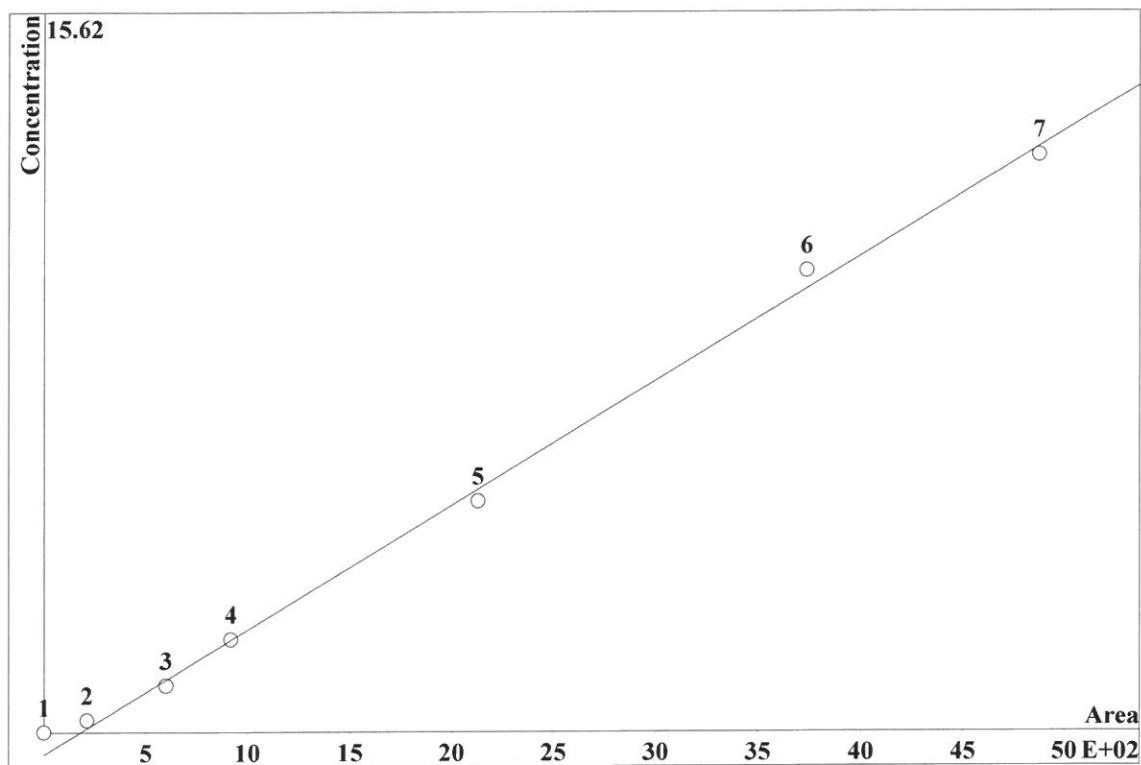


K3 = 0 K2 = 0 K1 = 0.0540131 K0 = -9.81679
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1		0	0	0			0
2	4.678	211.5	0.25	20			23.13
3	13.9	600.4	1	20			23.13
4	21.89	919	2	20			23.13
5	53.45	2130	5	20			23.13
6	96.42	3738	10	20			23.13
7	111.5	4878	12.5	20			23.13

CALIBRATION OF COMPONENT SO4

Method: AnionsIC2-031218.mtw
 Equation: $Q = 0.0653755 \cdot A + 3.57615$
 RSD: 1.648 %
 Correlation coefficient: 0.999889

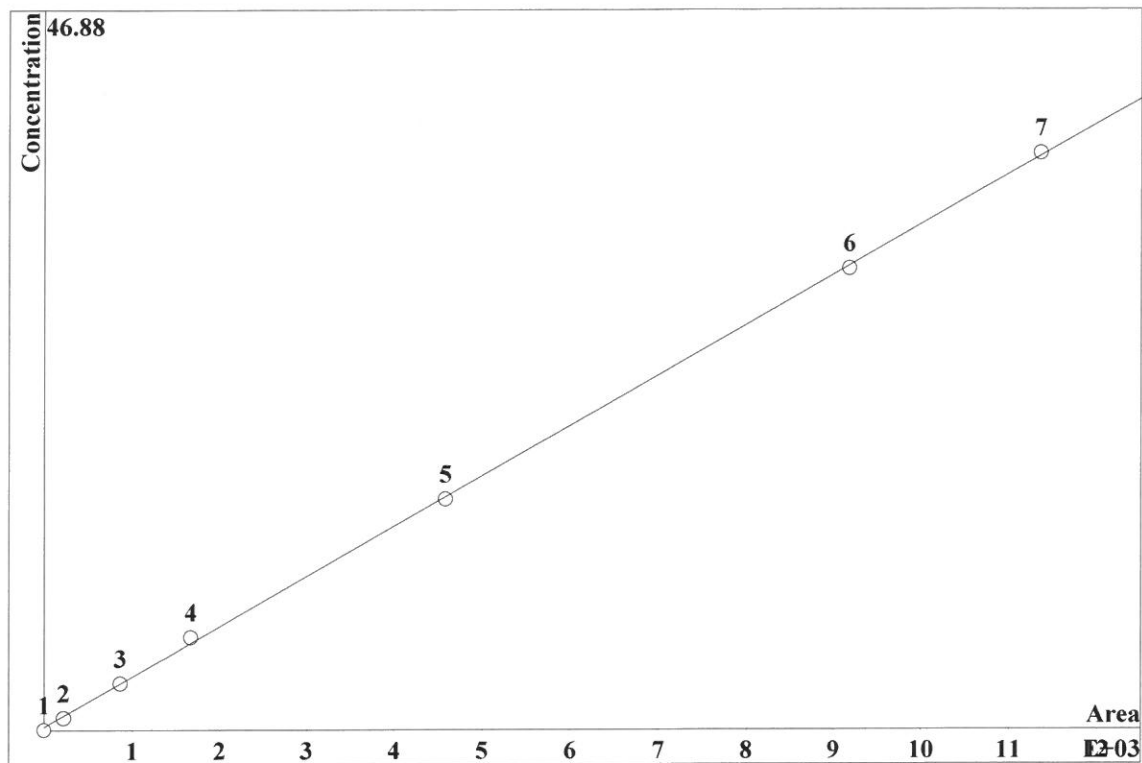

K3 = 0 K2 = 0 K1 = 0.0653755 K0 = 3.57615
 Base: Area
 Ref.channel: ch1
 ISTD:
 Formula: Linear
 Weight: 1

Level	Height	Area	Conc.	Vol/Dil	Retention	Used	File
1	0	0	0	0	0		0
2	6.231	225.4	0.75	20	25.36		
3	24.05	865.8	3	20	25.36		
4	46.34	1671	6	20	25.36		
5	127.1	4583	15	20	25.36		
6	253.6	9186	30	20	25.36		
7	310.5	1.136e+04	37.5	20	25.36		

Report date: 3/15/2018 9:22:39 AM
Printed by: wet


Ident: STD1
Analysis from: 3/12/2018 2:48:21 PM
File: _2018-03-12_

Last save: 3/12/2018 3:16:21 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16713

Last save: 3/12/2018 1:40:

SAMPLE:
:
Vial number: 2
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

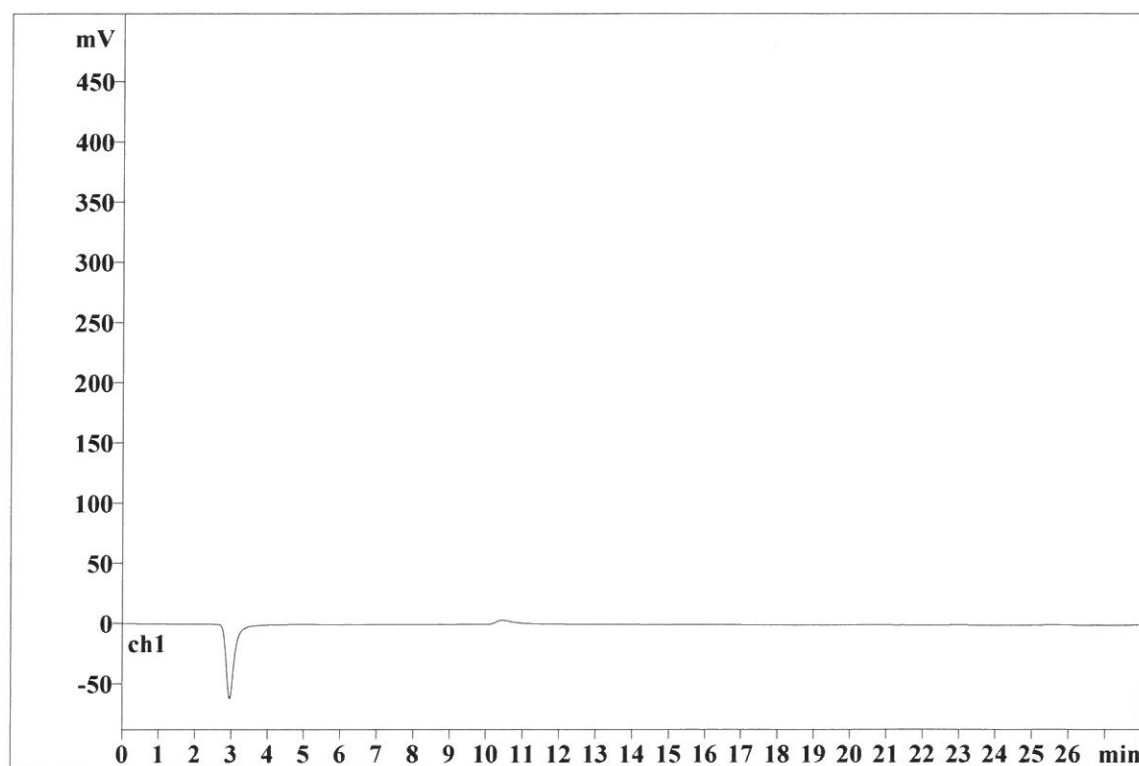

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:27:52 AM
Printed by: wet


Ident: STD2
Analysis from: 3/12/2018 3:19:16 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16714

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

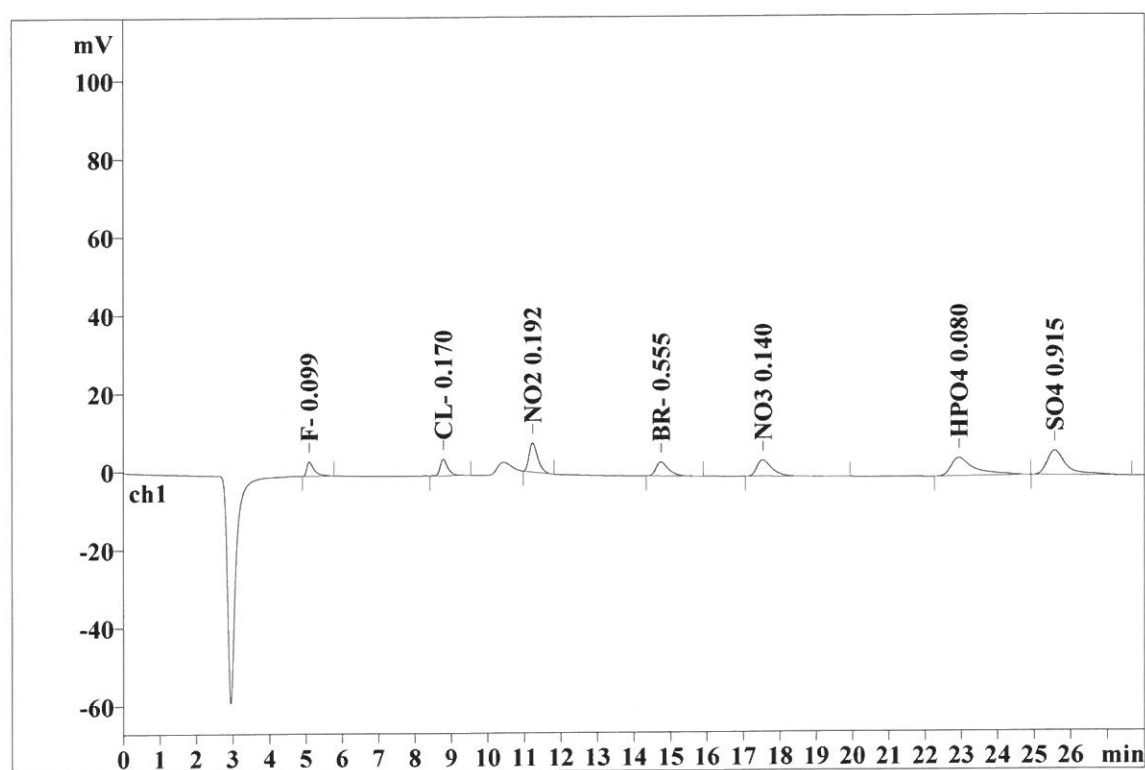

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.10	0.199	3.69	10.83	52.635	5.97
2	8.79	0.216	4.21	12.37	61.667	6.99
3	11.24	0.254	7.46	21.92	124.683	14.14
4	14.74	0.357	3.61	10.59	87.097	9.88
5	17.54	0.422	4.17	12.24	118.598	13.45
6	22.94	0.580	4.68	13.73	211.548	24.00
7	25.57	0.494	6.23	18.29	225.363	25.56
7	28.00	0.360	34.04	99.98	881.591	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:28:14 AM
Printed by: wet


Ident: STD3
Analysis from: 3/12/2018 3:50:12 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16715

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

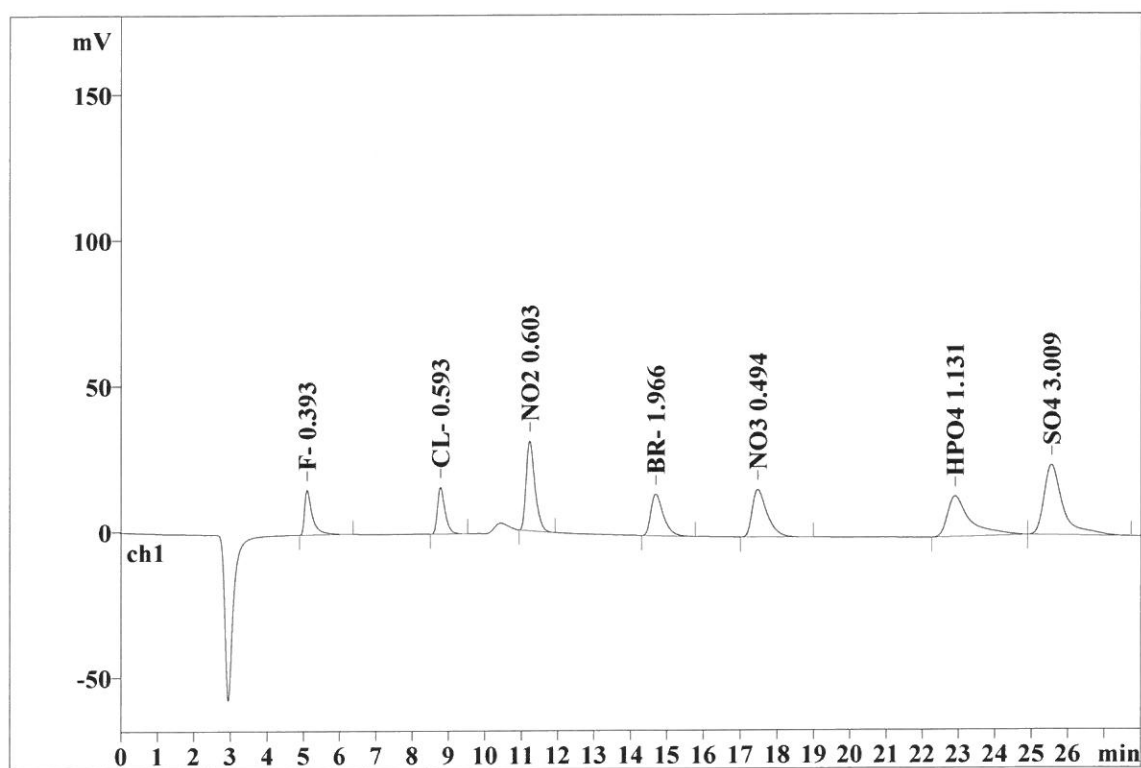

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.201	15.34	11.75	233.152	7.16
2	8.78	0.215	15.96	12.22	231.849	7.12
3	11.23	0.255	30.76	23.56	523.099	16.07
4	14.70	0.354	14.28	10.94	338.575	10.40
5	17.47	0.424	16.30	12.48	462.750	14.21
6	22.91	0.555	13.90	10.64	600.416	18.44
7	25.55	0.493	24.05	18.41	865.815	26.59
7	28.00	0.357	130.59	100.00	3255.658	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:28:24 AM
Printed by: wet


Ident: STD4
Analysis from: 3/12/2018 4:21:07 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16716

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

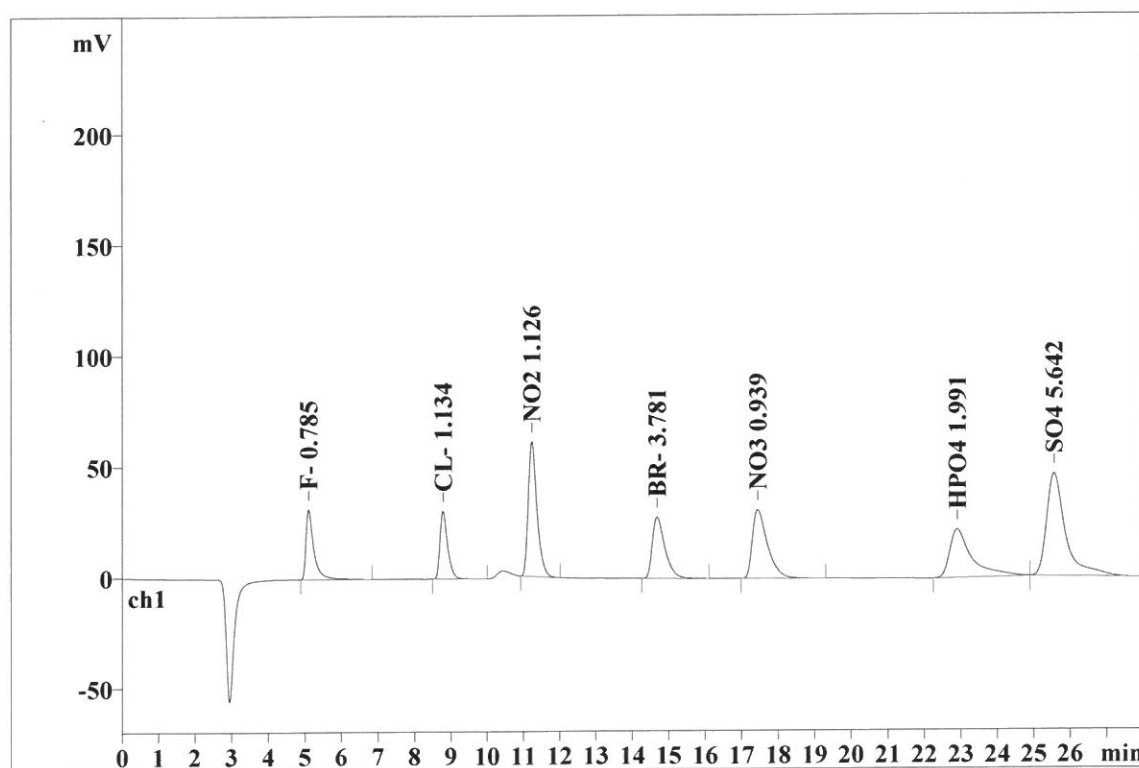

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.10	0.200	31.64	12.65	473.320	7.76
2	8.78	0.215	30.65	12.26	449.624	7.37
3	11.24	0.252	60.82	24.32	1030.197	16.89
4	14.68	0.355	27.68	11.07	662.135	10.85
5	17.44	0.430	31.02	12.41	895.396	14.68
6	22.90	0.543	21.89	8.75	919.000	15.06
7	25.56	0.493	46.34	18.53	1671.278	27.39
7	28.00	0.356	250.03	100.00	6100.950	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:28:37 AM
Printed by: wet


Ident: STD5
Analysis from: 3/12/2018 4:52:03 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16717

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 6
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

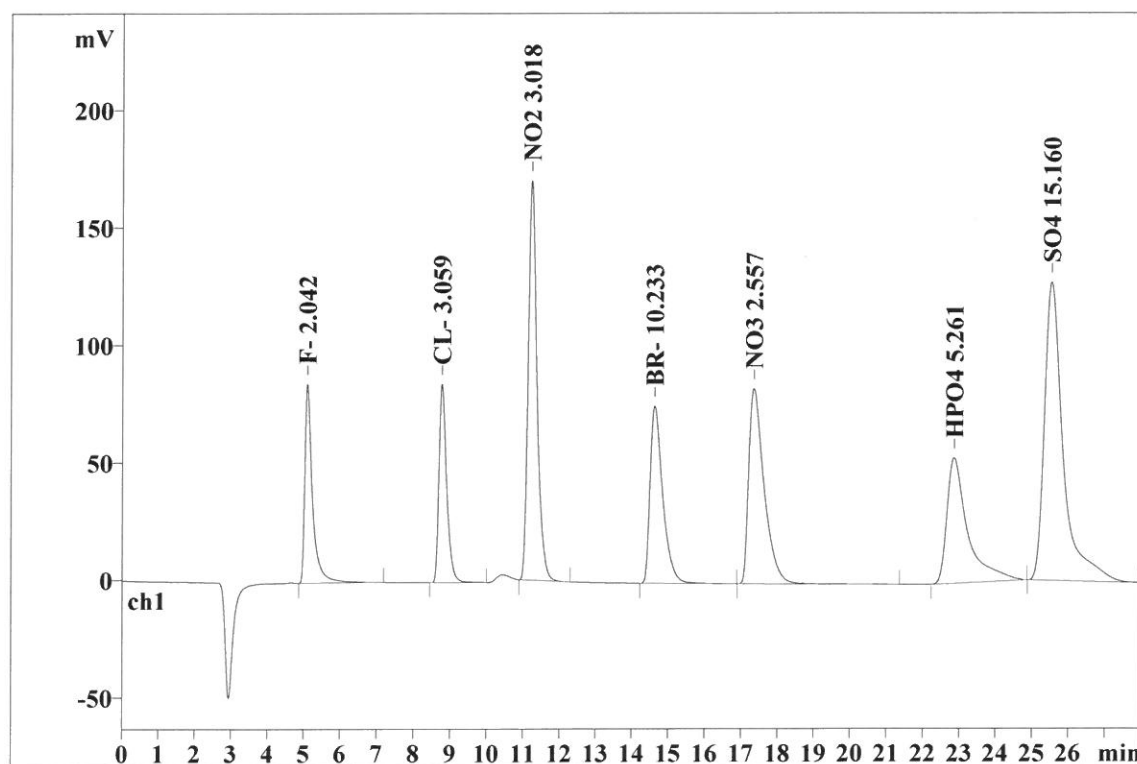

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.10	0.195	84.72	12.49	1243.953	7.62
2	8.78	0.212	84.50	12.45	1224.371	7.50
3	11.24	0.248	170.18	25.09	2864.331	17.55
4	14.63	0.356	75.38	11.11	1811.944	11.10
5	17.35	0.444	83.08	12.25	2467.367	15.11
6	22.85	0.520	53.44	7.88	2129.894	13.05
7	25.54	0.493	127.10	18.73	4583.220	28.07
7	28.00	0.353	678.41	100.00	16325.081	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:28:50 AM
Printed by: wet


Ident: STD6
Analysis from: 3/12/2018 5:22:59 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16718

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 7
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

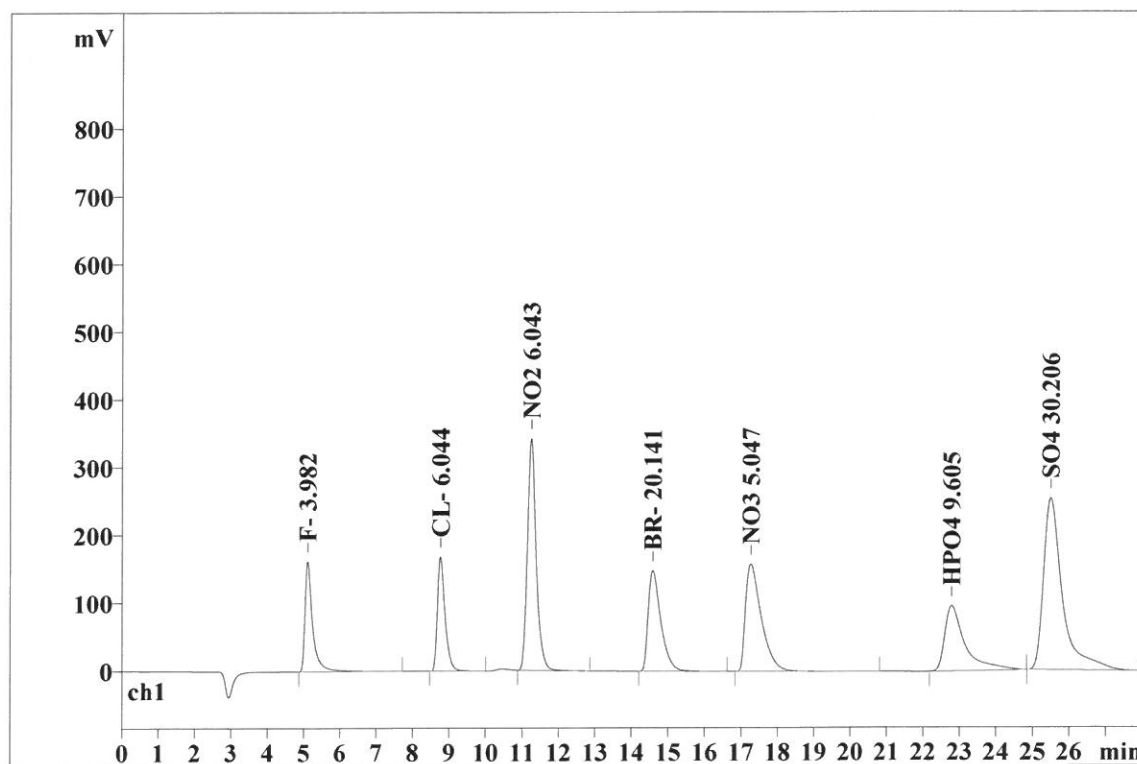

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.11	0.199	162.62	12.21	2433.439	7.59
2	8.77	0.210	169.02	12.69	2425.395	7.57
3	11.26	0.249	342.33	25.71	5797.554	18.09
4	14.58	0.358	148.60	11.16	3577.601	11.16
5	17.26	0.465	158.84	11.93	4886.878	15.25
6	22.78	0.512	96.42	7.24	3738.176	11.67
7	25.49	0.495	253.60	19.05	9185.915	28.67
7	28.00	0.356	1331.44	100.00	32044.959	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:29:03 AM
Printed by: wet


Ident: STD7
Analysis from: 3/12/2018 5:53:54 PM
File: _2018-03-12_

Last save: 3/15/2018 9:26:30 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16719

Last save: 3/12/2018 5:50:

SAMPLE:
: AK/AP
Vial number: 8
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

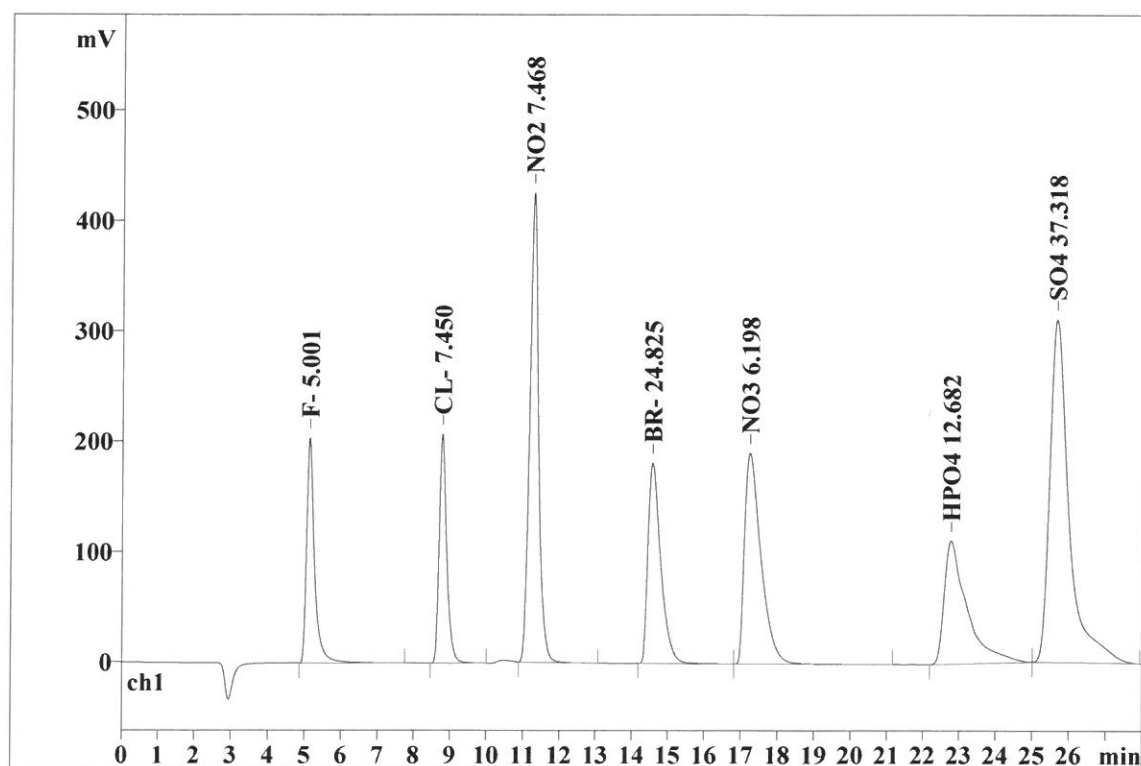

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.12	0.205	204.14	12.51	3058.124	7.67
2	8.77	0.211	207.64	12.72	2991.295	7.50
3	11.27	0.248	425.32	26.06	7179.305	18.00
4	14.57	0.361	181.84	11.14	4412.390	11.06
5	17.23	0.476	191.01	11.70	6004.853	15.06
6	22.77	0.617	111.54	6.83	4877.587	12.23
7	25.65	0.501	310.48	19.02	11361.773	28.49
7	28.00	0.374	1631.96	100.00	39885.328	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:32:31 AM
Printed by: wet


Ident: ICV
Analysis from: 3/12/2018 7:26:41 PM
File: _2018-03-12_

Last save: 3/12/2018 7:54:41 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16722

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

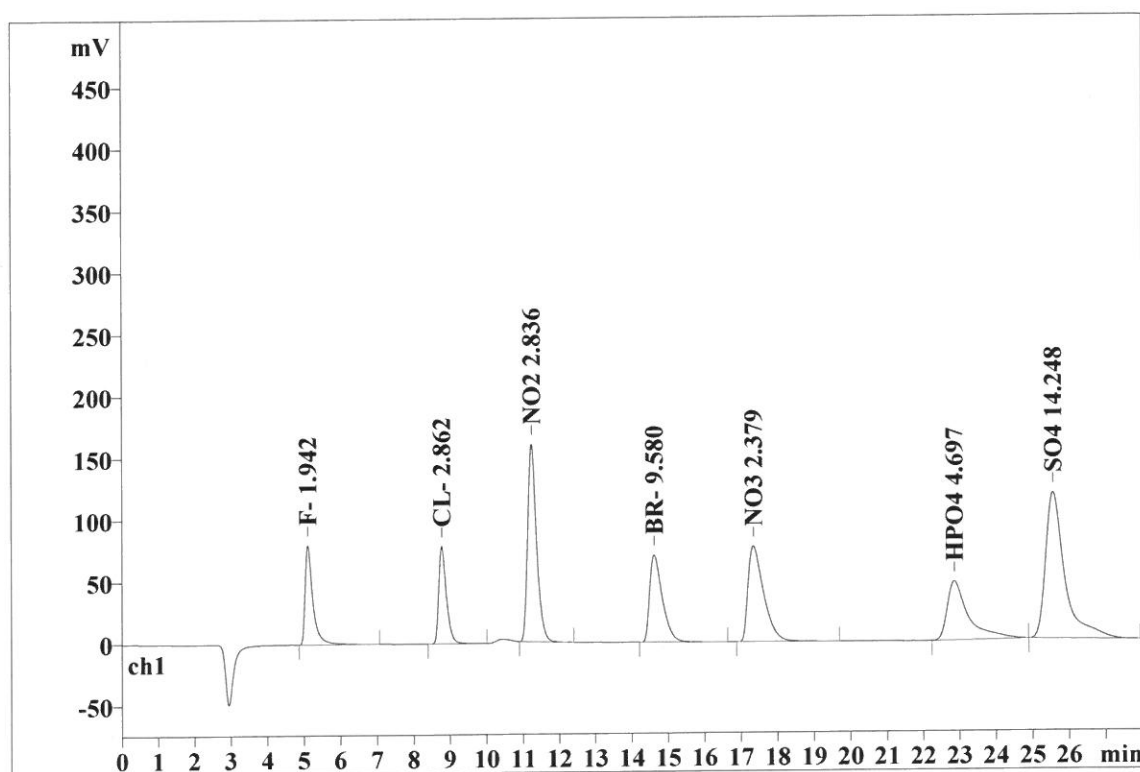

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.11	0.199	80.26	12.69	1182.971	7.77
2	8.78	0.215	78.76	12.45	1145.119	7.52
3	11.24	0.250	159.65	25.24	2688.082	17.65
4	14.62	0.360	70.56	11.16	1695.607	11.13
5	17.34	0.449	77.35	12.23	2294.187	15.06
6	22.85	0.525	47.60	7.53	1920.950	12.61
7	25.56	0.496	118.25	18.70	4304.268	28.26
7	28.00	0.356	632.44	100.00	15231.184	100.00

This report has been created by IC Net
METROHM LTD

Report date: 3/15/2018 9:32:41 AM
Printed by: wet


Ident: ICB
Analysis from: 3/12/2018 7:57:37 PM
File: _2018-03-12_

Last save: 3/12/2018 8:25:37 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16723

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 12
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

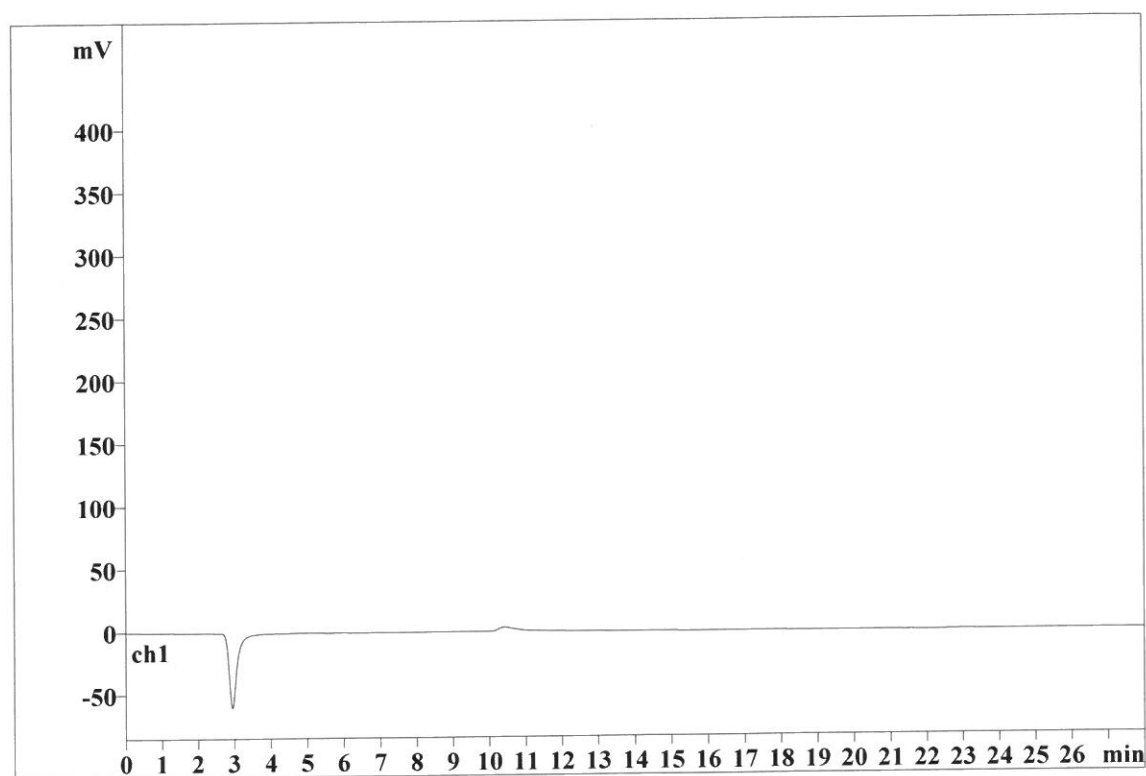

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 4/6/2018 6:26:01 PM
Printed by: wet


Ident: CCV
Analysis from: 3/15/2018 7:18:24 PM
File: _2018-03-15_

Last save: 3/15/2018 7:46:24 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16802

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 2
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

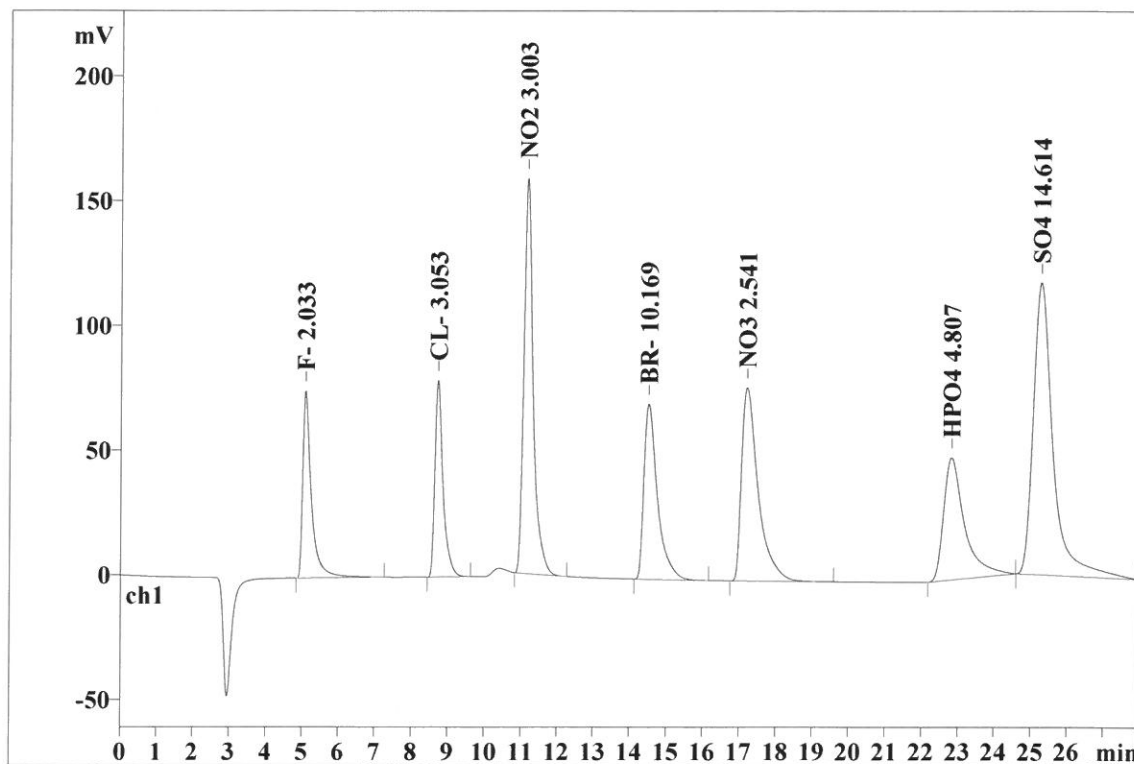

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.219	75.05	11.98	1238.728	7.77
2	8.72	0.221	78.90	12.60	1221.754	7.66
3	11.17	0.257	158.58	25.32	2849.734	17.88
4	14.51	0.367	70.25	11.22	1800.463	11.29
5	17.20	0.456	77.44	12.36	2452.084	15.38
6	22.81	0.556	49.01	7.82	1961.607	12.31
7	25.27	0.523	117.12	18.70	4416.067	27.70
7	28.00	0.371	626.35	100.00	15940.437	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/6/2018 6:26:08 PM
Printed by: wet


Ident: CCB
Analysis from: 3/15/2018 7:49:20 PM
File: _2018-03-15_

Last save: 3/15/2018 8:17:20 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16803

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 3
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

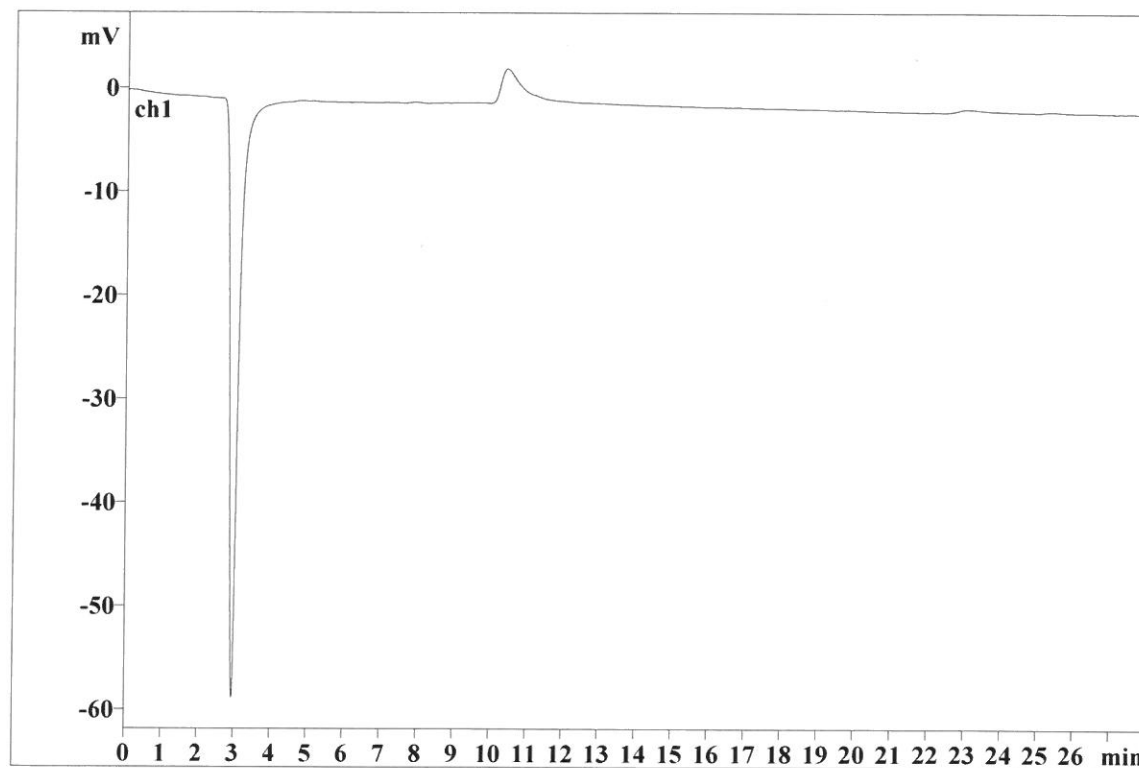

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 4/6/2018 6:26:13 PM
Printed by: wet


Ident: LB94460BLW
Analysis from: 3/15/2018 8:20:15 PM
File: _2018-03-15_

Last save: 4/6/2018 6:24:27 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16804

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 4
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

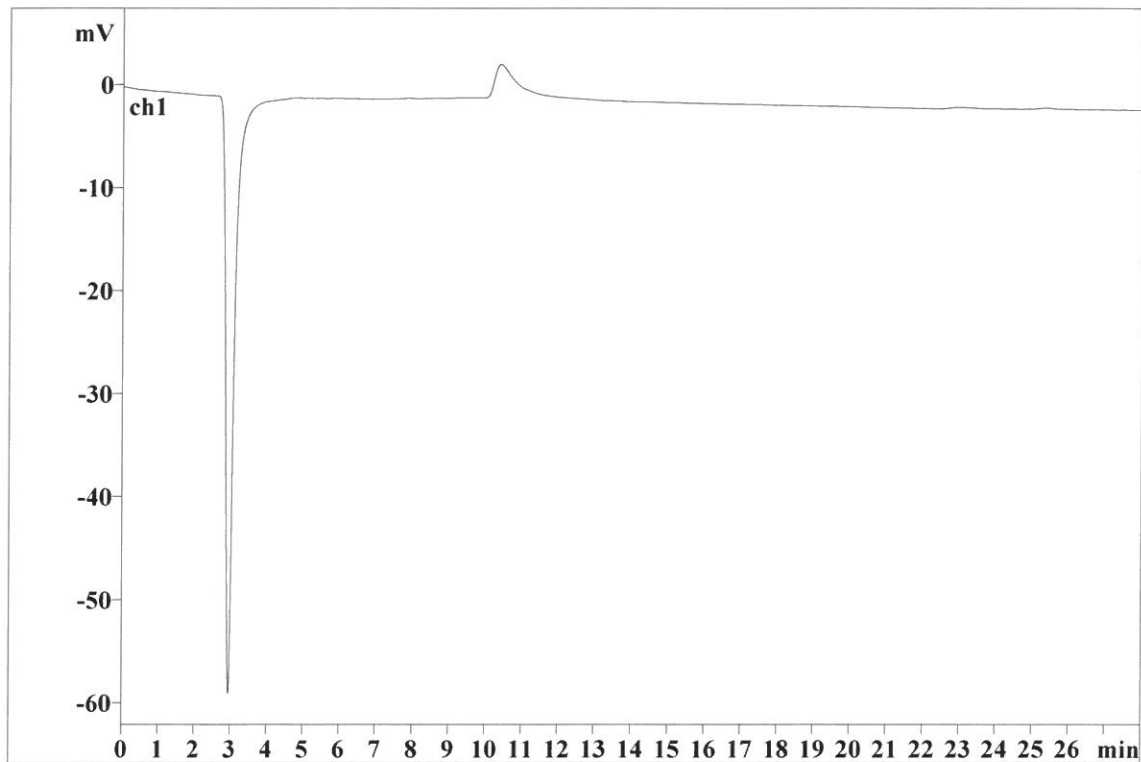

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD

Report date: 4/6/2018 6:26:19 PM
Printed by: wet


Ident: LB94460BSW
Analysis from: 3/15/2018 8:51:10 PM
File: _2018-03-15_

Last save: 4/6/2018 6:24:27 PM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16805

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 5
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

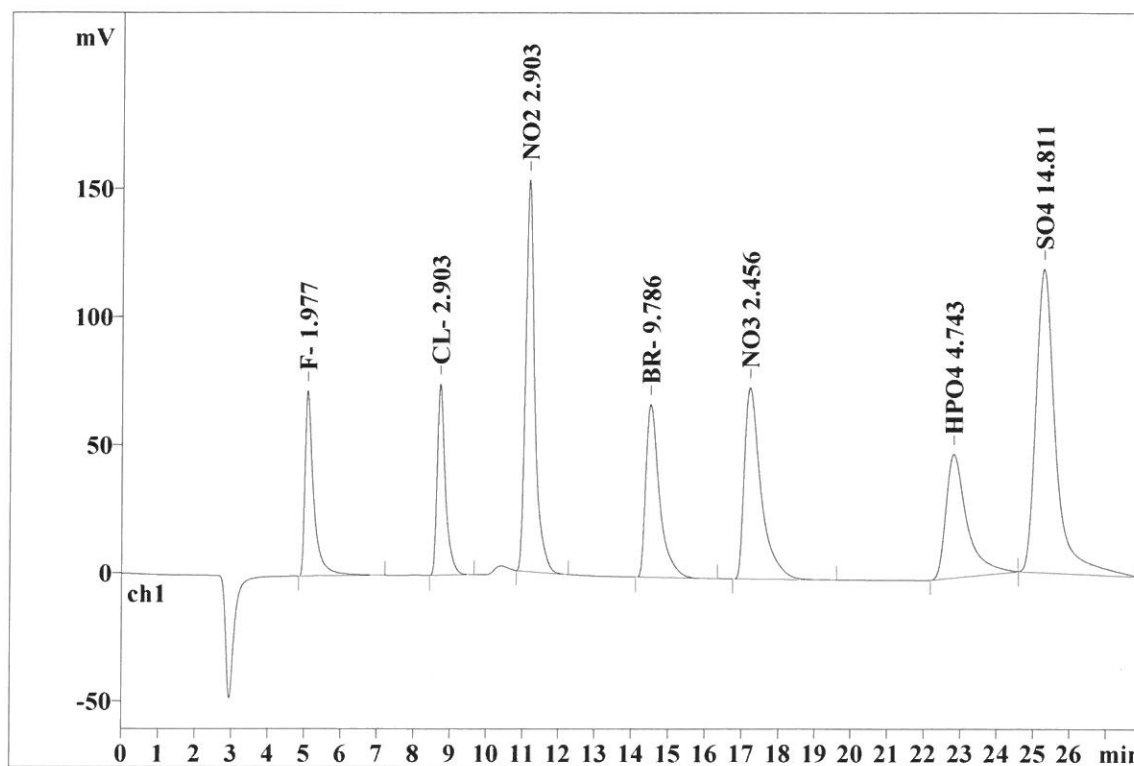

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.08	0.221	72.42	11.90	1204.164	7.70
2	8.72	0.222	74.55	12.25	1161.416	7.43
3	11.16	0.257	152.79	25.10	2753.204	17.61
4	14.51	0.367	67.46	11.08	1732.211	11.08
5	17.20	0.457	74.63	12.26	2369.382	15.15
6	22.80	0.558	48.30	7.93	1938.059	12.40
7	25.26	0.524	118.52	19.47	4476.502	28.63
7	28.00	0.373	608.66	100.00	15634.938	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/6/2018 6:26:27 PM
Printed by: wet


Ident: J1161-07
Analysis from: 3/16/2018 12:58:48 AM
File: _2018-03-16_

Last save: 3/16/2018 1:26:48 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16813

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 10
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

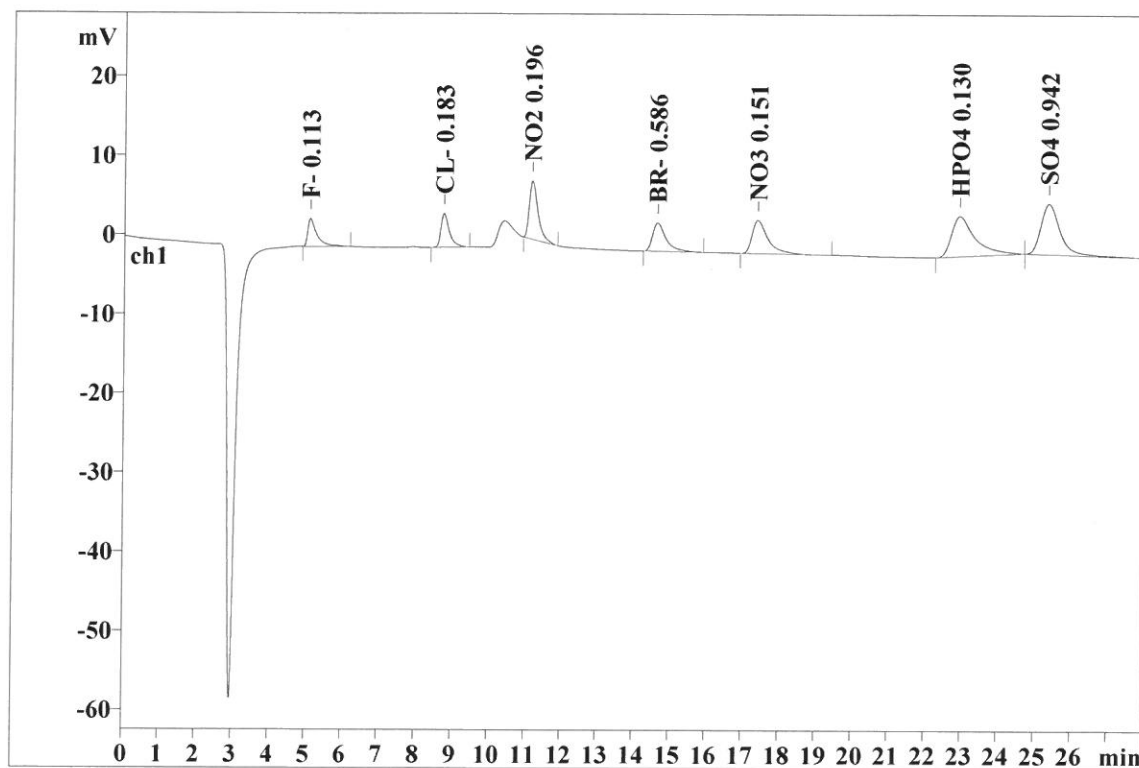

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.231	3.53	10.27	61.291	6.51
2	8.74	0.225	4.24	12.34	66.968	7.11
3	11.16	0.257	7.38	21.45	128.262	13.63
4	14.62	0.370	3.57	10.37	92.751	9.85
5	17.38	0.433	4.19	12.18	128.883	13.69
6	22.91	0.623	5.08	14.77	229.833	24.42
7	25.34	0.527	6.40	18.61	233.351	24.79
7	28.00	0.381	34.39	99.99	941.339	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/6/2018 6:26:33 PM
Printed by: wet


Ident: J1161-09
Analysis from: 3/16/2018 1:29:43 AM
File: _2018-03-16_

Last save: 3/16/2018 1:57:43 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16814

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 11
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

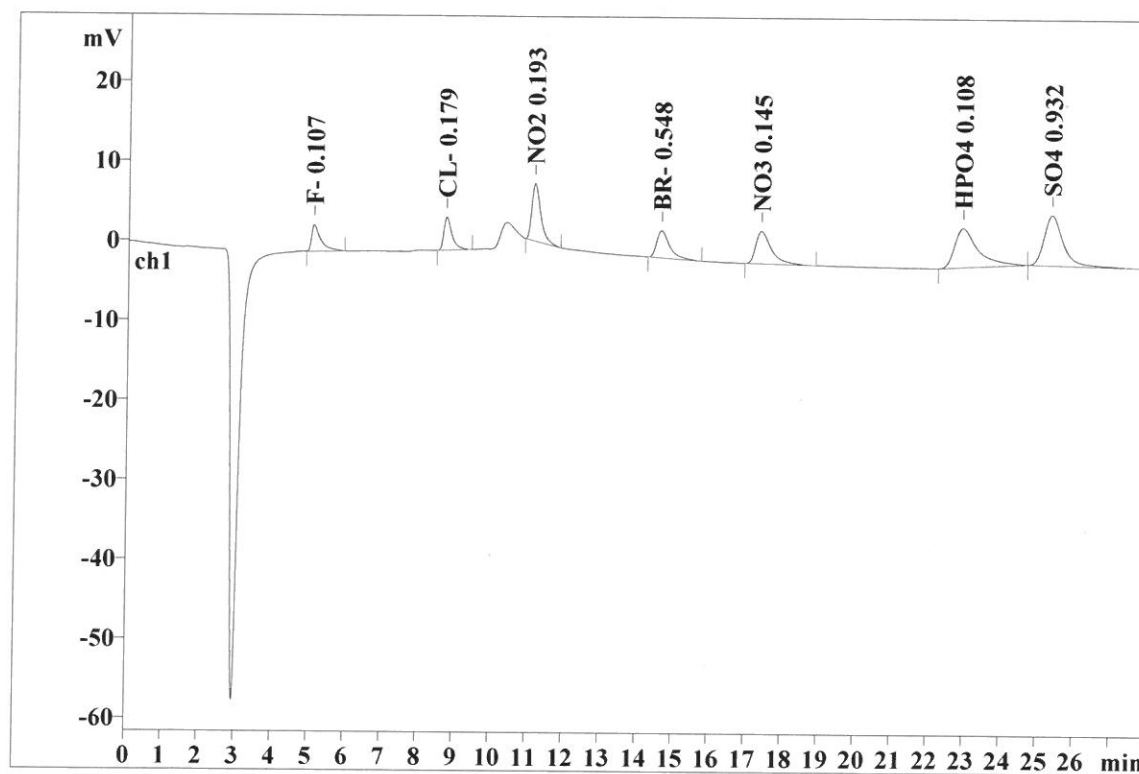

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.08	0.235	3.33	9.97	57.903	6.36
2	8.73	0.225	4.16	12.45	65.490	7.20
3	11.15	0.257	7.21	21.58	125.319	13.77
4	14.61	0.362	3.42	10.23	85.950	9.44
5	17.37	0.431	4.08	12.22	123.531	13.57
6	22.89	0.621	4.90	14.68	221.558	24.35
7	25.32	0.528	6.29	18.84	230.292	25.31
7	28.00	0.380	33.40	99.98	910.043	100.00

This report has been created by IC Net
METROHM LTD

Report date: 4/6/2018 6:26:39 PM
Printed by: wet


Ident: J1161-08
Analysis from: 3/16/2018 2:31:37 AM
File: _2018-03-16_

Last save: 3/16/2018 2:59:37 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16816

Last save: 3/12/2018 6:21:

SAMPLE:
: AK/AP
Vial number: 9
Volume: 20.0 µL
Dilution: 1.00
Amount: 1.0000

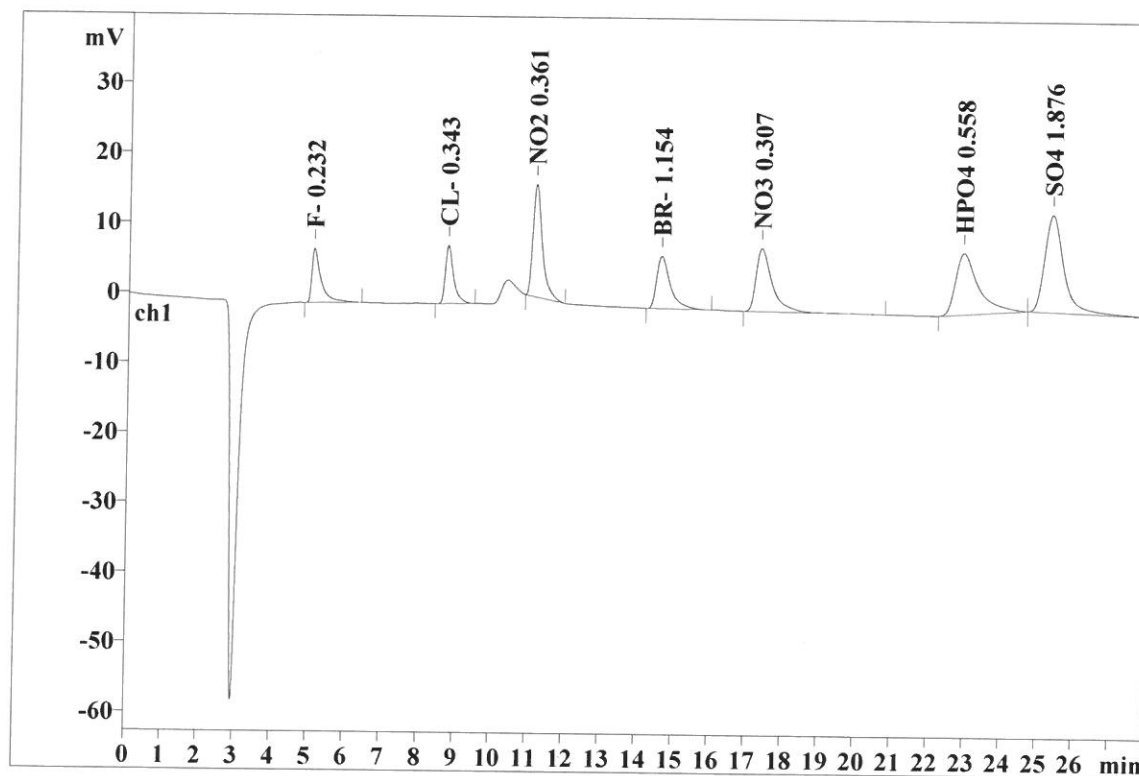

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.229	7.77	10.89	134.515	6.94
2	8.73	0.226	8.31	11.64	131.497	6.79
3	11.15	0.260	16.10	22.55	288.778	14.91
4	14.59	0.368	7.49	10.49	193.984	10.01
5	17.34	0.437	9.01	12.62	280.801	14.50
6	22.88	0.610	8.78	12.29	388.330	20.05
7	25.33	0.530	13.94	19.53	519.139	26.80
7	28.00	0.380	71.39	100.00	1937.043	100.00

This report has been created by IC Net
METROHM LTD


Report date: 4/6/2018 6:26:43 PM
 Printed by: wet
 Ident: CCV
 Analysis from: 3/16/2018 3:02:34 AM
 File: _2018-03-16_

Last save: 3/16/2018 3:30:34 AM

Method: AnionsIC2-031218.mtw
 Run operator: wet
 Analysis number: 16817

Last save: 3/12/2018 6:21:

SAMPLE:
 : AK/AP
 Vial number: 13
 Volume: 20.0 µL
 Dilution: 1.00
 Amount: 1.0000

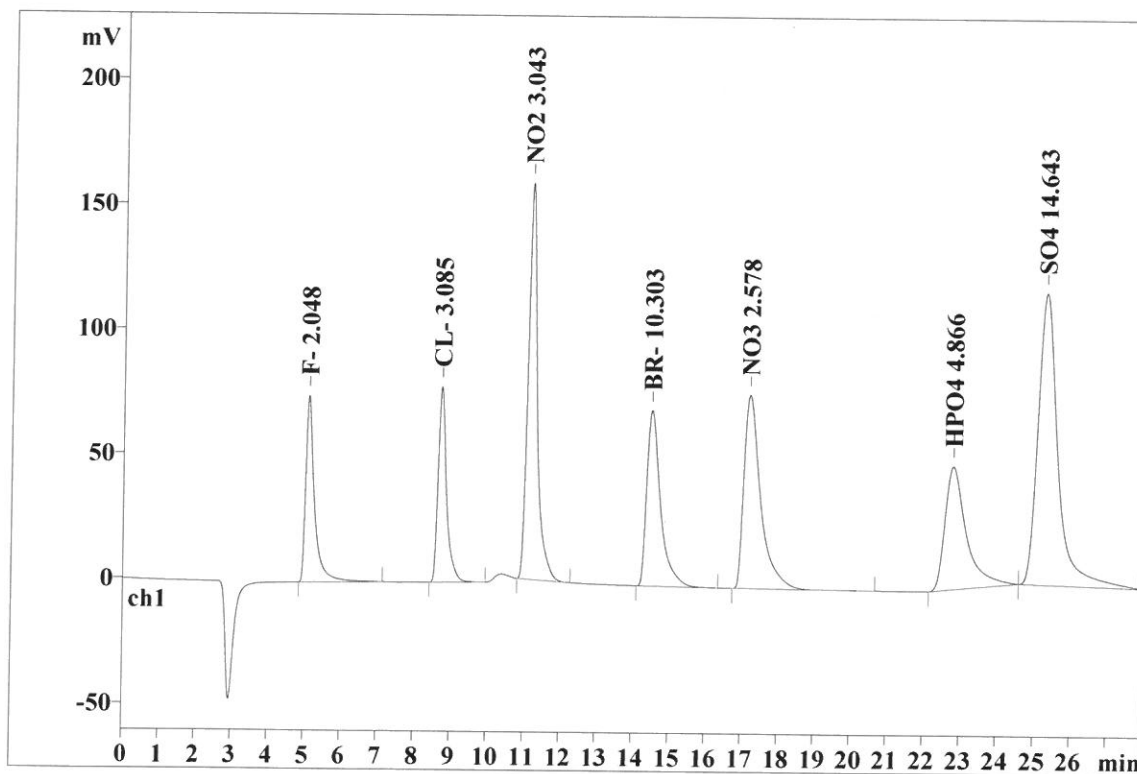

Quantitation method: Custom

No	Retention min	Width/2 min	Height mV	Height %	Area mV*sec	Area %
1	5.09	0.223	74.61	11.94	1247.676	7.75
2	8.72	0.224	78.18	12.51	1234.915	7.67
3	11.16	0.259	158.59	25.39	2888.800	17.95
4	14.50	0.370	70.19	11.24	1824.417	11.34
5	17.19	0.460	77.34	12.38	2487.251	15.46
6	22.79	0.563	49.12	7.86	1983.596	12.33
7	25.28	0.532	116.62	18.67	4425.104	27.50
7	28.00	0.376	624.66	100.00	16091.758	100.00

This report has been created by IC Net
 METROHM LTD

Report date: 4/6/2018 6:26:48 PM
Printed by: wet


Ident: CCB
Analysis from: 3/16/2018 3:33:29 AM
File: _2018-03-16_

Last save: 3/16/2018 4:01:29 AM

Method: AnionsIC2-031218.mtw
Run operator: wet
Analysis number: 16818

Last save: 3/12/2018 6:21:

SAMPLE:
:
Vial number: 14
Volume: 20.0 μ L
Dilution: 1.00
Amount: 1.0000

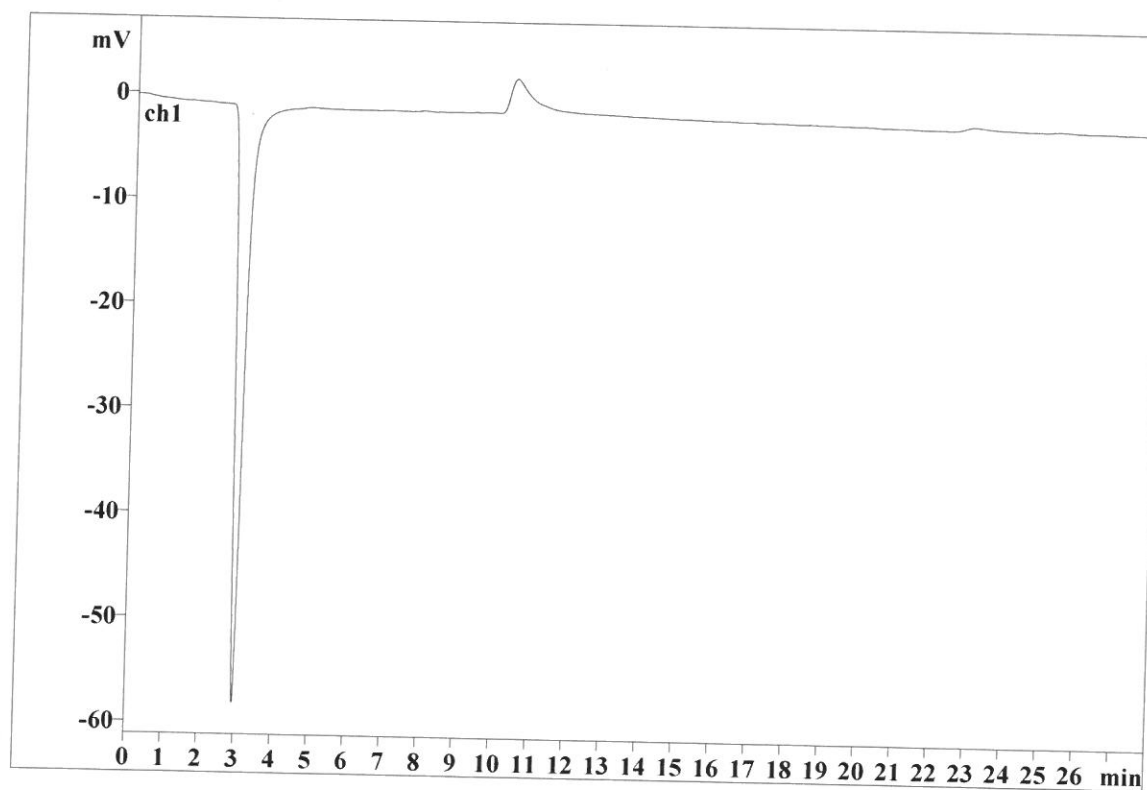

Quantitation method: Custom

No peaks

This report has been created by IC Net
METROHM LTD