

21396016

Test results

Aquakem 7.2AQ1

Page:

1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

6/14/2018 15:31

Test: ^{Reactive} ~~Total~~ CN Mg/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.296	0.0	0.091	
ICB1	-0.397	0.0	0.003	
CCV1	248.225	0.0	0.228	
CCB1	0.033	0.0	0.004	
PB110259BL	0.583	0.0	0.004	
J3490-04	0.645	0.0	0.004	
J3490-04DUP	1.495	0.0	0.005	
J3493-02	-0.545	0.0	0.003	
J3498-12	-0.696	0.0	0.003	
J3498-16	0.403	0.0	0.004	
J3501-04	0.022	0.0	0.004	
J3501-08	-0.110	0.0	0.004	
J3501-12	-0.097	0.0	0.004	
PB110258BL	1.177	0.0	0.005	
CCV2	245.221	0.0	0.225	
CCB2	-0.511	0.0	0.003	
J3469-02	0.320	0.0	0.004	
J3469-02DUP	-0.170	0.0	0.003	
J3485-08	0.065	0.0	0.004	
J3497-02	0.990	0.0	0.005	
CCV3	248.523	0.0	0.228	
CCB3	-0.080	0.0	0.004	
N	22			
Mean	38.245			
SD	87.4543			
CV%	228.67			

AS

Aquakem v. 7.2AQ1

Results from time period:

Thu Jun 14 15:14:41 2018

Thu Jun 14 15:22:26 2018

Sample Id	Sam/Ctr/c/	Test short nar	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.5677	µg/l	6/14/2018 10:10:45	
5.0PPBCN	A	Reactive CN	P	4.8148	µg/l	6/14/2018 10:10:46	
10PPBCN	A	Reactive CN	P	10.0883	µg/l	6/14/2018 10:10:47	
50PPBCN	A	Reactive CN	P	50.5474	µg/l	6/14/2018 10:10:48	
100PPBCN	A	Reactive CN	P	99.7078	µg/l	6/14/2018 10:10:49	
250PPBCN	A	Reactive CN	P	250.8113	µg/l	6/14/2018 10:10:50	
500PPBCN	A	Reactive CN	P	499.5981	µg/l	6/14/2018 10:10:51	
ICV1	S	Reactive CN	P	96.296	µg/l	6/14/2018 15:14:41	
ICB1	S	Reactive CN	P	-0.3967	µg/l	6/14/2018 15:14:42	
CCV1	S	Reactive CN	P	248.225	µg/l	6/14/2018 15:14:43	
CCB1	S	Reactive CN	P	0.0328	µg/l	6/14/2018 15:14:44	
PB110259BL	S	Reactive CN	P	0.5835	µg/l	6/14/2018 15:14:45	
J3490-04	S	Reactive CN	P	0.6451	µg/l	6/14/2018 15:14:46	
J3490-04DUP	S	Reactive CN	P	1.4952	µg/l	6/14/2018 15:14:47	
J3493-02	S	Reactive CN	P	-0.5449	µg/l	6/14/2018 15:14:48	
J3498-12	S	Reactive CN	P	-0.6957	µg/l	6/14/2018 15:14:49	
J3498-16	S	Reactive CN	P	0.4029	µg/l	6/14/2018 15:14:50	
J3501-04	S	Reactive CN	P	0.022	µg/l	6/14/2018 15:14:51	
J3501-08	S	Reactive CN	P	-0.1096	µg/l	6/14/2018 15:22:16	
J3501-12	S	Reactive CN	P	-0.0968	µg/l	6/14/2018 15:22:17	
PB110258BL	S	Reactive CN	P	1.1766	µg/l	6/14/2018 15:22:18	
CCV2	S	Reactive CN	P	245.2213	µg/l	6/14/2018 15:22:19	
CCB2	S	Reactive CN	P	-0.5113	µg/l	6/14/2018 15:22:20	
J3469-02	S	Reactive CN	P	0.3202	µg/l	6/14/2018 15:22:21	
J3469-02DUP	S	Reactive CN	P	-0.1703	µg/l	6/14/2018 15:22:22	
J3485-08	S	Reactive CN	P	0.065	µg/l	6/14/2018 15:22:23	
J3497-02	S	Reactive CN	P	0.9904	µg/l	6/14/2018 15:22:24	
CCV3	S	Reactive CN	P	248.5231	µg/l	6/14/2018 15:22:25	
CCB3	S	Reactive CN	P	-0.0802	µg/l	6/14/2018 15:22:26	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

6/14/2018 10:30


Test Total CN

Accepted 6/14/2018 10:30

Factor 1107
Bias 0.004

Coeff. of det. 0.999992

Errors

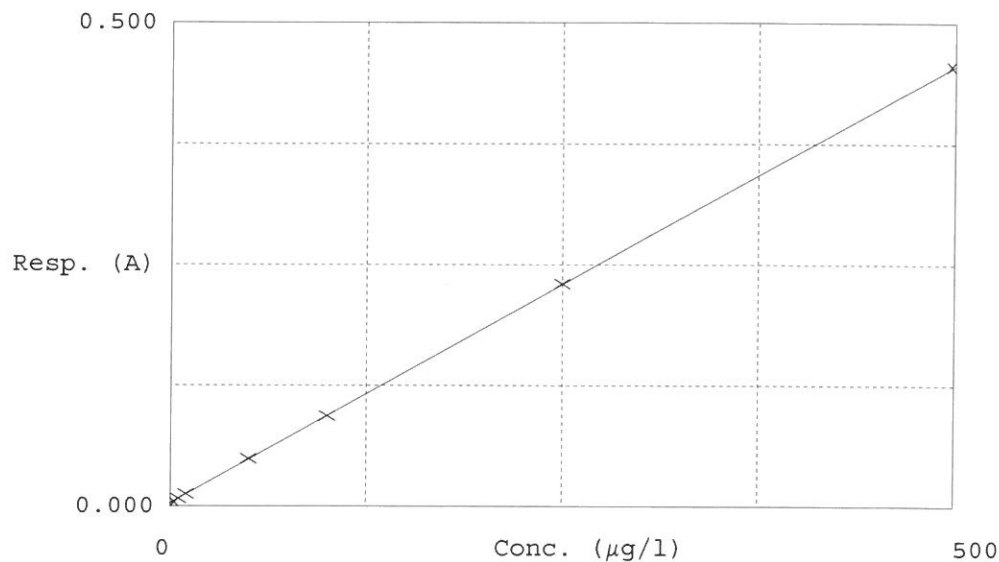

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.5677	0.0000	
2	5.0PPBCN	0.008	4.8148	5.0000	
3	10PPBCN	0.013	10.0883	10.0000	
4	50PPBCN	0.049	50.5474	50.0000	
5	100PPBCN	0.094	99.7078	100.0000	
6	250PPBCN	0.230	250.8113	250.0000	
7	500PPBCN	0.455	499.5981	500.0000	