

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

6/21/2018 12:07

Test: Total CN *Uyld*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	98.313	0.0	0.096	
ICB1	-0.041	0.0	0.004	
CCV1	242.404	0.0	0.230	
CCB1	0.157	0.0	0.004	
PB110470BL	-0.151	0.0	0.003	
J3246-04	-0.152	0.0	0.003	
J3246-04DUP	-0.303	0.0	0.003	
J3594-02	-0.403	0.0	0.003	
J3594-04	-0.270	0.0	0.003	
J3594-06	-0.294	0.0	0.003	
J3594-08	-0.448	0.0	0.003	
J3595-02	-0.163	0.0	0.003	
J3595-04	-0.028	0.0	0.004	
J3622-03	-0.507	0.0	0.003	
CCV2	249.200	0.0	0.237	
CCB2	0.349	0.0	0.004	
J3622-07	-0.051	0.0	0.004	
J3622-11	-0.829	0.0	0.003	
J3622-15	-0.315	0.0	0.003	
J3622-19	-0.117	0.0	0.004	
PB110471BL	-0.248	0.0	0.003	
J3627-36	-0.107	0.0	0.004	
J3627-36DUP	0.709	0.0	0.004	
CCV3	261.948	0.0	0.249	
CCB3	-0.319	0.0	0.003	

N	25
Mean	33.933
SD	84.2513
CV%	248.28

Aquakem v. 7.2AQ1

AS

Results from time period:

Thu Jun 21 10:00:01 2018

Thu Jun 21 11:41:55 2018

Sample Id	Sam/Ctr/c/	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.6597	µg/l	6/21/2018 10:00:01	
5.OPPBCN	A	Reactive CN	P	4.5005	µg/l	6/21/2018 10:00:02	
10PPBCN	A	Reactive CN	P	9.8349	µg/l	6/21/2018 10:00:03	
50PPBCN	A	Reactive CN	P	49.6711	µg/l	6/21/2018 10:00:04	
100PPBCN	A	Reactive CN	P	100.233	µg/l	6/21/2018 10:00:05	
250PPBCN	A	Reactive CN	P	252.8513	µg/l	6/21/2018 10:00:06	
500PPBCN	A	Reactive CN	P	498.569	µg/l	6/21/2018 10:00:07	
ICV1	S	Reactive CN	P	98.3135	µg/l	6/21/2018 11:30:27	
ICB1	S	Reactive CN	P	-0.0409	µg/l	6/21/2018 11:30:28	
CCV1	S	Reactive CN	P	242.4044	µg/l	6/21/2018 11:30:29	
CCB1	S	Reactive CN	P	0.1566	µg/l	6/21/2018 11:30:30	
PB110470BL	S	Reactive CN	P	-0.1511	µg/l	6/21/2018 11:30:31	
J3246-04	S	Reactive CN	P	-0.152	µg/l	6/21/2018 11:30:32	
J3246-04DUP	S	Reactive CN	P	-0.3025	µg/l	6/21/2018 11:30:33	
J3594-02	S	Reactive CN	P	-0.4034	µg/l	6/21/2018 11:30:34	
J3594-04	S	Reactive CN	P	-0.2698	µg/l	6/21/2018 11:30:35	
J3594-06	S	Reactive CN	P	-0.2944	µg/l	6/21/2018 11:30:36	
J3594-08	S	Reactive CN	P	-0.4479	µg/l	6/21/2018 11:30:37	
J3595-02	S	Reactive CN	P	-0.1631	µg/l	6/21/2018 11:38:02	
J3595-04	S	Reactive CN	P	-0.0282	µg/l	6/21/2018 11:38:03	
J3622-03	S	Reactive CN	P	-0.5072	µg/l	6/21/2018 11:38:04	
CCV2	S	Reactive CN	P	249.2001	µg/l	6/21/2018 11:38:05	
CCB2	S	Reactive CN	P	0.3493	µg/l	6/21/2018 11:38:06	
J3622-07	S	Reactive CN	P	-0.0506	µg/l	6/21/2018 11:38:07	
J3622-11	S	Reactive CN	P	-0.8289	µg/l	6/21/2018 11:38:08	
J3622-15	S	Reactive CN	P	-0.3153	µg/l	6/21/2018 11:38:09	
J3622-19	S	Reactive CN	P	-0.1174	µg/l	6/21/2018 11:38:10	
PB110471BL	S	Reactive CN	P	-0.2479	µg/l	6/21/2018 11:38:11	
J3627-36	S	Reactive CN	P	-0.1072	µg/l	6/21/2018 11:38:12	
J3627-36DUP	S	Reactive CN	P	0.7092	µg/l	6/21/2018 11:41:53	
CCV3	S	Reactive CN	P	261.9483	µg/l	6/21/2018 11:41:54	
CCB3	S	Reactive CN	P	-0.3195	µg/l	6/21/2018 11:41:55	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

6/21/2018 10:00


Test Total CN

Accepted 6/21/2018 10:00

Factor 1069
Bias 0.004

Coeff. of det. 0.999946

Errors

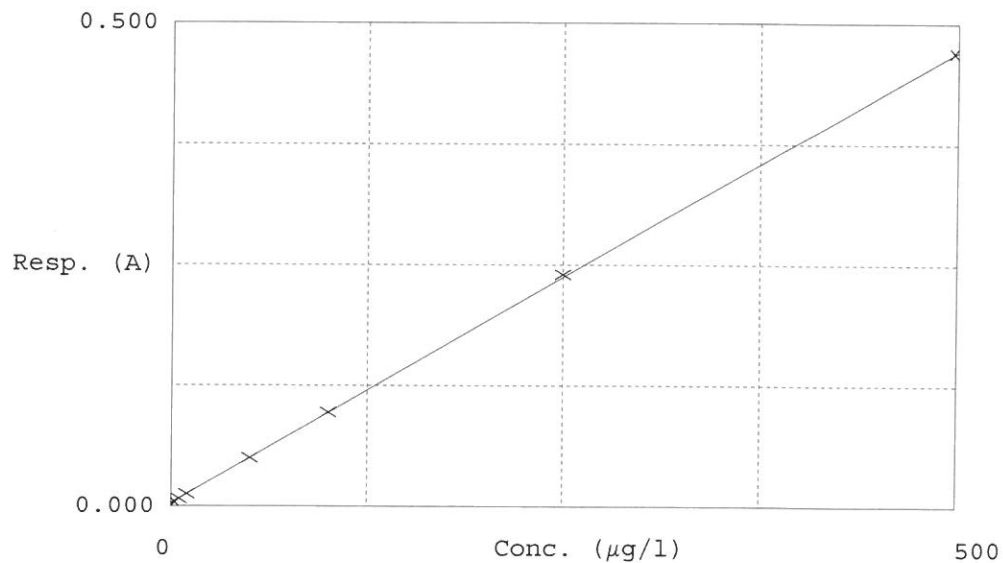

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.6597	0.0000	
2	5.0PPBCN	0.008	4.5005	5.0000	
3	10PPBCN	0.013	9.8349	10.0000	
4	50PPBCN	0.050	49.6711	50.0000	
5	100PPBCN	0.097	100.2330	100.0000	
6	250PPBCN	0.240	252.8513	250.0000	
7	500PPBCN	0.470	498.5690	500.0000	