

LB96247

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

6/25/2018 14:18

Test: ^{Reactive} ~~Total~~ CN ^{ug/d}

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.321	0.0	0.095	
ICB1	-0.184	0.0	0.003	
CCV1	243.876	0.0	0.238	
CCB1	-0.156	0.0	0.003	
PB110545BL	-0.108	0.0	0.003	
J3240-06	-0.085	0.0	0.003	
J3240-06DUP	-0.212	0.0	0.003	
J3241-14	-0.018	0.0	0.003	
J3241-16	-0.112	0.0	0.003	
J3214-18	-0.498	0.0	0.003	
J3667-02	-0.586	0.0	0.003	
J3676-04	-0.331	0.0	0.003	
J3676-08	0.149	0.0	0.004	
J3676-12	0.130	0.0	0.004	
CCV2	245.857	0.0	0.240	
CCB2	-0.210	0.0	0.003	
J3684-04	0.120	0.0	0.004	
J3684-08	-0.707	0.0	0.003	
J3684-11	-0.125	0.0	0.003	
PB110546BL	0.035	0.0	0.004	
J3692-01	-0.023	0.0	0.003	
J3692-01DUP	-0.034	0.0	0.003	
CCV3	250.559	0.0	0.244	
CCB3	0.073	0.0	0.004	

N	24
Mean	34.697
SD	84.1569
CV%	242.55

AS
06/25/18
J3241-18

AS

Aquakem v. 7.2AQ1

Results from time period:

Mon Jun 25 10:20:45 2018

Mon Jun 25 14:17:45 2018

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.2682	µg/l	6/25/2018 10:20:45	
5.OPPBCN	A	Reactive CN	P	4.2126	µg/l	6/25/2018 10:20:46	
10PPBCN	A	Reactive CN	P	9.9635	µg/l	6/25/2018 10:20:47	
50PPBCN	A	Reactive CN	P	49.9478	µg/l	6/25/2018 10:20:48	
100PPBCN	A	Reactive CN	P	100.395	µg/l	6/25/2018 10:20:49	
250PPBCN	A	Reactive CN	P	251.6288	µg/l	6/25/2018 10:20:50	
500PPBCN	A	Reactive CN	P	499.1204	µg/l	6/25/2018 10:20:51	
ICV1	S	Reactive CN	P	95.3206	µg/l	6/25/2018 13:47:44	
ICB1	S	Reactive CN	P	-0.1842	µg/l	6/25/2018 13:47:45	
CCV1	S	Reactive CN	P	243.8755	µg/l	6/25/2018 13:47:46	
CCB1	S	Reactive CN	P	-0.1563	µg/l	6/25/2018 13:47:47	
PB110545BL	S	Reactive CN	P	-0.1083	µg/l	6/25/2018 13:47:48	
J3240-06	S	Reactive CN	P	-0.0846	µg/l	6/25/2018 13:47:49	
J3240-06DUP	S	Reactive CN	P	-0.2125	µg/l	6/25/2018 13:47:50	
J3241-14	S	Reactive CN	P	-0.0178	µg/l	6/25/2018 13:47:51	
J3241-16	S	Reactive CN	P	-0.1118	µg/l	6/25/2018 13:47:52	
J3214-18	S	Reactive CN	P	-0.4978	µg/l	6/25/2018 13:47:53	
J3667-02	S	Reactive CN	P	-0.5862	µg/l	6/25/2018 13:47:54	
J3676-04	S	Reactive CN	P	-0.3308	µg/l	6/25/2018 13:55:19	
J3676-08	S	Reactive CN	P	0.1488	µg/l	6/25/2018 13:55:20	
J3676-12	S	Reactive CN	P	0.1298	µg/l	6/25/2018 13:55:21	
CCV2	S	Reactive CN	P	245.8565	µg/l	6/25/2018 14:17:36	
CCB2	S	Reactive CN	P	-0.2096	µg/l	6/25/2018 14:17:37	
J3684-04	S	Reactive CN	P	0.1202	µg/l	6/25/2018 14:17:38	
J3684-08	S	Reactive CN	P	-0.7067	µg/l	6/25/2018 14:17:39	
J3684-11	S	Reactive CN	P	-0.125	µg/l	6/25/2018 14:17:40	
PB110546BL	S	Reactive CN	P	0.0351	µg/l	6/25/2018 14:17:41	
J3692-01	S	Reactive CN	P	-0.0225	µg/l	6/25/2018 14:17:42	
J3692-01DUP	S	Reactive CN	P	-0.0342	µg/l	6/25/2018 14:17:43	
CCV3	S	Reactive CN	P	250.559	µg/l	6/25/2018 14:17:44	
CCB3	S	Reactive CN	P	0.0727	µg/l	6/25/2018 14:17:45	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

6/25/2018 10:21


Test Total CN

Accepted 6/25/2018 10:21

Factor 1042
Bias 0.003

Coeff. of det. 0.999979

Errors

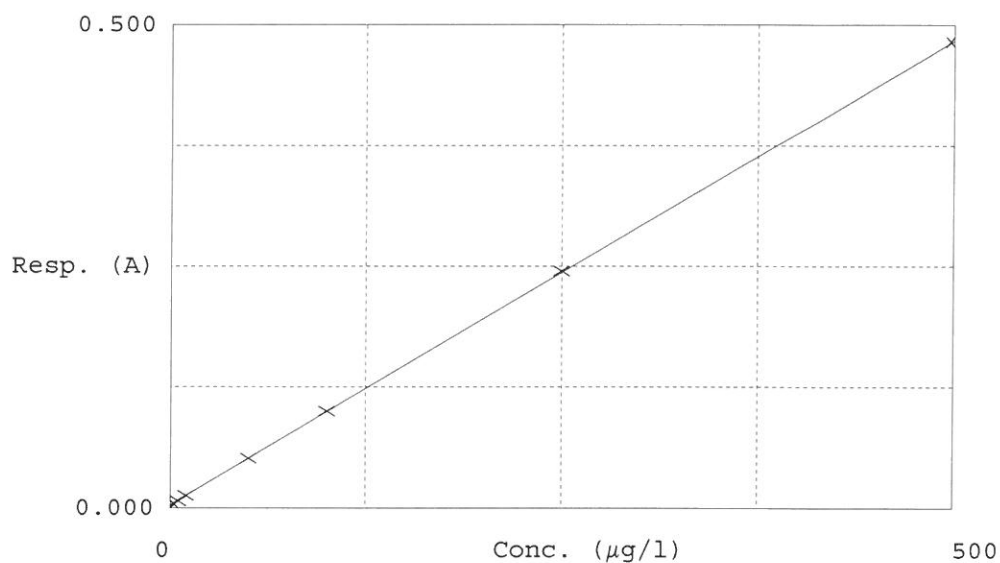

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.2682	0.0000	
2	5.0PPBCN	0.008	4.2126	5.0000	
3	10PPBCN	0.013	9.9635	10.0000	
4	50PPBCN	0.051	49.9478	50.0000	
5	100PPBCN	0.100	100.3950	100.0000	
6	250PPBCN	0.245	251.6288	250.0000	
7	500PPBCN	0.483	499.1204	500.0000	