

LB96270

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

6/26/2018 13:14

Test: ^{Reactive} ~~Total~~ CN _{ug/L}

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.838	0.0	0.095	
ICB1	1.111	0.0	0.004	
CCV1	241.593	0.0	0.233	
CCB1	1.116	0.0	0.004	
PB110609BL	1.342	0.0	0.004	
J3251-06	0.957	0.0	0.004	
J3251-06DUP	1.199	0.0	0.004	
J3677-13	1.173	0.0	0.004	
J3702-02	0.983	0.0	0.004	
J3706-04	1.163	0.0	0.004	
CCV2	243.565	0.0	0.235	
CCB2	1.075	0.0	0.004	

N 12
Mean 49.343
SD 94.3223
CV% 191.16

AS

Aquakem v. 7.2AQ1

Results from time period:

Tue Jun 26 13:05:50 2018

Tue Jun 26 13:08:38 2018

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	0.2968	µg/l	6/26/2018 8:34:28	
5.OPPBCN	A	Reactive CN	P	5.6593	µg/l	6/26/2018 8:34:29	
10PPBCN	A	Reactive CN	P	10.3417	µg/l	6/26/2018 8:34:30	
50PPBCN	A	Reactive CN	P	50.5843	µg/l	6/26/2018 8:34:31	
100PPBCN	A	Reactive CN	P	99.9319	µg/l	6/26/2018 8:34:32	
250PPBCN	A	Reactive CN	P	246.4886	µg/l	6/26/2018 8:34:33	
500PPBCN	A	Reactive CN	P	501.6974	µg/l	6/26/2018 8:34:34	
ICV1	S	Reactive CN	P	96.8383	µg/l	6/26/2018 13:05:50	
ICB1	S	Reactive CN	P	1.1115	µg/l	6/26/2018 13:05:51	
CCV1	S	Reactive CN	P	241.5935	µg/l	6/26/2018 13:05:52	
CCB1	S	Reactive CN	P	1.1164	µg/l	6/26/2018 13:05:53	
PB110609BL	S	Reactive CN	P	1.3417	µg/l	6/26/2018 13:05:54	
J3251-06	S	Reactive CN	P	0.9566	µg/l	6/26/2018 13:05:55	
J3251-06DUP	S	Reactive CN	P	1.1992	µg/l	6/26/2018 13:05:56	
J3677-13	S	Reactive CN	P	1.1735	µg/l	6/26/2018 13:05:57	
J3702-02	S	Reactive CN	P	0.9826	µg/l	6/26/2018 13:05:58	
J3706-04	S	Reactive CN	P	1.1627	µg/l	6/26/2018 13:05:59	
CCV2	S	Reactive CN	P	243.5652	µg/l	6/26/2018 13:06:00	
CCB2	S	Reactive CN	P	1.0748	µg/l	6/26/2018 13:08:38	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

6/26/2018 8:34


Test Total CN

Accepted 6/26/2018 8:34

Factor 1049
Bias 0.003

Coeff. of det. 0.999921

Errors

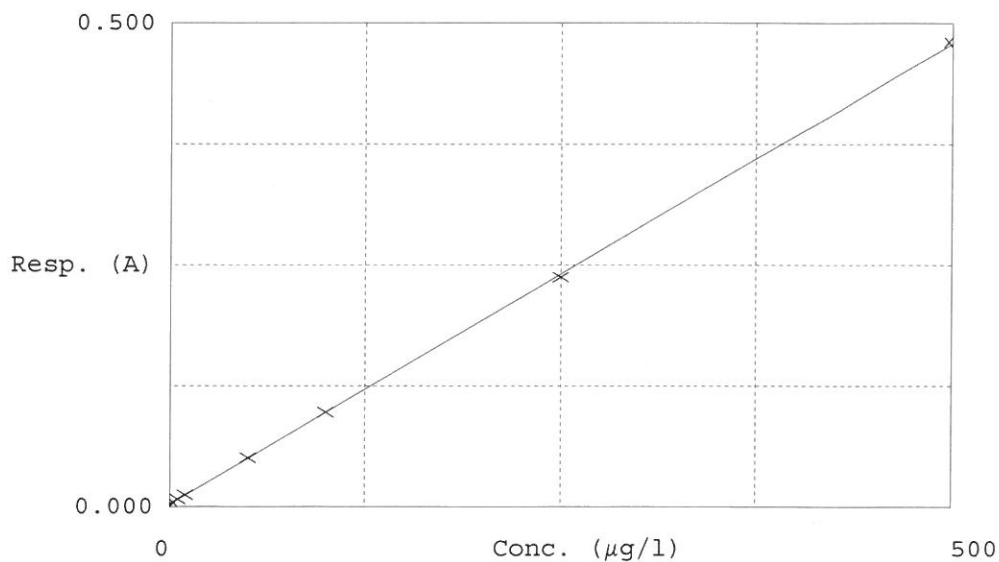

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.2968	0.0000	
2	5.0PPBCN	0.008	5.6593	5.0000	
3	10PPBCN	0.012	10.3417	10.0000	
4	50PPBCN	0.051	50.5843	50.0000	
5	100PPBCN	0.098	99.9319	100.0000	
6	250PPBCN	0.238	246.4886	250.0000	
7	500PPBCN	0.481	501.6974	500.0000	