

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

7/3/2018 10:02

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.268	0.0	0.097	
ICB1	0.333	0.0	0.004	
CCV1	243.083	0.0	0.238	
CCB1	0.054	0.0	0.004	
PB110770BL	-0.627	0.0	0.003	
J3243-06	-0.284	0.0	0.003	
J3243-06DUP	0.099	0.0	0.004	
J3245-18	-0.440	0.0	0.003	
J3245-20	-0.016	0.0	0.004	
J3245-22	-0.664	0.0	0.003	
J3245-24	-0.469	0.0	0.003	
J3248-08	-0.577	0.0	0.003	
J3248-10	-0.122	0.0	0.003	
J3248-12	0.313	0.0	0.004	
CCV2	245.328	0.0	0.240	
CCB2	0.193	0.0	0.004	
J3252-06	-0.210	0.0	0.003	
J3771-02	0.035	0.0	0.004	
J3790-01	0.031	0.0	0.004	
J3796-02	-0.650	0.0	0.003	
PB110771BL	-0.369	0.0	0.003	
J3790-03	-0.442	0.0	0.003	
J3790-03DUP	-0.074	0.0	0.004	
J3798-02	-0.373	0.0	0.003	
J3798-05	-0.295	0.0	0.003	
J3798-08	-0.245	0.0	0.003	
CCV3	254.719	0.0	0.249	
CCB3	-0.258	0.0	0.003	

N	28
Mean	29.833
SD	79.0452
CV%	264.95

LB96404

AK

Aquakem v. 7.2AQ1

Results from time period:

Tue Jul 03 08:33:08 2018

Tue Jul 03 09:59:34 2018

Sample Id	Sam/Ctr/c	Test short	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive	Cl P	-0.3316	µg/l	7/3/2018 9:07:26	
5.0PPBCN	A	Reactive	Cl P	4.3018	µg/l	7/3/2018 9:07:27	
10PPBCN	A	Reactive	Cl P	9.8691	µg/l	7/3/2018 9:07:28	
50PPBCN	A	Reactive	Cl P	50.1003	µg/l	7/3/2018 9:07:29	
100PPBCN	A	Reactive	Cl P	100.442	µg/l	7/3/2018 9:07:30	
250PPBCN	A	Reactive	Cl P	251.4144	µg/l	7/3/2018 9:07:31	
500PPBCN	A	Reactive	Cl P	499.2039	µg/l	7/3/2018 9:07:32	
ICV1	S	Reactive	Cl P	97.2682	µg/l	7/3/2018 9:46:41	
ICB1	S	Reactive	Cl P	0.3327	µg/l	7/3/2018 9:46:42	
CCV1	S	Reactive	Cl P	243.0825	µg/l	7/3/2018 9:46:43	
CCB1	S	Reactive	Cl P	0.0537	µg/l	7/3/2018 9:46:44	
PB110770BL	S	Reactive	Cl P	-0.6271	µg/l	7/3/2018 9:46:45	
J3243-06	S	Reactive	Cl P	-0.2845	µg/l	7/3/2018 9:46:46	
J3243-06DUP	S	Reactive	Cl P	0.0995	µg/l	7/3/2018 9:46:47	
J3245-18	S	Reactive	Cl P	-0.4405	µg/l	7/3/2018 9:46:48	
J3245-20	S	Reactive	Cl P	-0.0163	µg/l	7/3/2018 9:46:49	
J3245-22	S	Reactive	Cl P	-0.6638	µg/l	7/3/2018 9:46:50	
J3245-24	S	Reactive	Cl P	-0.4687	µg/l	7/3/2018 9:46:51	
J3248-08	S	Reactive	Cl P	-0.5774	µg/l	7/3/2018 9:54:14	
J3248-10	S	Reactive	Cl P	-0.122	µg/l	7/3/2018 9:54:15	
J3248-12	S	Reactive	Cl P	0.3127	µg/l	7/3/2018 9:54:16	
CCV2	S	Reactive	Cl P	245.3283	µg/l	7/3/2018 9:54:17	
CCB2	S	Reactive	Cl P	0.1931	µg/l	7/3/2018 9:54:18	
J3252-06	S	Reactive	Cl P	-0.2097	µg/l	7/3/2018 9:54:19	
J3771-02	S	Reactive	Cl P	0.0352	µg/l	7/3/2018 9:54:20	
J3790-01	S	Reactive	Cl P	0.0306	µg/l	7/3/2018 9:54:21	
J3796-02	S	Reactive	Cl P	-0.6496	µg/l	7/3/2018 9:54:22	
PB110771BL	S	Reactive	Cl P	-0.3693	µg/l	7/3/2018 9:54:23	
J3790-03	S	Reactive	Cl P	-0.4425	µg/l	7/3/2018 9:54:24	
J3790-03DUP	S	Reactive	Cl P	-0.0743	µg/l	7/3/2018 9:59:29	
J3798-02	S	Reactive	Cl P	-0.3728	µg/l	7/3/2018 9:59:30	
J3798-05	S	Reactive	Cl P	-0.2953	µg/l	7/3/2018 9:59:31	
J3798-08	S	Reactive	Cl P	-0.2453	µg/l	7/3/2018 9:59:32	
CCV3	S	Reactive	Cl P	254.7188	µg/l	7/3/2018 9:59:33	
CCB3	S	Reactive	Cl P	-0.2584	µg/l	7/3/2018 9:59:34	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

7/3/2018 9:12


Test Total CN

Accepted 7/3/2018 9:12

Factor 1037
Bias 0.004

Coeff. of det. 0.999983

Errors

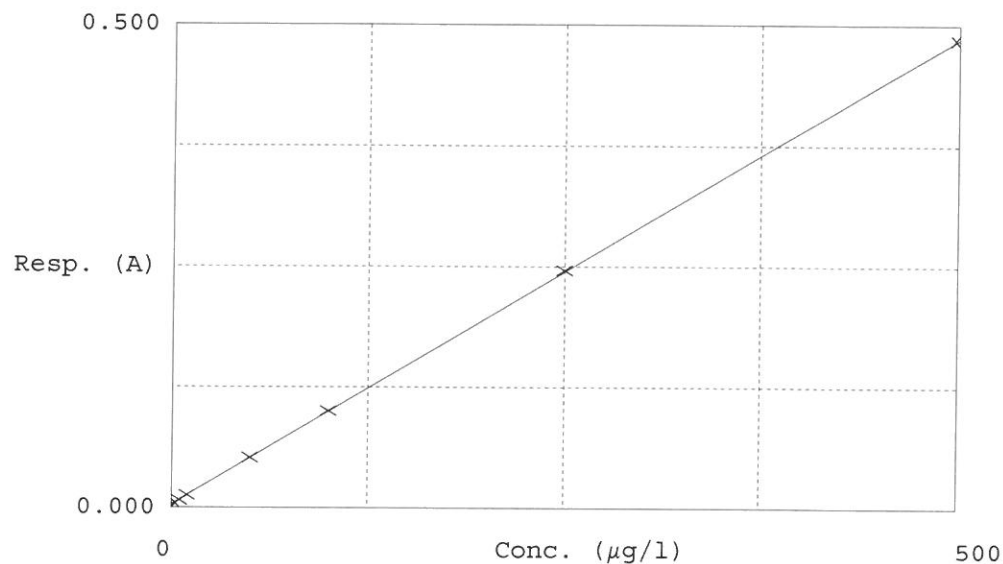

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.3316	0.0000	
2	5.0PPBCN	0.008	4.3018	5.0000	
3	10PPBCN	0.013	9.8691	10.0000	
4	50PPBCN	0.052	50.1003	50.0000	
5	100PPBCN	0.100	100.4420	100.0000	
6	250PPBCN	0.246	251.4144	250.0000	
7	500PPBCN	0.485	499.2039	500.0000	