

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : WJ

7/13/2018 15:16

Test: *Acetate*
~~Total~~ CN *ug/l*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.993	0.0	0.090	
ICB1	0.064	0.0	0.004	
CCV1	239.427	0.0	0.222	
CCB1	0.071	0.0	0.004	
PB111107BL	-0.571	0.0	0.003	
J3545-06	-0.261	0.0	0.003	
J3545-06DUP	-0.466	0.0	0.003	
J3954-02	-0.503	0.0	0.003	
J3959-02	-0.269	0.0	0.003	
J3964-02	-0.136	0.0	0.004	
J3975-14	-0.370	0.0	0.003	
CCV2	255.695	0.0	0.237	
CCB2	0.002	0.0	0.004	

N 13
Mean 45.206
SD 93.6144
CV% 207.09

AS

Aquakem v. 7.2AQ1

Results from time period:

Fri Jul 13 15:13:14 2018

Fri Jul 13 15:16:38 2018

Sample Id	Sam/Ctr/c/	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.3874	µg/l	7/13/2018 10:37:53	
5.0PPBCN	A	Reactive CN	P	4.5807	µg/l	7/13/2018 10:37:54	
10PPBCN	A	Reactive CN	P	9.5382	µg/l	7/13/2018 10:37:55	
50PPBCN	A	Reactive CN	P	50.8747	µg/l	7/13/2018 10:37:56	
100PPBCN	A	Reactive CN	P	99.9885	µg/l	7/13/2018 10:37:57	
250PPBCN	A	Reactive CN	P	250.9542	µg/l	7/13/2018 10:37:58	
500PPBCN	A	Reactive CN	P	499.4512	µg/l	7/13/2018 10:37:59	
ICV1	S	Reactive CN	P	94.9926	µg/l	7/13/2018 15:13:14	
ICB1	S	Reactive CN	P	0.0642	µg/l	7/13/2018 15:13:15	
CCV1	S	Reactive CN	P	239.427	µg/l	7/13/2018 15:13:16	
CCB1	S	Reactive CN	P	0.0705	µg/l	7/13/2018 15:13:17	
PB111107BL	S	Reactive CN	P	-0.5713	µg/l	7/13/2018 15:13:18	
J3545-06	S	Reactive CN	P	-0.2613	µg/l	7/13/2018 15:13:19	
J3545-06DUP	S	Reactive CN	P	-0.4665	µg/l	7/13/2018 15:13:20	
J3954-02	S	Reactive CN	P	-0.5034	µg/l	7/13/2018 15:13:21	
J3959-02	S	Reactive CN	P	-0.2688	µg/l	7/13/2018 15:13:22	
J3964-02	S	Reactive CN	P	-0.1362	µg/l	7/13/2018 15:13:23	
J3975-14	S	Reactive CN	P	-0.3699	µg/l	7/13/2018 15:13:24	
CCV2	S	Reactive CN	P	255.6952	µg/l	7/13/2018 15:16:37	
CCB2	S	Reactive CN	P	0.0023	µg/l	7/13/2018 15:16:38	


Test Total CN

Accepted 7/13/2018 10:38

Factor 1097
Bias 0.004

Coeff. of det. 0.999988

Errors

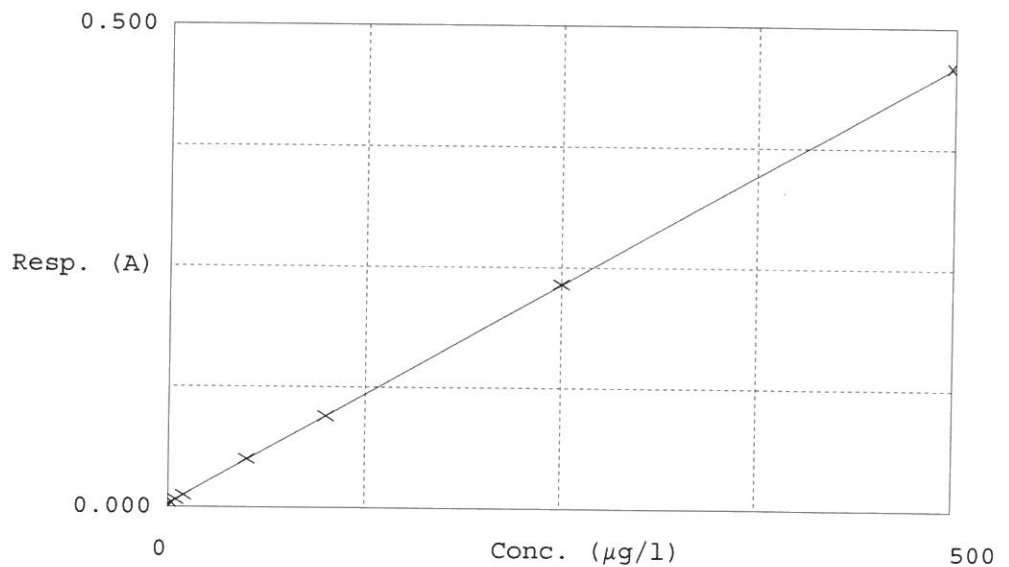

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.3874	0.0000	
2	5.0PPBCN	0.008	4.5807	5.0000	
3	10PPBCN	0.012	9.5382	10.0000	
4	50PPBCN	0.050	50.8747	50.0000	
5	100PPBCN	0.095	99.9885	100.0000	
6	250PPBCN	0.232	250.9542	250.0000	
7	500PPBCN	0.459	499.4512	500.0000	