

2B97153

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

8/7/2018 14:10

Test: ^{Reactive} Total CN ^{Mg/d}

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.659	0.0	0.094	
ICB1	0.681	0.0	0.004	
CCV1	241.320	0.0	0.227	
CCB1	0.156	0.0	0.004	
PB111832BL	0.019	0.0	0.004	
J4360-03	-0.236	0.0	0.003	
J4360-03DUP	-0.249	0.0	0.003	
J4360-06	-0.368	0.0	0.003	
PB111833BL	-0.334	0.0	0.003	
J4366-02	0.273	0.0	0.004	
J4366-02DUP	0.057	0.0	0.004	
CCV2	259.798	0.0	0.244	
CCB2	-0.026	0.0	0.004	

N	13
Mean	46.058
SD	94.7327
CV%	205.68

AS

Aquakem v. 7.2AQ1

Results from time period:

Tue Aug 07 13:56:17 2018

Tue Aug 07 13:59:41 2018

Sample Id	Sam/Ctr/c	Test short nan	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.3765	µg/l	8/7/2018 12:24:19	
5.OPPBCN	A	Reactive CN	P	4.6016	µg/l	8/7/2018 12:24:20	
10PPBCN	A	Reactive CN	P	9.5372	µg/l	8/7/2018 12:24:21	
50PPBCN	A	Reactive CN	P	50.2575	µg/l	8/7/2018 12:24:22	
100PPBCN	A	Reactive CN	P	101.2321	µg/l	8/7/2018 12:24:23	
250PPBCN	A	Reactive CN	P	250.0143	µg/l	8/7/2018 12:24:24	
500PPBCN	A	Reactive CN	P	499.7339	µg/l	8/7/2018 12:24:25	
ICV1	S	Reactive CN	P	97.6587	µg/l	8/7/2018 13:56:17	
ICB1	S	Reactive CN	P	0.681	µg/l	8/7/2018 13:56:18	
CCV1	S	Reactive CN	P	241.3198	µg/l	8/7/2018 13:56:19	
CCB1	S	Reactive CN	P	0.1556	µg/l	8/7/2018 13:56:20	
PB111832BL	S	Reactive CN	P	0.0186	µg/l	8/7/2018 13:56:21	
J4360-03	S	Reactive CN	P	-0.236	µg/l	8/7/2018 13:56:22	
J4360-03DUP	S	Reactive CN	P	-0.2494	µg/l	8/7/2018 13:56:23	
J4360-06	S	Reactive CN	P	-0.3677	µg/l	8/7/2018 13:56:24	
PB111833BL	S	Reactive CN	P	-0.3345	µg/l	8/7/2018 13:56:25	
J4366-02	S	Reactive CN	P	0.2729	µg/l	8/7/2018 13:56:26	
J4366-02DUP	S	Reactive CN	P	0.057	µg/l	8/7/2018 13:56:27	
CCV2	S	Reactive CN	P	259.7977	µg/l	8/7/2018 13:59:40	
CCB2	S	Reactive CN	P	-0.0258	µg/l	8/7/2018 13:59:41	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

8/7/2018 12:26


Test Total CN

Accepted 8/7/2018 12:26

Factor 1080
Bias 0.004

Coeff. of det. 0.999989

Errors

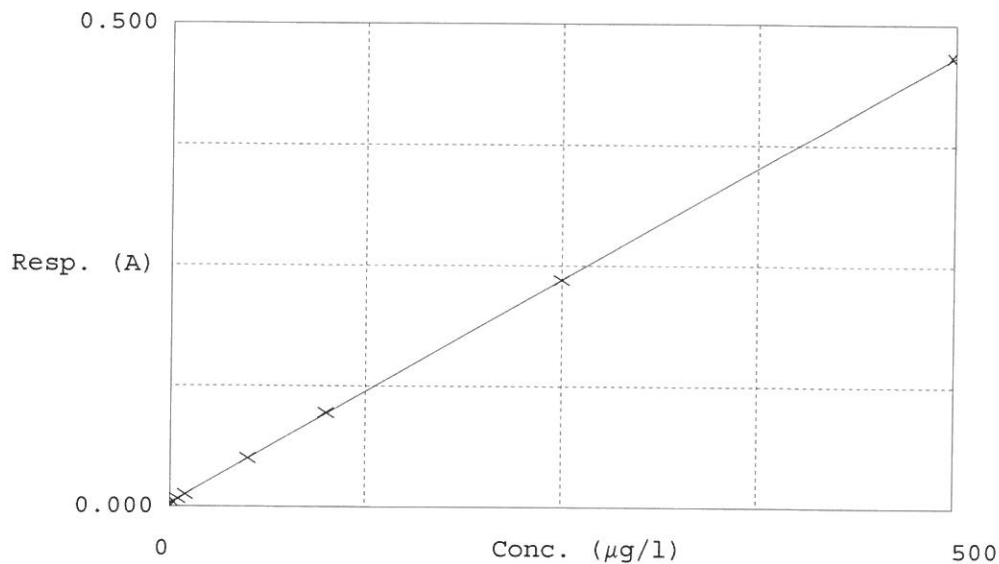

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.3765	0.0000	
2	5.0PPBCN	0.008	4.6016	5.0000	
3	10PPBCN	0.013	9.5372	10.0000	
4	50PPBCN	0.050	50.2575	50.0000	
5	100PPBCN	0.097	101.2321	100.0000	
6	250PPBCN	0.235	250.0143	250.0000	
7	500PPBCN	0.467	499.7339	500.0000	