

LB97445

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

8/21/2018 15:16

Test: Total CN ug/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	99.188	0.0	0.095	
ICB1	0.808	0.0	0.004	
CCV1	242.605	0.0	0.228	
CCB1	0.458	0.0	0.004	
PB112266BL	0.099	0.0	0.004	
PB112266BS	100.603	0.0	0.097	
J4556-01	0.606	0.0	0.004	
J4556-01DUP	0.372	0.0	0.004	
J4556-01MS	33.057	0.0	0.034	
J4556-01MSD	34.244	0.0	0.035	
J4566-01	10.394	0.0	0.013	
CCV2	258.176	0.0	0.243	
CCB2	0.533	0.0	0.004	

N	13
Mean	60.088
SD	91.7011
CV%	152.61

Aquakem v. 7.2AQ1

AS

Results from time period:

Tue Aug 21 15:03:49 2018

Tue Aug 21 15:15:44 2018

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	-0.2486	µg/l	8/21/2018 11:33:11	
5.OPPBCN	A	Total CN	P	4.6573	µg/l	8/21/2018 11:33:12	
10PPBCN	A	Total CN	P	10.0422	µg/l	8/21/2018 11:33:13	
50PPBCN	A	Total CN	P	49.0051	µg/l	8/21/2018 11:33:14	
100PPBCN	A	Total CN	P	102.2264	µg/l	8/21/2018 11:33:15	
250PPBCN	A	Total CN	P	249.3215	µg/l	8/21/2018 11:33:16	
500PPBCN	A	Total CN	P	499.996	µg/l	8/21/2018 11:33:17	
ICV1	S	Total CN	P	99.1877	µg/l	8/21/2018 15:03:49	
ICB1	S	Total CN	P	0.8076	µg/l	8/21/2018 15:03:50	
CCV1	S	Total CN	P	242.6047	µg/l	8/21/2018 15:11:25	
CCB1	S	Total CN	P	0.4577	µg/l	8/21/2018 15:11:26	
PB112266BL	S	Total CN	P	0.0991	µg/l	8/21/2018 15:11:28	
PB112266BS	S	Total CN	P	100.6033	µg/l	8/21/2018 15:11:29	
J4556-01	S	Total CN	P	0.6059	µg/l	8/21/2018 15:11:30	
J4556-01DUP	S	Total CN	P	0.3719	µg/l	8/21/2018 15:11:31	
J4556-01MS	S	Total CN	P	33.0574	µg/l	8/21/2018 15:11:32	
J4556-01MSD	S	Total CN	P	34.2439	µg/l	8/21/2018 15:15:41	
J4566-01	S	Total CN	P	10.3945	µg/l	8/21/2018 15:15:42	
CCV2	S	Total CN	P	258.1765	µg/l	8/21/2018 15:15:43	
CCB2	S	Total CN	P	0.5332	µg/l	8/21/2018 15:15:44	

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

8/21/2018 11:46


Test Total CN

Accepted 8/21/2018 11:46

Factor 1079
 Bias 0.004

Coeff. of det. 0.999968

Errors

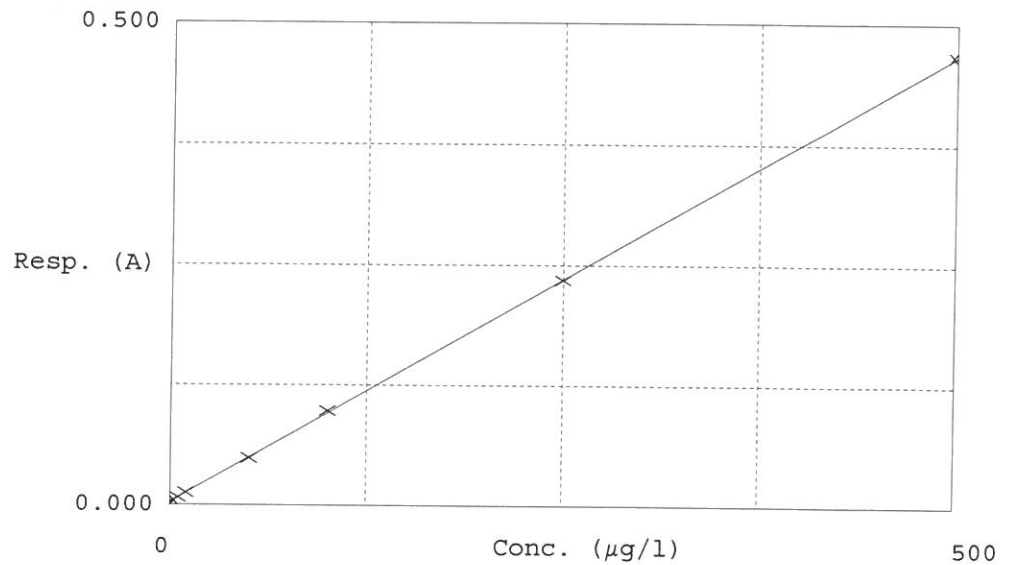

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.2486	0.0000	
2	5.0PPBCN	0.008	4.6573	5.0000	
3	10PPBCN	0.013	10.0422	10.0000	
4	50PPBCN	0.049	49.0051	50.0000	
5	100PPBCN	0.098	102.2264	100.0000	
6	250PPBCN	0.235	249.3215	250.0000	
7	500PPBCN	0.467	499.9960	500.0000	