

2B97761

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

9/6/2018 14:55

Test: *Reactive*
~~Total~~ CN *Mg/L*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.723	0.0	0.092	
ICB1	0.486	0.0	0.004	
CCV1	232.888	0.0	0.220	
CCB1	0.555	0.0	0.004	
PB112649BL	0.118	0.0	0.004	
J4801-04	-0.077	0.0	0.003	
J4801-04DUP	0.057	0.0	0.003	
PB112652BL	-0.106	0.0	0.003	
J4801-06	0.045	0.0	0.003	
J4801-06DUP	0.208	0.0	0.004	
CCV2	233.106	0.0	0.220	
CCB2	0.095	0.0	0.003	

N	12
Mean	46.925
SD	91.1120
CV%	194.17

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

9/6/2018 12:51


Test Total CN

Accepted 9/6/2018 12:51

Factor 1077
Bias 0.003

Coeff. of det. 0.999740

Errors

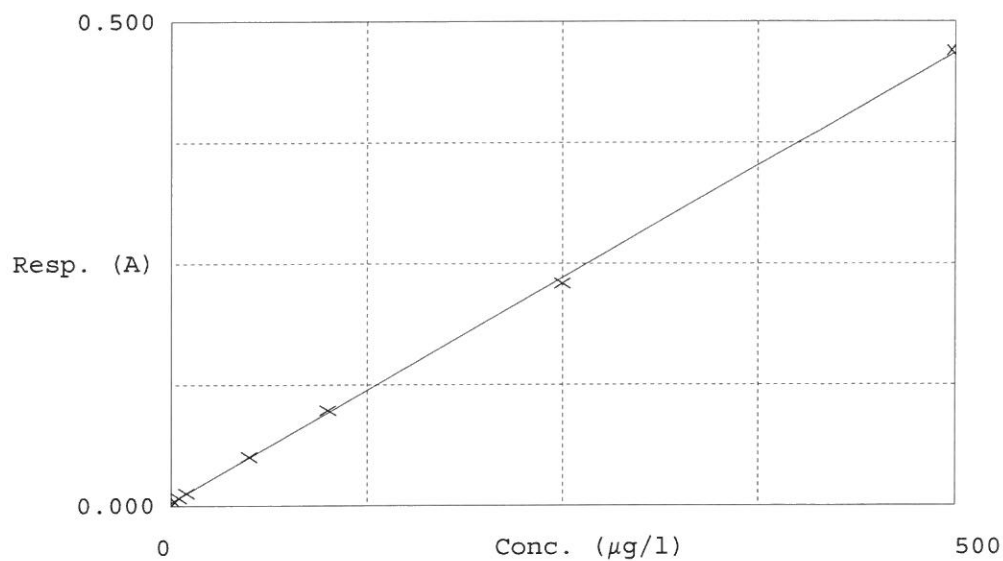

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.1764	0.0000	
2	5.0PPBCN	0.008	5.2231	5.0000	
3	10PPBCN	0.013	10.4181	10.0000	
4	50PPBCN	0.051	50.7833	50.0000	
5	100PPBCN	0.099	102.4938	100.0000	
6	250PPBCN	0.230	243.6918	250.0000	
7	500PPBCN	0.470	502.5664	500.0000	

Aquakem v. 7.2AQ1

Results from time period:

Thu Sep 06 14:43:19 2018

Thu Sep 06 14:46:07 2018

AB

Sample Id	Sam/Ctr/c	Test short name	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.1764	µg/l	9/6/2018 12:49:05	
5.0PPBCN	A	Reactive CN	P	5.2231	µg/l	9/6/2018 12:49:06	
10PPBCN	A	Reactive CN	P	10.4181	µg/l	9/6/2018 12:49:07	
50PPBCN	A	Reactive CN	P	50.7833	µg/l	9/6/2018 12:49:08	
100PPBCN	A	Reactive CN	P	102.4938	µg/l	9/6/2018 12:49:09	
250PPBCN	A	Reactive CN	P	243.6918	µg/l	9/6/2018 12:49:10	
500PPBCN	A	Reactive CN	P	502.5664	µg/l	9/6/2018 12:49:11	
ICV1	S	Reactive CN	P	95.7226	µg/l	9/6/2018 14:43:19	
ICB1	S	Reactive CN	P	0.4864	µg/l	9/6/2018 14:43:20	
CCV1	S	Reactive CN	P	232.8882	µg/l	9/6/2018 14:43:21	
CCB1	S	Reactive CN	P	0.5551	µg/l	9/6/2018 14:43:22	
PB112649BL	S	Reactive CN	P	0.1182	µg/l	9/6/2018 14:43:23	
J4801-04	S	Reactive CN	P	-0.0766	µg/l	9/6/2018 14:43:24	
J4801-04DUP	S	Reactive CN	P	0.0571	µg/l	9/6/2018 14:43:25	
PB112652BL	S	Reactive CN	P	-0.1056	µg/l	9/6/2018 14:43:26	
J4801-06	S	Reactive CN	P	0.0454	µg/l	9/6/2018 14:43:27	
J4801-06DUP	S	Reactive CN	P	0.2081	µg/l	9/6/2018 14:43:28	
CCV2	S	Reactive CN	P	233.1062	µg/l	9/6/2018 14:43:29	
CCB2	S	Reactive CN	P	0.0948	µg/l	9/6/2018 14:46:07	