

6897835

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AD

9/11/2018 12:13

Test: Reactive ug/L
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.977	0.0	0.092	
ICB1	-0.008	0.0	0.004	
CCV1	240.266	0.0	0.220	
CCB1	-0.213	0.0	0.004	
PB112754BL	-0.323	0.0	0.004	
J4724-19	-0.464	0.0	0.003	
J4724-19DUP	-0.577	0.0	0.003	
J4838-09	-0.482	0.0	0.003	
J4838-10	-0.654	0.0	0.003	
J4840-01	-0.331	0.0	0.004	
J4842-18	-0.743	0.0	0.003	
CCV2	254.636	0.0	0.233	
CCB2	-0.024	0.0	0.004	

N 13
Mean 45.312
SD 93.7536
CV% 206.91

4397835

Aquakem v. 7.2AQ1

Results from time period:

AK

Tue Sep 11 09:41:07 2018

Tue Sep 11 11:37:42 2018

Sample Id	Sam/Ctr/c/	Test short na	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.6383	µg/l	9/11/2018 10:44:29	
5.0PPBCN	A	Reactive CN	P	4.4454	µg/l	9/11/2018 10:44:30	
10PPBCN	A	Reactive CN	P	9.3879	µg/l	9/11/2018 10:44:31	
50PPBCN	A	Reactive CN	P	49.1385	µg/l	9/11/2018 10:44:32	
100PPBCN	A	Reactive CN	P	102.1154	µg/l	9/11/2018 10:44:33	
250PPBCN	A	Reactive CN	P	251.7406	µg/l	9/11/2018 10:44:34	
500PPBCN	A	Reactive CN	P	498.8106	µg/l	9/11/2018 10:44:35	
ICV1	S	Reactive CN	P	97.9774	µg/l	9/11/2018 11:34:18	
ICB1	S	Reactive CN	P	-0.0076	µg/l	9/11/2018 11:34:19	
CCV1	S	Reactive CN	P	240.2655	µg/l	9/11/2018 11:34:20	
CCB1	S	Reactive CN	P	-0.2135	µg/l	9/11/2018 11:34:21	
PB112754BL	S	Reactive CN	P	-0.3229	µg/l	9/11/2018 11:34:22	
J4724-19	S	Reactive CN	P	-0.464	µg/l	9/11/2018 11:34:23	
J4724-19DUP	S	Reactive CN	P	-0.5768	µg/l	9/11/2018 11:34:24	
J4838-09	S	Reactive CN	P	-0.4819	µg/l	9/11/2018 11:34:25	
J4838-10	S	Reactive CN	P	-0.6539	µg/l	9/11/2018 11:34:26	
J4840-01	S	Reactive CN	P	-0.3307	µg/l	9/11/2018 11:34:27	
J4842-18	S	Reactive CN	P	-0.7434	µg/l	9/11/2018 11:34:28	
CCV2	S	Reactive CN	P	254.6361	µg/l	9/11/2018 11:37:41	
CCB2	S	Reactive CN	P	-0.0239	µg/l	9/11/2018 11:37:42	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

9/11/2018 11:10


Test Total CN

Accepted 9/11/2018 11:10

Factor 1111
Bias 0.004

Coeff. of det. 0.999948

Errors

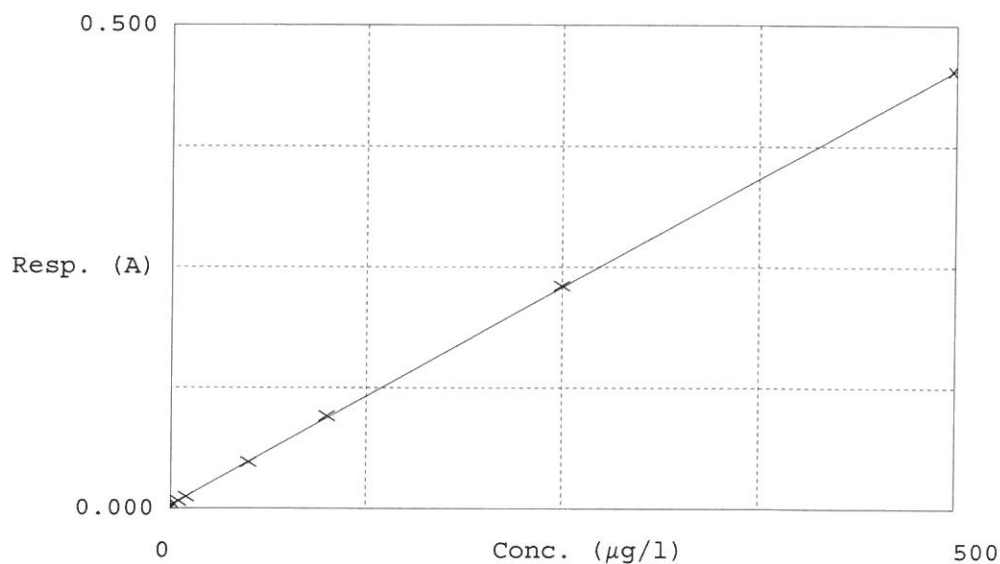

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.6383	0.0000	
2	5.0PPBCN	0.008	4.4454	5.0000	
3	10PPBCN	0.012	9.3879	10.0000	
4	50PPBCN	0.048	49.1385	50.0000	
5	100PPBCN	0.096	102.1154	100.0000	
6	250PPBCN	0.230	251.7406	250.0000	
7	500PPBCN	0.453	498.8106	500.0000	