

LB97857

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AW

9/12/2018 11:29

Test: ^{Reactive}
~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.065	0.0	0.092	
ICB1	0.344	0.0	0.003	
CCV1	239.683	0.0	0.228	
CCB1	0.164	0.0	0.003	
PB112781BL	-0.046	0.0	0.003	
J4780-02	-0.298	0.0	0.003	
J4780-02DUP	-0.247	0.0	0.003	
J4853-04	-0.067	0.0	0.003	
J4856-04	0.074	0.0	0.003	
J4856-11	0.295	0.0	0.003	
CCV2	239.487	0.0	0.228	
CCB2	0.270	0.0	0.003	

N	12
Mean	47.894
SD	93.5725
CV%	195.38

Aquakem v. 7.2AQ1

AR

Results from time period:

Wed Sep 12 09:38:33 2018

Wed Sep 12 11:24:30 2018

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive	Cl P	0.3611	µg/l	9/12/2018 9:38:33	
5.OPPBCN	A	Reactive	Cl P	5.0065	µg/l	9/12/2018 9:38:34	
10PPBCN	A	Reactive	Cl P	10.3141	µg/l	9/12/2018 9:38:35	
50PPBCN	A	Reactive	Cl P	49.8498	µg/l	9/12/2018 9:38:36	
100PPBCN	A	Reactive	Cl P	99.5471	µg/l	9/12/2018 9:38:37	
250PPBCN	A	Reactive	Cl P	249.6444	µg/l	9/12/2018 9:38:38	
500PPBCN	A	Reactive	Cl P	500.2771	µg/l	9/12/2018 9:38:39	
ICV1	S	Reactive	Cl P	95.0651	µg/l	9/12/2018 11:21:42	
ICB1	S	Reactive	Cl P	0.3436	µg/l	9/12/2018 11:21:43	
CCV1	S	Reactive	Cl P	239.6829	µg/l	9/12/2018 11:21:44	
CCB1	S	Reactive	Cl P	0.164	µg/l	9/12/2018 11:21:45	
PB112781BL	S	Reactive	Cl P	-0.0463	µg/l	9/12/2018 11:21:46	
J4780-02	S	Reactive	Cl P	-0.2982	µg/l	9/12/2018 11:21:47	
J4780-02DUP	S	Reactive	Cl P	-0.2465	µg/l	9/12/2018 11:21:48	
J4853-04	S	Reactive	Cl P	-0.067	µg/l	9/12/2018 11:21:49	
J4856-04	S	Reactive	Cl P	0.0741	µg/l	9/12/2018 11:21:50	
J4856-11	S	Reactive	Cl P	0.2954	µg/l	9/12/2018 11:21:51	
CCV2	S	Reactive	Cl P	239.4866	µg/l	9/12/2018 11:21:52	
CCB2	S	Reactive	Cl P	0.2703	µg/l	9/12/2018 11:24:30	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AB

9/12/2018 9:42


Test Total CN

Accepted 9/12/2018 9:40

Factor 1066
Bias 0.003

Coeff. of det. 0.999997

Errors

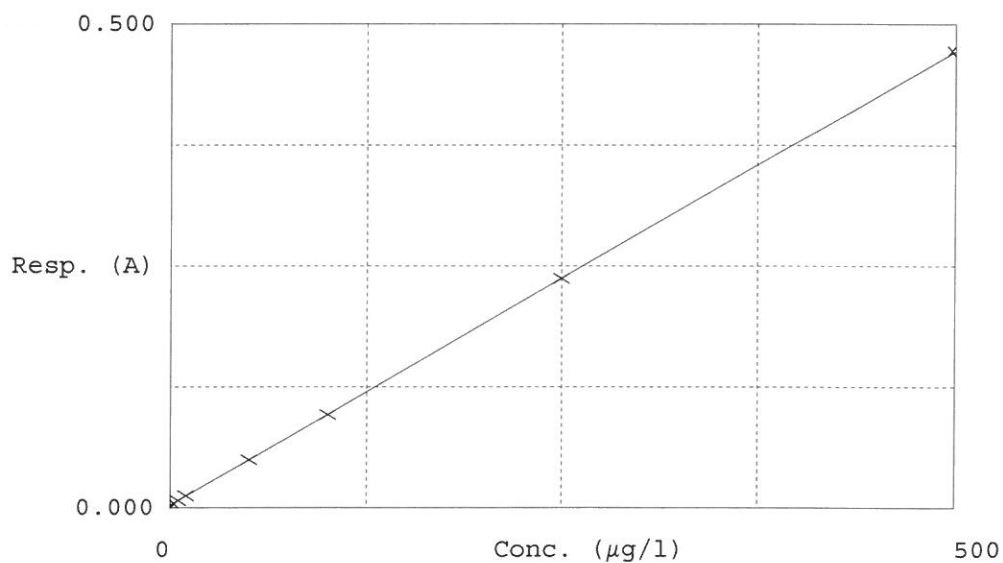

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.3611	0.0000	
2	5.0PPBCN	0.008	5.0065	5.0000	
3	10PPBCN	0.013	10.3141	10.0000	
4	50PPBCN	0.050	49.8498	50.0000	
5	100PPBCN	0.096	99.5471	100.0000	
6	250PPBCN	0.237	249.6444	250.0000	
7	500PPBCN	0.472	500.2771	500.0000	