

6397862

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

9/12/2018 14:24

Test: Total CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	94.971	0.0	0.092	
ICB1	0.206	0.0	0.003	
CCV1	241.573	0.0	0.230	
CCB1	0.275	0.0	0.003	
PB112790BL	0.126	0.0	0.003	
PB112790BS	95.762	0.0	0.093	
MIDPB112790	243.019	0.0	0.231	
J4790-02	1.670	0.0	0.004	
J4790-02DUP	1.338	0.0	0.004	
J4790-02MS	36.325	0.0	0.037	
J4790-02MSD	36.077	0.0	0.037	
CCV2	254.140	0.0	0.241	
CCB2	0.626	0.0	0.003	

N	13
Mean	77.393
SD	102.0430
CV%	131.85

U397862

Aquakem v. 7.2AQ1

Results from time period:

Wed Sep 12 14:16:00 2018

Wed Sep 12 14:19:24 2018

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Total CN	P	0.3611	µg/l	9/12/2018 9:38:33	
5.OPPBCN	A	Total CN	P	5.0065	µg/l	9/12/2018 9:38:34	
10PPBCN	A	Total CN	P	10.3141	µg/l	9/12/2018 9:38:35	
50PPBCN	A	Total CN	P	49.8498	µg/l	9/12/2018 9:38:36	
100PPBCN	A	Total CN	P	99.5471	µg/l	9/12/2018 9:38:37	
250PPBCN	A	Total CN	P	249.6444	µg/l	9/12/2018 9:38:38	
500PPBCN	A	Total CN	P	500.2771	µg/l	9/12/2018 9:38:39	
ICV1	S	Total CN	P	94.9707	µg/l	9/12/2018 14:16:00	
ICB1	S	Total CN	P	0.2063	µg/l	9/12/2018 14:16:01	
CCV1	S	Total CN	P	241.5732	µg/l	9/12/2018 14:16:02	
CCB1	S	Total CN	P	0.2753	µg/l	9/12/2018 14:16:03	
PB112790BL	S	Total CN	P	0.1258	µg/l	9/12/2018 14:16:04	
PB112790BS	S	Total CN	P	95.7619	µg/l	9/12/2018 14:16:05	
MIDPB112790	S	Total CN	P	243.0195	µg/l	9/12/2018 14:16:06	
J4790-02	S	Total CN	P	1.6699	µg/l	9/12/2018 14:16:07	
J4790-02DUP	S	Total CN	P	1.3384	µg/l	9/12/2018 14:16:08	
J4790-02MS	S	Total CN	P	36.3254	µg/l	9/12/2018 14:16:09	
J4790-02MSD	S	Total CN	P	36.0775	µg/l	9/12/2018 14:16:10	
CCV2	S	Total CN	P	254.1395	µg/l	9/12/2018 14:19:23	
CCB2	S	Total CN	P	0.6256	µg/l	9/12/2018 14:19:24	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by :

9/12/2018 9:40


Test Total CN

Accepted 9/12/2018 9:40

Factor 1066
Bias 0.003

Coeff. of det. 0.999997

Errors

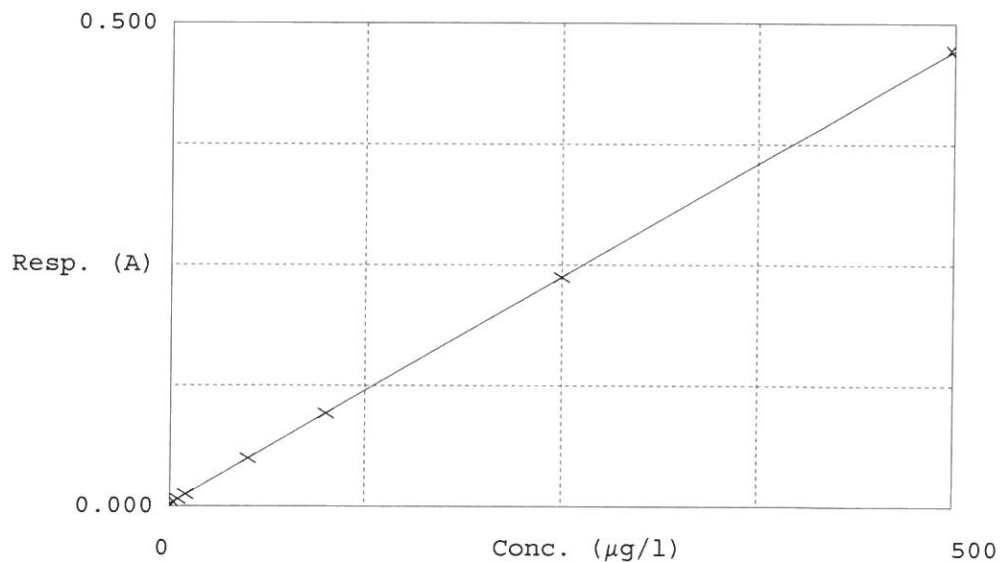

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	0.3611	0.0000	
2	5.0PPBCN	0.008	5.0065	5.0000	
3	10PPBCN	0.013	10.3141	10.0000	
4	50PPBCN	0.050	49.8498	50.0000	
5	100PPBCN	0.096	99.5471	100.0000	
6	250PPBCN	0.237	249.6444	250.0000	
7	500PPBCN	0.472	500.2771	500.0000	