

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

9/27/2018 14:52

Test: *Residue*
~~Total~~ CN *ng/d*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	97.718	0.0	0.096	
ICB1	0.296	0.0	0.005	
CCV1	247.005	0.0	0.236	
CCB1	0.244	0.0	0.004	
PB113281BL	0.297	0.0	0.005	
J5096-02	-0.034	0.0	0.004	
J5096-02DUP	0.199	0.0	0.004	
J5097-02	0.435	0.0	0.005	
J5097-04	-0.316	0.0	0.004	
J5097-06	0.441	0.0	0.005	
J5097-08	0.342	0.0	0.005	
J5099-02	-0.027	0.0	0.004	
J5100-04	0.097	0.0	0.004	
PB113243BL	0.250	0.0	0.004	
CCV2	244.970	0.0	0.234	
CCB2	-0.176	0.0	0.004	
PB113243BS	100.143	0.0	0.098	
J5078-02	0.268	0.0	0.004	
J5078-02DUP	-0.200	0.0	0.004	
J5083-04	-0.167	0.0	0.004	
J5083-05	-0.490	0.0	0.004	
J5083-06	-0.310	0.0	0.004	
J5101-02	0.114	0.0	0.004	
CCV3	261.464	0.0	0.250	
CCB3	0.077	0.0	0.004	

N	25
Mean	38.106
SD	84.8192
CV%	222.59

Aquakem v. 7.2AQ1

Results from time period:

Thu Sep 27 12:01:35 2018

Thu Sep 27 14:52:04 2018

AS

Sample Id	Sam/Ctr/c	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A	Reactive CN	P	-0.9005	µg/l	9/27/2018 10:01:32	
5.OPPBCN	A	Reactive CN	P	4.6644	µg/l	9/27/2018 10:01:33	
10PPBCN	A	Reactive CN	P	8.7634	µg/l	9/27/2018 10:01:34	
50PPBCN	A	Reactive CN	P	50.2629	µg/l	9/27/2018 10:01:35	
100PPBCN	A	Reactive CN	P	100.551	µg/l	9/27/2018 10:01:36	
250PPBCN	A	Reactive CN	P	253.5342	µg/l	9/27/2018 10:01:37	
500PPBCN	A	Reactive CN	P	498.1245	µg/l	9/27/2018 10:01:38	
ICV1	S	Reactive CN	P	97.7176	µg/l	9/27/2018 14:39:54	
ICB1	S	Reactive CN	P	0.2961	µg/l	9/27/2018 14:39:55	
CCV1	S	Reactive CN	P	247.0048	µg/l	9/27/2018 14:39:56	
CCB1	S	Reactive CN	P	0.2441	µg/l	9/27/2018 14:39:57	
PB113281BL	S	Reactive CN	P	0.2971	µg/l	9/27/2018 14:39:58	
J5096-02	S	Reactive CN	P	-0.0341	µg/l	9/27/2018 14:39:59	
J5096-02DUP	S	Reactive CN	P	0.1988	µg/l	9/27/2018 14:40:00	
J5097-02	S	Reactive CN	P	0.4347	µg/l	9/27/2018 14:40:01	
J5097-04	S	Reactive CN	P	-0.3161	µg/l	9/27/2018 14:40:02	
J5097-06	S	Reactive CN	P	0.4413	µg/l	9/27/2018 14:40:03	
J5097-08	S	Reactive CN	P	0.3417	µg/l	9/27/2018 14:40:04	
J5099-02	S	Reactive CN	P	-0.0271	µg/l	9/27/2018 14:47:29	
J5100-04	S	Reactive CN	P	0.0971	µg/l	9/27/2018 14:47:30	
PB113243BL	S	Reactive CN	P	0.2496	µg/l	9/27/2018 14:47:31	
CCV2	S	Reactive CN	P	244.97	µg/l	9/27/2018 14:47:32	
CCB2	S	Reactive CN	P	-0.1763	µg/l	9/27/2018 14:47:33	
PB113243BS	S	Reactive CN	P	100.1434	µg/l	9/27/2018 14:47:34	
J5078-02	S	Reactive CN	P	0.2684	µg/l	9/27/2018 14:47:35	
J5078-02DUP	S	Reactive CN	P	-0.1998	µg/l	9/27/2018 14:47:36	
J5083-04	S	Reactive CN	P	-0.1671	µg/l	9/27/2018 14:47:37	
J5083-05	S	Reactive CN	P	-0.4897	µg/l	9/27/2018 14:47:38	
J5083-06	S	Reactive CN	P	-0.3099	µg/l	9/27/2018 14:47:39	
J5101-02	S	Reactive CN	P	0.114	µg/l	9/27/2018 14:52:02	
CCV3	S	Reactive CN	P	261.464	µg/l	9/27/2018 14:52:03	
CCB3	S	Reactive CN	P	0.0769	µg/l	9/27/2018 14:52:04	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AD

9/27/2018 10:02


Test Total CN

Accepted 9/27/2018 10:02

Factor 1064
Bias 0.004

Coeff. of det. 0.999908

Errors

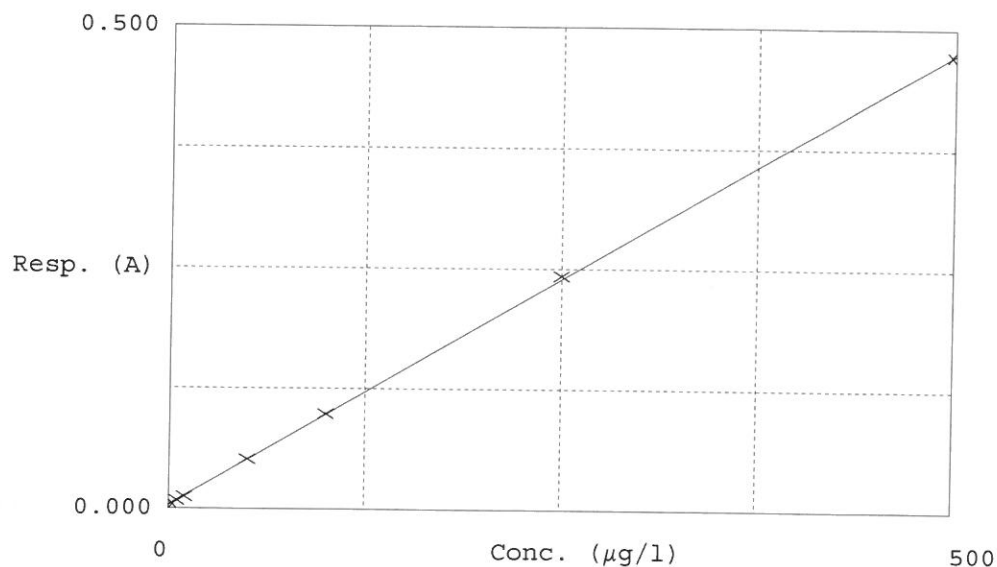

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.9005	0.0000	
2	5.0PPBCN	0.009	4.6644	5.0000	
3	10PPBCN	0.012	8.7634	10.0000	
4	50PPBCN	0.051	50.2629	50.0000	
5	100PPBCN	0.099	100.5510	100.0000	
6	250PPBCN	0.243	253.5342	250.0000	
7	500PPBCN	0.472	498.1245	500.0000	