

LB98897

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH

284 Sheffield Street,
Mountainside, NJ 07092Reviewed by : AL

10/29/2018 12:11

Test: ~~Total~~ CN

Reactive
ng/L

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.721	0.0	0.097	
ICB1	-0.186	0.0	0.004	
CCV1	241.855	0.0	0.236	
CCB1	-0.378	0.0	0.004	
PB114261BL	-0.453	0.0	0.003	
J5194-08	-0.280	0.0	0.004	
J5194-08DUP	-0.688	0.0	0.003	
J5194-12	-0.604	0.0	0.003	
J5697-02	-1.166	0.0	0.003	
J5194-10	-0.609	0.0	0.003	
CCV2	259.442	0.0	0.253	
CCB2	-0.352	0.0	0.004	

N	12
Mean	49.442
SD	98.0855
CV%	198.39

Aquakem v. 7.2AQ1

Results from time period:

Mon Oct 29 10:39:11 2018

AL

Mon Oct 29 11:54:08 2018

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time	Stat
0.0PPBCN	A	Reactive CN	P	-0.6295	µg/l	10/29/2018 11:01:56	
5.0PPBCN	A	Reactive CN	P	4.3298	µg/l	10/29/2018 11:01:57	
10PPBCN	A	Reactive CN	P	9.6182	µg/l	10/29/2018 11:01:58	
50PPBCN	A	Reactive CN	P	50.5513	µg/l	10/29/2018 11:01:59	
100PPBCN	A	Reactive CN	P	100.3907	µg/l	10/29/2018 11:02:00	
250PPBCN	A	Reactive CN	P	251.7168	µg/l	10/29/2018 11:02:01	
500PPBCN	A	Reactive CN	P	499.0227	µg/l	10/29/2018 11:02:02	
ICV1	S	Reactive CN	P	96.7213	µg/l	10/29/2018 11:30:32	
ICB1	S	Reactive CN	P	-0.1864	µg/l	10/29/2018 11:30:33	
CCV1	S	Reactive CN	P	241.8553	µg/l	10/29/2018 11:30:34	
CCB1	S	Reactive CN	P	-0.3776	µg/l	10/29/2018 11:30:35	
PB114261BL	S	Reactive CN	P	-0.4533	µg/l	10/29/2018 11:30:36	
J5194-08	S	Reactive CN	P	-0.2804	µg/l	10/29/2018 11:30:37	
J5194-08DUP	S	Reactive CN	P	-0.6877	µg/l	10/29/2018 11:30:38	
J5194-12	S	Reactive CN	P	-0.6041	µg/l	10/29/2018 11:30:40	
J5697-02	S	Reactive CN	P	-1.1664	µg/l	10/29/2018 11:30:41	
J5194-10	S	Reactive CN	P	-0.6086	µg/l	10/29/2018 11:54:06	
CCV2	S	Reactive CN	P	259.4422	µg/l	10/29/2018 11:54:07	
CCB2	S	Reactive CN	P	-0.3516	µg/l	10/29/2018 11:54:08	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AC

10/29/2018 11:07


Test Total CN

Accepted 10/29/2018 11:07

Factor 1040
Bias 0.004

Coeff. of det. 0.999974

Errors

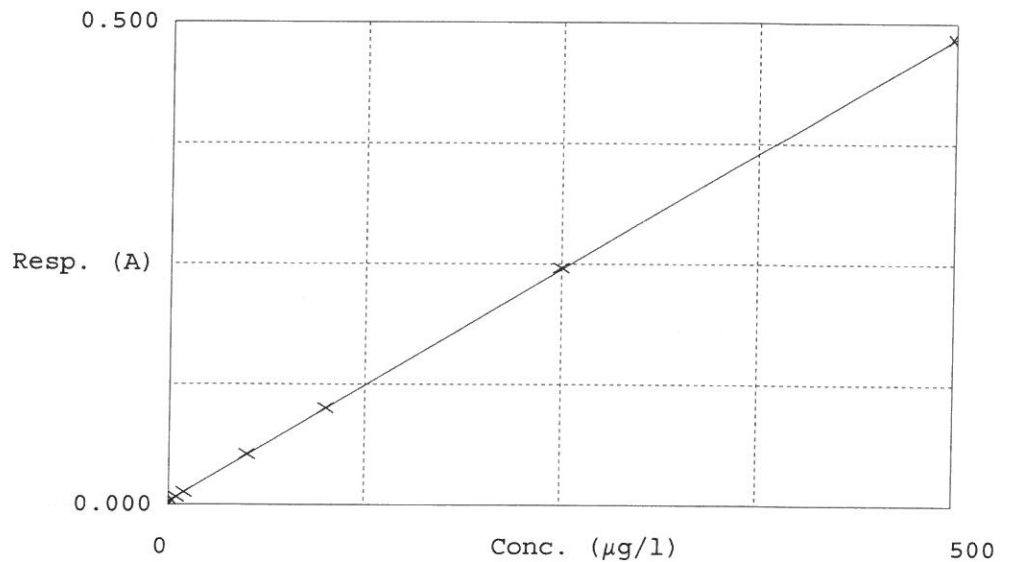

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.6295	0.0000	
2	5.0PPBCN	0.008	4.3298	5.0000	
3	10PPBCN	0.013	9.6182	10.0000	
4	50PPBCN	0.053	50.5513	50.0000	
5	100PPBCN	0.100	100.3907	100.0000	
6	250PPBCN	0.246	251.7168	250.0000	
7	500PPBCN	0.484	499.0227	500.0000	