

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AR

11/6/2018 12:43

Test: ~~Total~~ CN

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	95.264	0.0	0.101	
ICB1	0.272	0.0	0.004	
CCV1	246.171	0.0	0.255	
CCB1	-0.251	0.0	0.004	
PB114554BL	-0.138	0.0	0.004	
J5765-02	-0.238	0.0	0.004	
J5765-02DUP	1.718	0.0	0.006	
J5772-02	-0.175	0.0	0.004	
J5819-09	-0.256	0.0	0.004	
J5821-01	2.495	0.0	0.006	
J5821-02	1.850	0.0	0.006	
J5821-04	54.277	0.0	0.059	
J5826-04	0.140	0.0	0.004	
J5826-08	-0.154	0.0	0.004	
CCV2	253.737	0.0	0.262	
CCB2	-0.067	0.0	0.004	
J5826-12	-0.223	0.0	0.004	
J5827-10	0.023	0.0	0.004	
J5827-20	-0.045	0.0	0.004	
J5827-30	-0.025	0.0	0.004	
J5827-40	-0.149	0.0	0.004	
J5827-50	-0.074	0.0	0.004	
J5821-03	1.070	0.0	0.005	
CCV3	253.218	0.0	0.262	
CCB3	-0.221	0.0	0.004	

N	25
Mean	36.329
SD	83.7016
CV%	230.40

Aquakem v. 7.2AQ1

Results from time period:

Tue Nov 06 11:49:13 2018

Tue Nov 06 12:36:21 2018

AL

Sample Id	Sam/Ctr/c/	Test short	Test type	Result	Result unit	Result date and time	Stat
0.OPPBCN	A		Reactive Cl P	-0.3484	µg/l	11/6/2018 10:40:43	
5.OPPBCN	A		Reactive Cl P	4.9163	µg/l	11/6/2018 10:40:44	
10PPBCN	A		Reactive Cl P	9.9339	µg/l	11/6/2018 10:40:45	
50PPBCN	A		Reactive Cl P	49.3515	µg/l	11/6/2018 10:40:46	
100PPBCN	A		Reactive Cl P	98.3438	µg/l	11/6/2018 10:40:47	
250PPBCN	A		Reactive Cl P	254.8093	µg/l	11/6/2018 10:40:48	
500PPBCN	A		Reactive Cl P	497.9937	µg/l	11/6/2018 10:40:49	
ICV1	S		Reactive Cl P	95.2642	µg/l	11/6/2018 11:49:13	
ICB1	S		Reactive Cl P	0.2721	µg/l	11/6/2018 11:49:14	
CCV1	S		Reactive Cl P	246.1712	µg/l	11/6/2018 12:25:58	
CCB1	S		Reactive Cl P	-0.2509	µg/l	11/6/2018 12:25:59	
PB114554BL	S		Reactive Cl P	-0.1376	µg/l	11/6/2018 12:26:00	
J5765-02	S		Reactive Cl P	-0.2385	µg/l	11/6/2018 12:26:01	
J5765-02DUP	S		Reactive Cl P	1.7184	µg/l	11/6/2018 12:26:02	
J5772-02	S		Reactive Cl P	-0.175	µg/l	11/6/2018 12:26:03	
J5819-09	S		Reactive Cl P	-0.2556	µg/l	11/6/2018 12:26:04	
J5821-01	S		Reactive Cl P	2.4946	µg/l	11/6/2018 12:26:05	
J5821-02	S		Reactive Cl P	1.8505	µg/l	11/6/2018 12:26:06	
J5821-04	S		Reactive Cl P	54.2771	µg/l	11/6/2018 12:26:07	
J5826-04	S		Reactive Cl P	0.1402	µg/l	11/6/2018 12:26:08	
J5826-08	S		Reactive Cl P	-0.1541	µg/l	11/6/2018 12:33:33	
CCV2	S		Reactive Cl P	253.7371	µg/l	11/6/2018 12:33:34	
CCB2	S		Reactive Cl P	-0.0668	µg/l	11/6/2018 12:33:35	
J5826-12	S		Reactive Cl P	-0.223	µg/l	11/6/2018 12:33:36	
J5827-10	S		Reactive Cl P	0.0231	µg/l	11/6/2018 12:33:37	
J5827-20	S		Reactive Cl P	-0.0448	µg/l	11/6/2018 12:33:38	
J5827-30	S		Reactive Cl P	-0.0255	µg/l	11/6/2018 12:33:39	
J5827-40	S		Reactive Cl P	-0.1493	µg/l	11/6/2018 12:33:40	
J5827-50	S		Reactive Cl P	-0.0745	µg/l	11/6/2018 12:33:41	
J5821-03	S		Reactive Cl P	1.0703	µg/l	11/6/2018 12:33:42	
CCV3	S		Reactive Cl P	253.2181	µg/l	11/6/2018 12:33:43	
CCB3	S		Reactive Cl P	-0.2213	µg/l	11/6/2018 12:36:21	

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AK

11/6/2018 10:41


Test Total CN

Accepted 11/6/2018 10:41

Factor 980.9
Bias 0.004

Coeff. of det. 0.999852

Errors

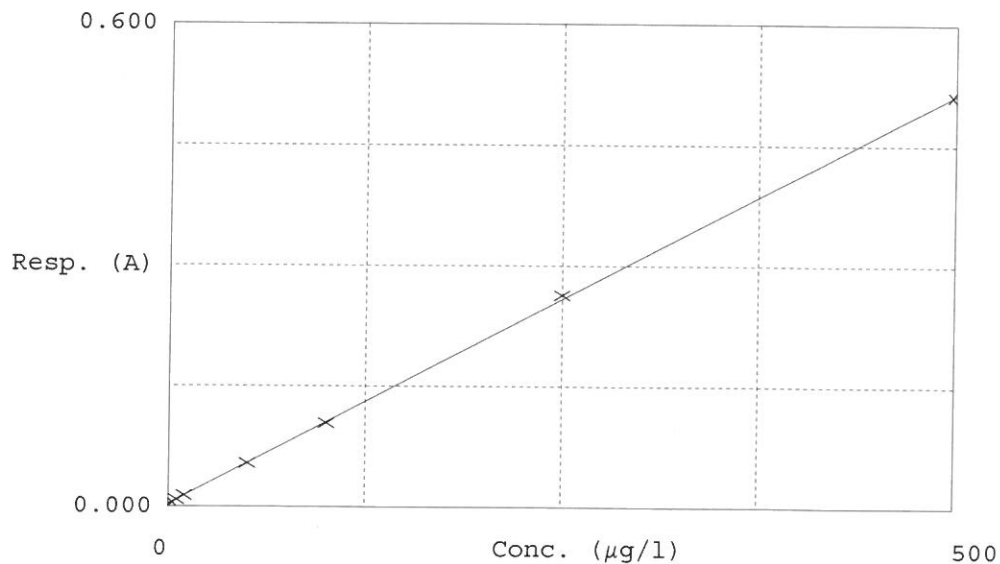

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-0.3484	0.0000	
2	5.0PPBCN	0.009	4.9163	5.0000	
3	10PPBCN	0.014	9.9339	10.0000	
4	50PPBCN	0.054	49.3515	50.0000	
5	100PPBCN	0.104	98.3438	100.0000	
6	250PPBCN	0.264	254.8093	250.0000	
7	500PPBCN	0.511	497.9937	500.0000	