

2B99697

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

12/10/2018 13:57

Test: *Acetone* Total CN*mg/d*

Sample Id	Result	Dil. 1 +	Response	Errors
ICV1	96.801	0.0	0.089	
ICB1	-0.160	0.0	0.004	
CCV1	239.595	0.0	0.213	
CCB1	-0.351	0.0	0.004	
PB115489BL	0.016	0.0	0.004	
J6196-02	-0.091	0.0	0.004	
J6196-02DUP	-0.469	0.0	0.004	
J6196-04	-0.396	0.0	0.004	
J6197-02	-0.371	0.0	0.004	
J6214-44	-0.485	0.0	0.004	
J6290-02	-0.137	0.0	0.004	
J6296-01	-0.510	0.0	0.004	
J6302-03	-0.076	0.0	0.004	
J6306-03	-0.394	0.0	0.004	
CCV2	242.406	0.0	0.216	
CCB2	-0.074	0.0	0.004	
J6309-01	-0.148	0.0	0.004	
J6309-03	-0.691	0.0	0.003	
J6316-02	0.941	0.0	0.005	
J6316-06	-0.842	0.0	0.003	
J6316-14	-0.812	0.0	0.003	
J6316-18	-1.195	0.0	0.003	
J6316-22	-0.558	0.0	0.004	
PB115490BL	-0.798	0.0	0.003	
J6309-02	-0.639	0.0	0.003	
CCV3	243.765	0.0	0.217	
CCB3	-0.578	0.0	0.004	
J6309-02DUP	-0.739	0.0	0.003	
J6196-06	-0.838	0.0	0.003	
J6316-10	-0.881	0.0	0.003	
<i>AS</i> <i>CCV4</i> CV4	257.875	0.0	0.229	
CCB4	-0.383	0.0	0.004	

N 32
 Mean 33.400
 SD 83.4287
 CV% 249.79

Aquakem v. 7.2AQ1

Results from time period:

Mon Dec 10 12:30:40 2018

Mon Dec 10 13:57:01 2018

AS

Sample Id	Sam/Ctr/c/	Test short nam	Test type	Result	Result unit	Result date and time
0.OPPBCN	A	Reactive CN	P	-1.104	µg/l	12/10/2018 12:30:40
5.OPPBCN	A	Reactive CN	P	4.0236	µg/l	12/10/2018 12:30:41
10PPBCN	A	Reactive CN	P	12.1804	µg/l	12/10/2018 12:30:42
50PPBCN	A	Reactive CN	P	48.8695	µg/l	12/10/2018 12:30:43
100PPBCN	A	Reactive CN	P	100.1098	µg/l	12/10/2018 12:30:44
250PPBCN	A	Reactive CN	P	251.727	µg/l	12/10/2018 12:30:45
500PPBCN	A	Reactive CN	P	499.1937	µg/l	12/10/2018 12:30:46
ICV1	S	Reactive CN	P	96.8014	µg/l	12/10/2018 13:12:58
ICB1	S	Reactive CN	P	-0.1599	µg/l	12/10/2018 13:12:59
CCV1	S	Reactive CN	P	239.5954	µg/l	12/10/2018 13:13:02
CCB1	S	Reactive CN	P	-0.3514	µg/l	12/10/2018 13:13:04
PB115489BL	S	Reactive CN	P	0.0161	µg/l	12/10/2018 13:13:05
J6196-02	S	Reactive CN	P	-0.0907	µg/l	12/10/2018 13:13:06
J6196-02DUP	S	Reactive CN	P	-0.4687	µg/l	12/10/2018 13:13:07
J6196-04	S	Reactive CN	P	-0.3963	µg/l	12/10/2018 13:20:29
J6197-02	S	Reactive CN	P	-0.3711	µg/l	12/10/2018 13:20:30
J6214-44	S	Reactive CN	P	-0.485	µg/l	12/10/2018 13:20:31
J6290-02	S	Reactive CN	P	-0.1371	µg/l	12/10/2018 13:20:32
J6296-01	S	Reactive CN	P	-0.5103	µg/l	12/10/2018 13:20:33
J6302-03	S	Reactive CN	P	-0.0761	µg/l	12/10/2018 13:20:34
J6306-03	S	Reactive CN	P	-0.3943	µg/l	12/10/2018 13:20:35
CCV2	S	Reactive CN	P	242.4062	µg/l	12/10/2018 13:20:36
CCB2	S	Reactive CN	P	-0.0739	µg/l	12/10/2018 13:20:37
J6309-01	S	Reactive CN	P	-0.1484	µg/l	12/10/2018 13:20:38
J6309-03	S	Reactive CN	P	-0.6906	µg/l	12/10/2018 13:20:39
J6316-02	S	Reactive CN	P	0.9413	µg/l	12/10/2018 13:28:04
J6316-06	S	Reactive CN	P	-0.8422	µg/l	12/10/2018 13:28:05
J6316-14	S	Reactive CN	P	-0.812	µg/l	12/10/2018 13:28:07
J6316-18	S	Reactive CN	P	-1.1949	µg/l	12/10/2018 13:28:08
J6316-22	S	Reactive CN	P	-0.5578	µg/l	12/10/2018 13:28:09
PB115490BL	S	Reactive CN	P	-0.798	µg/l	12/10/2018 13:28:10
J6309-02	S	Reactive CN	P	-0.6388	µg/l	12/10/2018 13:28:11
CCV3	S	Reactive CN	P	243.7649	µg/l	12/10/2018 13:28:12
CCB3	S	Reactive CN	P	-0.5782	µg/l	12/10/2018 13:28:13
J6309-02DUP	S	Reactive CN	P	-0.7391	µg/l	12/10/2018 13:28:14
J6196-06	S	Reactive CN	P	-0.8379	µg/l	12/10/2018 13:31:55
J6316-10	S	Reactive CN	P	-0.8809	µg/l	12/10/2018 13:42:46
CCV4	S	Reactive CN	P	257.8752	µg/l	12/10/2018 13:57:00
CCB4	S	Reactive CN	P	-0.3826	µg/l	12/10/2018 13:57:01

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

12/10/2018 12:39


Test Total CN

Accepted 12/10/2018 12:39

Factor 1144
Bias 0.004

Coeff. of det. 0.999942

Errors

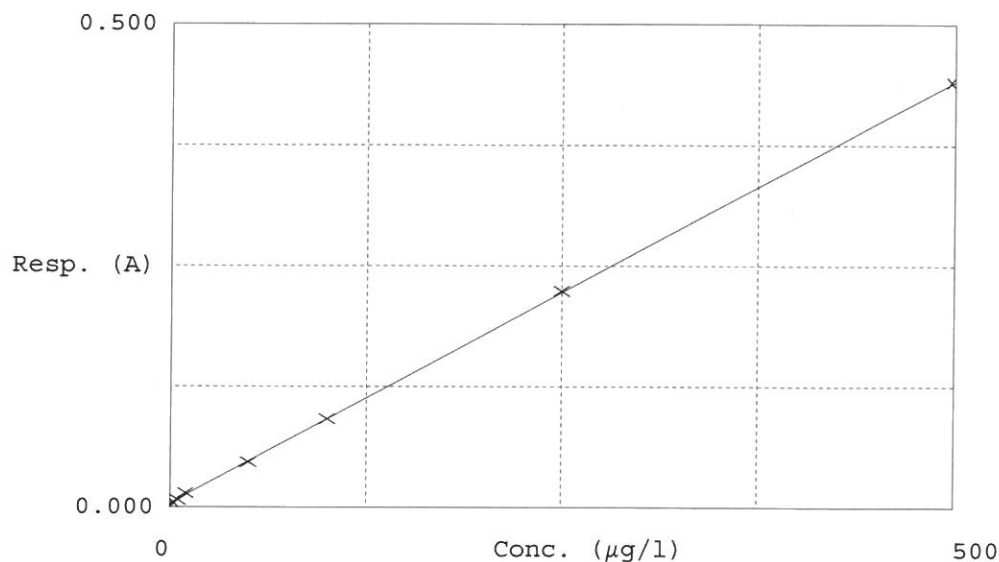

	Calibrator	Response	Calc. con.	Conc.	Errors
1	0.0PPBCN	0.003	-1.1040	0.0000	
2	5.0PPBCN	0.008	4.0236	5.0000	
3	10PPBCN	0.015	12.1804	10.0000	
4	50PPBCN	0.047	48.8695	50.0000	
5	100PPBCN	0.092	100.1098	100.0000	
6	250PPBCN	0.224	251.7270	250.0000	
7	500PPBCN	0.440	499.1937	500.0000	