

21399946

Test results

Aquakem 7.2AQ1

Page: 1

CHEMTECH
284 Sheffield Street,
Mountainside, NJ 07092
Reviewed by : AS

12/20/2018 9:12

Test: CNEPA-NEW

mg/d

Sample Id	Result	Dil. 1 +	Response	Errors
ICV ICV	94.922	0.0	0.100	
ICB ICB	-0.393	0.0	0.008	
CCV001 CCV001	235.539	0.0	0.234	
CCB001 CCB001	-0.350	0.0	0.008	
<i>AS</i> PB115864BL PBW864	-0.169	0.0	0.009	
J6366-01 METC10	1.635	0.0	0.010	
J6366-02 METC11	7.879	0.0	0.016	
J6366-03 METC11D	5.486	0.0	0.014	
J6366-04 METC11S	88.995	0.0	0.094	
CCV002 CCV002	239.650	0.0	0.238	
CCB002 CCB002	-0.801	0.0	0.008	

N	11
Mean	61.127
SD	94.2527
CV%	154.19

Aquakem v. 7.2AQ1

Results from time period:

Thu Dec 20 08:01:27 2018

Thu Dec 20 09:11:42 2018

AS

Sample Id	Sam/Ctr/c/	Test short name	Test type	Result	Result unit	Result date and time
S0.0	A	CNEPA-NEW	P	-1.3266	µg/l	12/20/2018 8:39:22
S5.0	A	CNEPA-NEW	P	4.1768	µg/l	12/20/2018 8:39:23
S10.0	A	CNEPA-NEW	P	11.2346	µg/l	12/20/2018 8:39:24
S100.0	A	CNEPA-NEW	P	101.3419	µg/l	12/20/2018 8:39:25
S250.0	A	CNEPA-NEW	P	249.7163	µg/l	12/20/2018 8:39:26
S500.0	A	CNEPA-NEW	P	499.857	µg/l	12/20/2018 8:39:27
ICV ICV	S	CNEPA-NEW	P	94.9221	µg/l	12/20/2018 9:05:25
ICB ICB	S	CNEPA-NEW	P	-0.3935	µg/l	12/20/2018 9:05:26
CCV001 CCV001	S	CNEPA-NEW	P	235.5393	µg/l	12/20/2018 9:05:28
CCB001 CCB001	S	CNEPA-NEW	P	-0.3496	µg/l	12/20/2018 9:05:29
PB115864BL PBW864	S	CNEPA-NEW	P	-0.1686	µg/l	12/20/2018 9:05:30
J6366-01 METC10	S	CNEPA-NEW	P	1.6354	µg/l	12/20/2018 9:05:31
J6366-02 METC11	S	CNEPA-NEW	P	7.8794	µg/l	12/20/2018 9:05:32
J6366-03 METC11D	S	CNEPA-NEW	P	5.4855	µg/l	12/20/2018 9:05:33
J6366-04 METC11S	S	CNEPA-NEW	P	88.9954	µg/l	12/20/2018 9:05:34
CCV002 CCV002	S	CNEPA-NEW	P	239.65	µg/l	12/20/2018 9:11:35
CCB002 CCB002	S	CNEPA-NEW	P	-0.8013	µg/l	12/20/2018 9:11:36

CHEMTECH
 284 Sheffield Street,
 Mountainside, NJ 07092
 Reviewed by : AS

12/20/2018 8:40


Test CNEPA-NEW (Instrument ID: Konelab)

Accepted 12/20/2018 8:40

Factor (slope) 1045
 Bias (y-intercept) 0.009

Coeff. of det. 0.999970

Errors

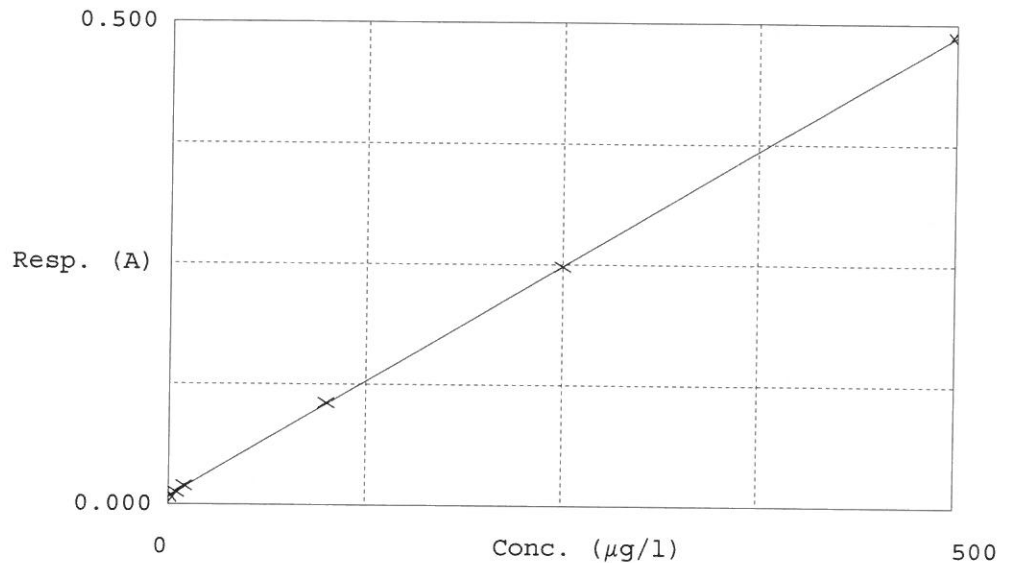

	Calibrator	Response	Calc. con.	Conc.	Errors - Percentage
1	0.0PPBCN	0.008	-1.3266	0.0000	
2	5.0PPBCN	0.013	4.1768	5.0000	83.536%
3	10PPBCN	0.020	11.2346	10.0000	112.36%
4	100PPBCN	0.106	101.3419	100.0000	101.341%
5	250PPBCN	0.248	249.7163	250.0000	99.8865%
6	500PPBCN	0.487	499.8570	500.0000	99.9714%

AS
 12/20/18