


Data Path : Z:\HPCHEM1\BNA_B\DATA\BB030917\
 Data File : BB058699.D
 Acq On : 9 Mar 2017 9:46
 Operator : UM/SJ
 Sample : DFTPP76
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_B
 ClientSampleId :
 DFTPP76

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_B\METHOD\SOM-EPA-BB030917-PAH.M
 Title : SVOA CALIBRATION
 Last Update : Fri Mar 10 14:54:06 2017

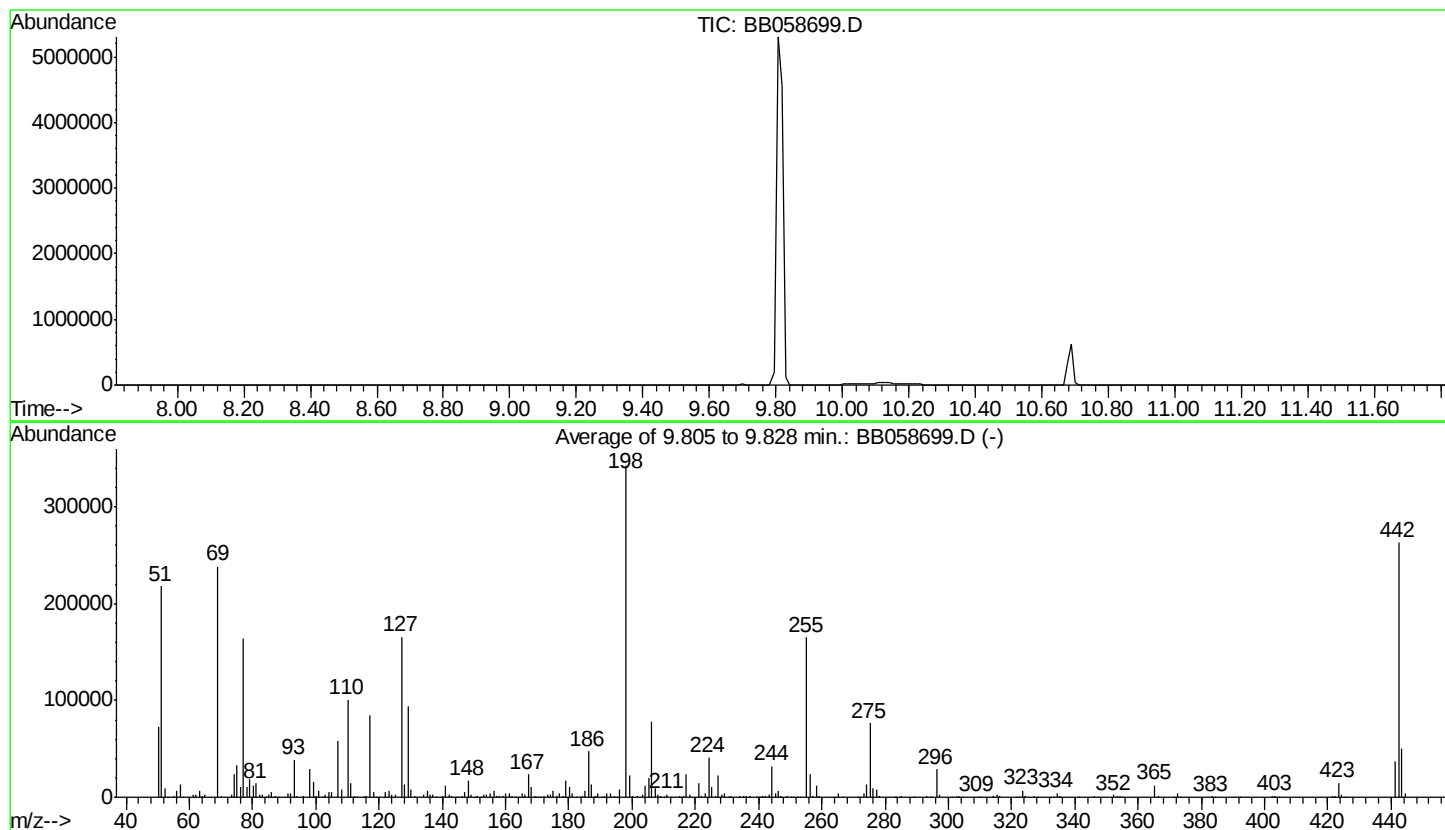

AutoFind: Scans 567, 568, 569; Background Corrected with Scan 564

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	63.7	218053	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	69.6	238495	PASS
70	69	0.00	2	0.4	878	PASS
127	198	10	80	48.3	165590	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	342494	PASS
199	198	5	9	6.5	22325	PASS
275	198	10	60	22.2	76184	PASS
365	198	1	100	3.6	12476	PASS
441	442	0.01	100	14.1	37014	PASS
442	198	50	100	76.8	262896	PASS
443	442	15	24	19.4	50900	PASS

m/z	Abundance
50.10	165952.0
51.10	490752.0
52.15	21408.0
53.05	840.0
55.05	3749.0
56.05	14946.0
57.05	28536.0
58.00	1172.0
61.10	5721.0
62.10	7405.0
63.10	17344.0
64.05	1989.0
65.05	5384.0
69.05	521536.0
70.00	1782.0
73.30	5235.0
74.10	51232.0
75.10	72056.0
76.25	23304.0
77.15	348224.0
78.15	24544.0
79.05	41680.0
80.05	26728.0
81.05	30600.0
82.15	6388.0
83.00	4956.0
84.10	583.0
85.00	4533.0
86.10	10271.0
87.10	3795.0
88.10	1092.0
91.15	6641.0
92.05	8956.0
93.15	78360.0
94.15	3948.0
96.20	1549.0
98.10	56984.0
99.10	31272.0
100.10	2307.0
101.05	14624.0
102.15	825.0
103.05	5179.0
104.05	10959.0
105.05	11026.0
107.10	115688.0
108.10	16880.0
110.10	202496.0
111.10	29384.0
112.20	3278.0
113.10	748.0
114.95	554.0
117.15	159360.0
118.15	10275.0
119.25	686.0
120.10	1002.0
122.10	9880.0
123.10	12635.0
124.10	5460.0
125.10	4038.0
127.15	313152.0
128.15	24816.0
129.15	176832.0
130.15	13986.0
131.15	2236.0
132.10	1155.0
134.10	4584.0
135.10	11900.0
136.20	4198.0
137.10	5652.0
138.05	863.0
139.25	788.0
140.15	2014.0
141.15	23072.0
142.15	6727.0
143.15	4064.0
144.10	936.0
145.20	715.0
146.10	3551.0
147.10	10116.0
148.10	30240.0
149.10	4169.0
150.20	834.0
151.25	1842.0
152.25	1043.0
153.15	6274.0
154.15	3951.0
155.15	7582.0
156.15	12852.0
157.20	2360.0
158.10	3096.0
159.10	2497.0

Instrument :
BNA_B
ClientSampleId :
DFTPP76

160.10	5454.0
161.20	7690.0
162.20	1821.0
164.05	808.0
165.15	6949.0
166.25	5114.0
167.15	39872.0
168.15	17304.0
169.10	2425.0
170.20	769.0
171.10	1246.0
172.10	2962.0
173.10	3500.0
174.20	5441.0
175.15	11351.0
176.15	2792.0
177.15	6425.0
178.15	1908.0
179.15	26792.0
180.15	16896.0
181.15	6587.0
182.10	804.0
183.30	869.0
184.20	1495.0
185.20	10382.0
186.20	73504.0
187.20	19120.0
188.15	2211.0
189.15	5222.0
190.15	905.0
191.05	2048.0
192.15	7225.0
193.25	6624.0
194.20	1415.0
196.10	13216.0
198.10	502080.0
199.20	33616.0
200.15	2210.0
201.65	1668.0
203.15	3787.0
204.15	17976.0
205.15	27184.0
206.20	112360.0
207.10	14996.0
208.10	3581.0
209.10	1362.0
210.30	2080.0
211.20	3927.0
212.10	888.0
215.15	1270.0
216.25	2489.0
217.15	31584.0
218.15	3668.0
221.10	18584.0
222.00	4346.0
223.20	6084.0
224.20	55304.0
225.15	13076.0
226.25	1672.0
227.15	31008.0
228.15	3768.0
229.25	4730.0
231.20	1847.0
234.20	1271.0
235.20	1771.0
236.20	1297.0
237.15	1224.0
239.15	870.0
240.35	705.0
241.15	1460.0
242.25	2287.0
243.20	2734.0
244.20	39360.0
245.30	4530.0
246.20	8501.0
247.10	1904.0
249.20	866.0
252.25	613.0
253.25	871.0
255.25	192704.0
256.20	27768.0
257.20	1978.0
258.30	13001.0
259.10	2098.0
264.15	576.0
265.25	4027.0
266.25	572.0
272.30	572.0
273.20	4322.0
274.25	14321.0
275.25	77336.0
276.25	9221.0
277.25	8691.0
278.25	1587.0
283.10	714.0

Instrument :
BNA_B
ClientSampleId :
DFTPP76

285.20	1127.0
293.20	1243.0
296.30	26712.0
297.30	2944.0
303.25	1983.0
304.35	567.0
314.25	937.0
315.25	3336.0
316.35	1190.0
323.40	5294.0
324.25	1237.0
327.15	1181.0
328.35	522.0
332.30	673.0
334.30	3454.0
335.30	685.0
346.50	778.0
352.35	1340.0
353.55	844.0
354.35	1371.0
365.35	8585.0
366.35	959.0
372.40	1978.0
383.40	579.0
402.35	546.0
403.25	762.0
421.40	782.0
422.60	570.0
423.35	6163.0
424.35	1343.0
441.50	13098.0
442.40	96640.0
443.40	19024.0
444.40	1512.0

Instrument :
BNA_B
ClientSampleId :
DFTPP76

m/z	Abundance
50.10	51208.0
51.10	161216.0
52.05	6248.0
55.05	1282.0
56.05	4190.0
57.05	9987.0
58.00	506.0
61.00	1368.0
62.10	1954.0
63.10	4578.0
64.05	832.0
65.05	2135.0
69.05	191936.0
70.10	852.0
73.20	1995.0
74.10	18832.0
75.10	26496.0
76.15	9448.0
77.05	140864.0
78.05	7585.0
79.05	14031.0
80.05	9780.0
81.05	11283.0
82.05	2196.0
83.10	1472.0
85.10	2073.0
86.10	4263.0
87.10	1398.0
88.10	730.0
91.05	4155.0
92.15	3810.0
93.05	37480.0
94.15	1436.0
96.10	612.0
98.10	28904.0
99.10	15354.0
100.10	919.0
101.05	5691.0
103.05	2129.0
104.05	4341.0
105.15	3973.0
107.10	58560.0
108.10	7182.0
110.10	97864.0
111.10	14249.0
112.10	1488.0
113.15	511.0
115.25	597.0
116.05	2872.0
117.15	92496.0
118.05	4353.0
120.00	567.0
122.10	5137.0
123.10	6630.0
124.10	3656.0
125.10	2319.0
127.15	181568.0
128.15	14319.0
129.15	102768.0
130.15	8168.0
130.95	1156.0
132.20	650.0
134.20	2288.0
135.10	7356.0
136.10	2844.0
137.10	2767.0
138.15	515.0
140.15	1302.0
141.15	13937.0
142.15	3195.0
143.15	1967.0
144.10	593.0
146.20	2124.0
147.10	5963.0
148.10	21352.0
149.20	3204.0
150.10	867.0
151.15	1518.0
152.05	927.0
153.15	3575.0
154.05	2943.0
155.15	5393.0
156.15	9107.0
157.30	1461.0
158.10	1965.0
159.00	1507.0
160.10	4853.0
161.20	5232.0
162.10	1542.0
163.25	570.0
164.15	611.0

Instrument :
BNA_B
ClientSampleId :
DFTPP76

165.15	5798.0
166.15	3559.0
167.15	30000.0
168.15	13495.0
169.10	2155.0
169.90	622.0
171.00	685.0
172.10	2334.0
173.20	3071.0
174.20	4382.0
175.15	9494.0
176.15	2028.0
177.15	4281.0
178.25	1561.0
179.15	23376.0
180.15	13554.0
181.15	5153.0
182.10	849.0
184.20	1144.0
185.20	9562.0
186.20	67392.0
187.20	19448.0
188.35	1535.0
189.15	5288.0
190.15	714.0
191.25	1914.0
192.15	5596.0
193.25	6804.0
194.20	1367.0
195.10	744.0
196.20	10794.0
198.10	515520.0
199.20	33360.0
200.15	2140.0
201.55	1728.0
203.15	3703.0
204.15	17824.0
205.15	31600.0
206.20	120520.0
207.20	13098.0
208.10	4563.0
209.20	1307.0
211.10	4915.0
215.15	1520.0
216.25	2792.0
217.15	39472.0
218.15	4559.0
221.20	25160.0
223.20	6418.0
224.20	65912.0
225.15	17288.0
226.25	1671.0
227.15	35200.0
228.25	4145.0
229.25	5394.0
230.25	687.0
231.20	2262.0
234.20	2133.0
235.20	2256.0
236.20	1511.0
237.05	1199.0
239.25	1213.0
240.05	835.0
241.25	1797.0
242.15	3155.0
243.30	4098.0
244.20	56024.0
245.20	6752.0
246.20	13196.0
247.20	2345.0
249.20	1496.0
250.05	513.0
251.15	626.0
253.25	1164.0
255.25	295936.0
256.20	41792.0
257.20	2775.0
258.20	20840.0
259.20	3002.0
265.25	8958.0
266.35	944.0
271.10	527.0
272.20	981.0
273.30	8858.0
274.15	25904.0
275.25	148864.0
276.25	18864.0
277.25	14601.0
278.25	2010.0
283.40	1047.0
285.20	1794.0
289.05	567.0
293.30	2942.0
294.20	1017.0
296.30	58128.0

Instrument :
BNA_B
ClientSampleId :
DFTPP76

297.30	6525.0
301.25	509.0
302.35	1008.0
303.35	3864.0
304.45	1388.0
308.20	528.0
309.30	557.0
310.30	517.0
314.25	2002.0
315.25	5921.0
316.25	2948.0
321.30	1599.0
322.20	671.0
323.40	15618.0
324.25	2975.0
327.25	3502.0
328.45	1489.0
332.30	1311.0
333.30	1559.0
334.30	9618.0
335.30	2270.0
341.35	1977.0
346.30	3414.0
347.30	671.0
352.35	5080.0
353.45	3152.0
354.35	3802.0
355.20	730.0
365.35	27664.0
366.35	3510.0
371.40	1475.0
372.40	8943.0
373.45	1746.0
383.40	2351.0
384.40	764.0
390.45	1312.0
391.55	701.0
392.30	674.0
402.45	3204.0
403.45	4250.0
404.40	1316.0
421.40	4560.0
422.40	3694.0
423.45	35752.0
424.45	7455.0
425.35	504.0
441.40	92064.0
442.40	643200.0
443.40	126320.0
444.40	10261.0

Instrument :
BNA_B
ClientSampleId :
DFTPP76

m/z	Abundance
50.10	697.0
51.10	2191.0
69.15	2013.0
74.90	526.0
77.05	1739.0
93.05	655.0
107.00	615.0
110.10	1180.0
117.15	1562.0
127.05	2050.0
129.05	1362.0
167.15	581.0
186.00	992.0
198.10	9883.0
206.10	1472.0
207.10	816.0
217.15	855.0
224.20	1188.0
227.25	866.0
244.20	666.0
255.25	6055.0
256.30	654.0
274.15	527.0
275.15	2352.0
296.30	1298.0
323.50	559.0
365.35	1181.0
423.35	1990.0
441.40	5881.0
442.40	48848.0
443.50	7356.0

Instrument :
BNA_B
ClientSampleId :
DFTPP76

m/z Abundance

Instrument :
BNA_B
ClientSampleId :
DFTPP76