


Data Path : Z:\HPCHEM1\BNA B\DATA\BB093016\
 Data File : BB058561.D
 Acq On : 29 Sep 2016 11:01
 Operator : UM/SJ
 Sample : DFTTP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_B
 ClientSampleId :
 DFTTP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_B\METHOD\8270-BB093016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 30 14:16:00 2016

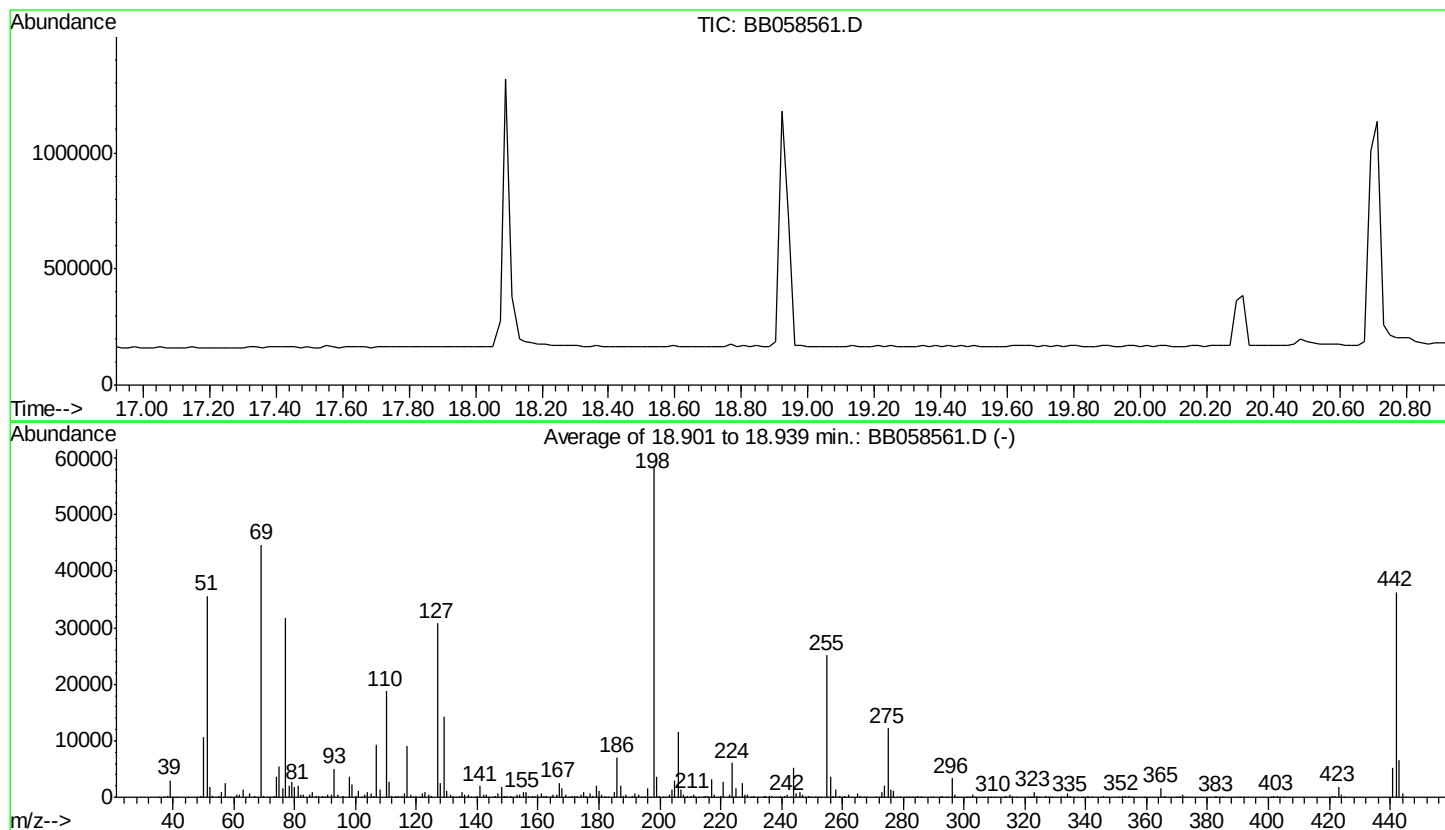

AutoFind: Scans 825, 826, 827; Background Corrected with Scan 821

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.7	35597	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	76.2	44689	PASS
70	69	0.00	2	0.4	167	PASS
127	198	10	80	52.5	30802	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58677	PASS
199	198	5	9	6.3	3690	PASS
275	198	10	60	20.7	12169	PASS
365	198	1	100	2.8	1656	PASS
441	442	0.01	24	14.2	5149	PASS
442	198	50	100	61.8	36289	PASS
443	442	15	24	18.4	6662	PASS