


Data Path : Z:\HPCHEM1\BNA B\DATA\BB093016\
 Data File : BB058570.D
 Acq On : 30 Sep 2016 15:29
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_B
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_B\METHOD\8270-BB093016.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Sep 30 14:16:00 2016

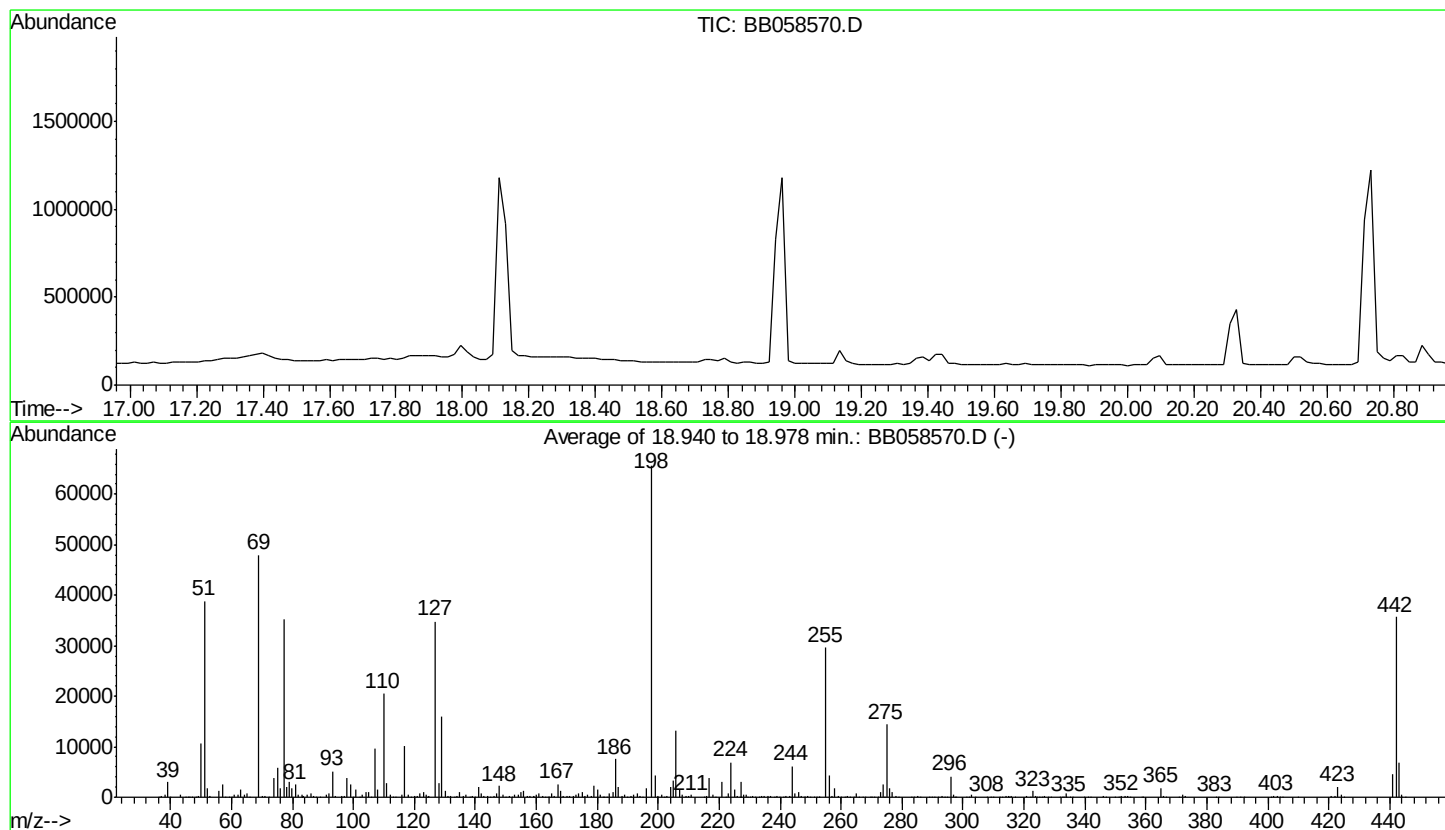

AutoFind: Scans 827, 828, 829; Background Corrected with Scan 822

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.2	38854	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	73.0	47917	PASS
70	69	0.00	2	0.3	142	PASS
127	198	10	80	53.0	34816	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	65655	PASS
199	198	5	9	6.5	4294	PASS
275	198	10	60	21.8	14336	PASS
365	198	1	100	2.7	1790	PASS
441	442	0.01	24	13.0	4647	PASS
442	198	50	100	54.3	35633	PASS
443	442	15	24	19.1	6803	PASS