

Data Path : Z:\HPCHEM1\BNA_B\DATA\BB101916\
 Data File : BB058666.D
 Acq On : 20 Oct 2016 00:15
 Operator : UM/SJ
 Sample : MDL-05-S-ML
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_B
 ClientSampleId :
 MDL-05-S-ML

Manual Integrations
 APPROVED

umangi
 10/20/2016 5:02:59 PM

Quant Time: Oct 20 16:23:05 2016
 Quant Method : Z:\HPCHEM1\BNA_B\METHOD\SOM02.2-EPA-BB101916-MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 04:39:59 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.68	152	564046	20.00	ng/ul	0.00
7) Naphthalene-d8	11.62	136	2214068	20.00	ng/ul	0.00
13) Acenaphthene-d10	15.57	164	1213077	20.00	ng/ul	-0.02
18) Phenanthrene-d10	18.42	188	1982361	20.00	ng/ul	0.00
23) Chrysene-d12	22.79	240	1990233	20.00	ng/ul	0.00
25) Perylene-d12	25.85	264	1352582	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.67	96	95453	7.35	ng/uL	0.02
3) Phenol-d5	7.81	99	1378110	31.92	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	7.96	67	1053088	34.63	ng/ul	0.00
5) 2-Chlorophenol-d4	8.20	132	1339235	31.27	ng/ul	0.00
6) 4-Methylphenol-d8	9.45	113	1072933	30.86	ng/ul	0.00
8) Nitrobenzene-d5	9.89	128	692261	31.28	ng/ul	0.00
9) 2-Nitrophenol-d4	10.66	143	737408	30.64	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	11.24	165	971427	29.31	ng/ul	0.00
11) 4-Chloroaniline-d4	11.76	131	1443548	34.07	ng/ul	0.00
14) Dimethylphthalate-d6	14.95	166	2532319	31.52	ng/ul	0.00
15) Acenaphthylene-d8	15.26	160	3190660	33.78	ng/ul	0.00
16) 4-Nitrophenol-d4	15.76	143	516308	28.51	ng/ul	-0.02
17) Fluorene-d10	16.61	176	2220278	33.94	ng/ul	0.00
19) 4,6-Dinitro-2-methylphenol	16.72	200	497747	23.90	ng/ul	0.00
20) Anthracene-d10	18.51	188	2718671m	30.17	ng/ul	0.10
24) Pyrene-d10	20.86	212	3074625	34.70	ng/ul	0.00
26) Benzo(a)pyrene-d12	25.66	264	1962933	32.20	ng/ul	0.00

Target Compounds					Qvalue
12) 1-Methylnaphthalene	13.55	142	213309m	3.05	ng/ul
21) 1,2,3,4-Tetrachlorobenzene	14.34	216	90400	2.58	ng/uL
22) Pentachlorobenzene	15.92	250	83494	2.44	ng/uL

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_B\DATA\BB101916\
Data File : BB058666.D
Acq On : 20 Oct 2016 00:15
Operator : UM/SJ
Sample : MDL-05-S-ML
Misc :
ALS Vial : 20 Sample Multiplier: 1


Instrument :
BNA_B
ClientSampleId :
MDL-05-S-ML

Manual Integrations
APPROVED

umangi
10/20/2016 5:02:59 PM

Quant Time: Oct 20 16:23:05 2016
Quant Method : Z:\HPCHEM1\BNA_B\METHOD\SOM02.2-EPA-BB101916-MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 04:39:59 2016
Response via : Initial Calibration

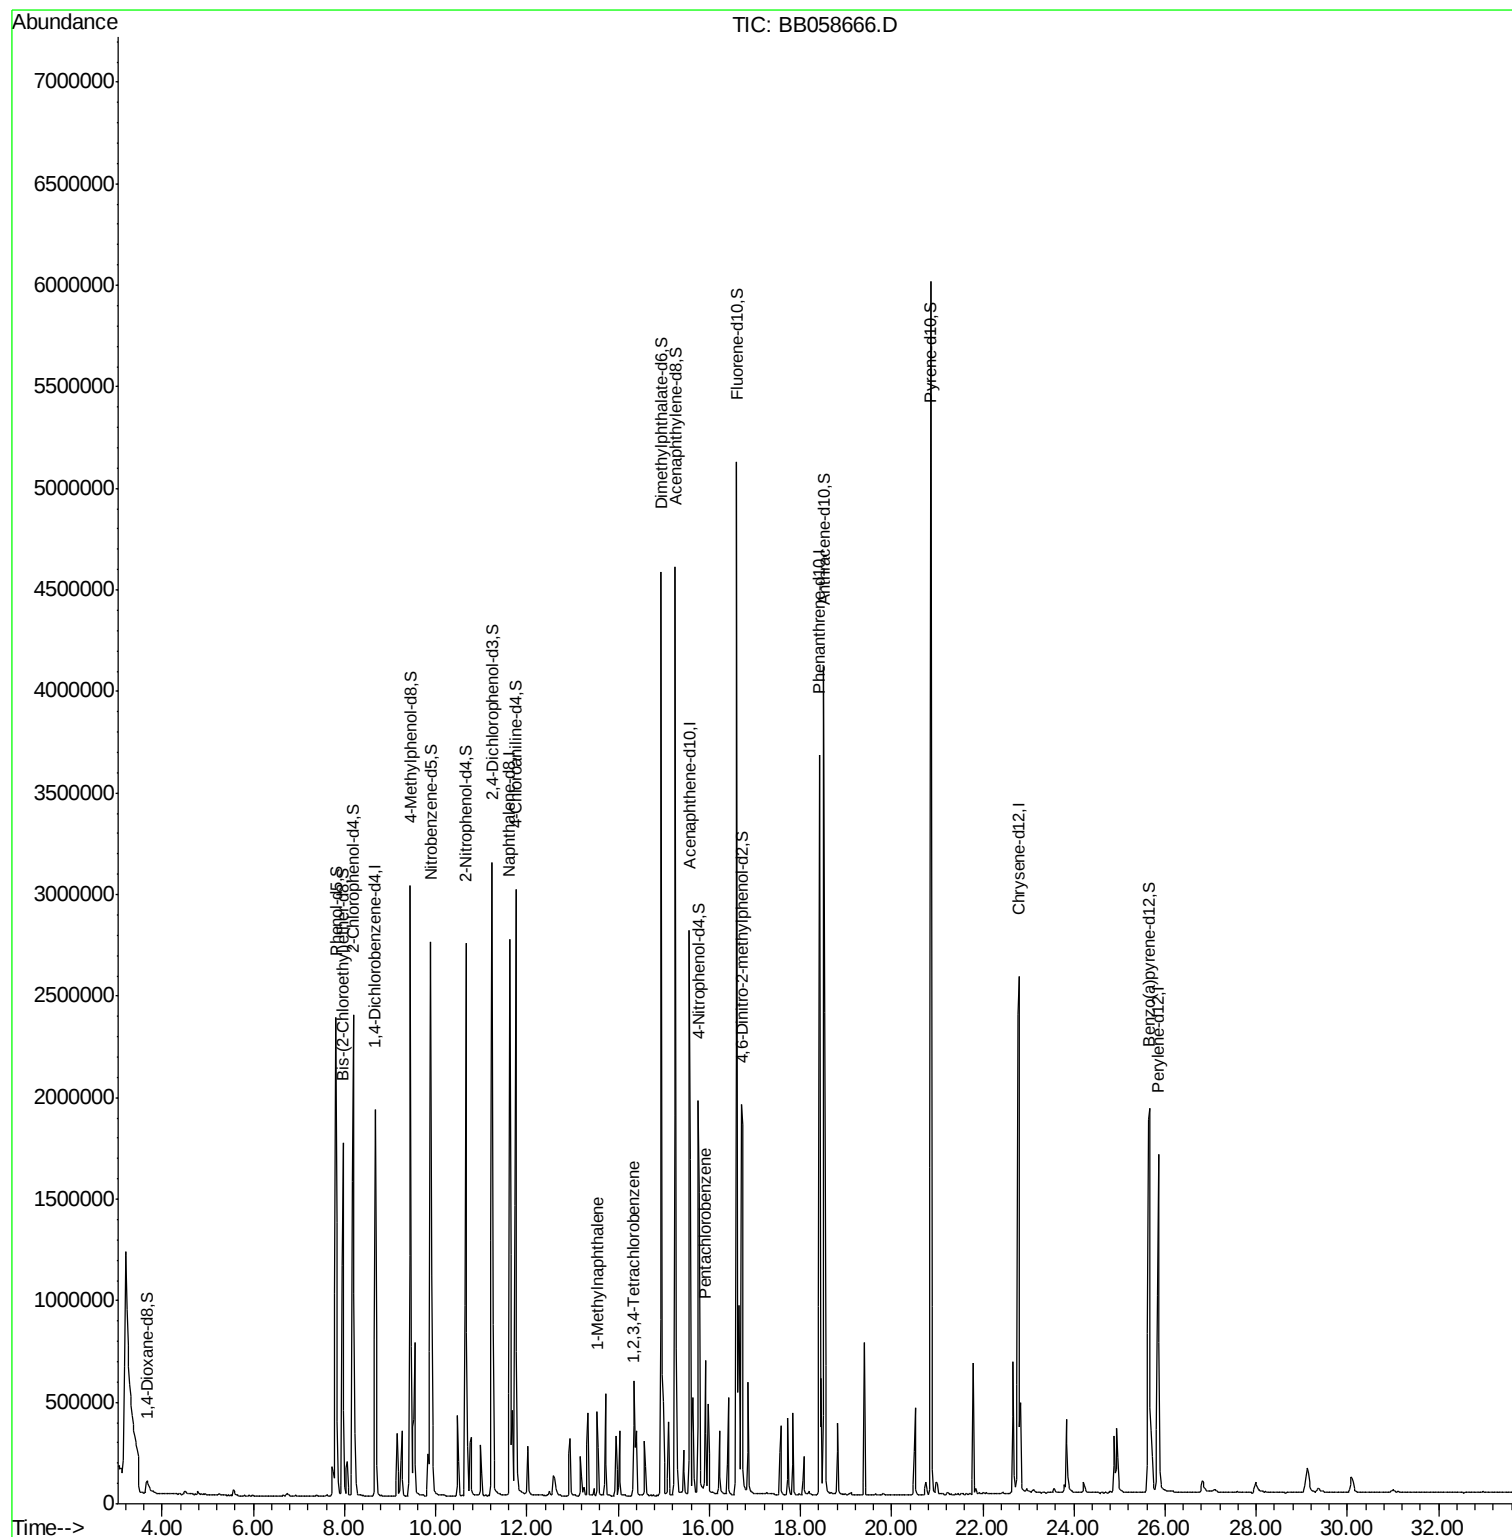

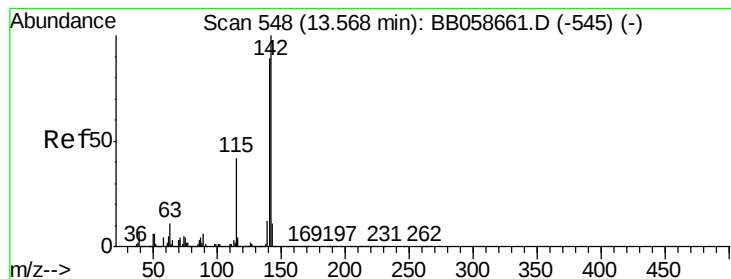

#12

1-Methylnaphthalene

Concen: 3.05 ng/uL m

RT: 13.55 min Scan# 547

Delta R.T. -0.02 min

Lab File: BB058666.D

Acq: 20 Oct 2016 00:15

Instrument :

BNA_B





ClientSampled :

MDL-05-S-ML

Tgt Ion:	142	Resp:	213309
Ion Ratio	Lower	Upper	
142	100		
141	87.6	74.9	112.3
116	5.2	3.1	4.7#

Manual Integrations
APPROVED

umangi
10/20/2016 5:02:59 PM

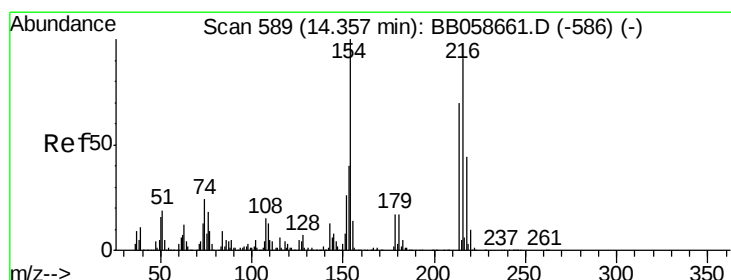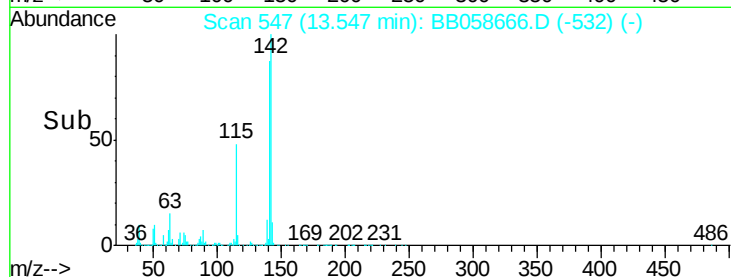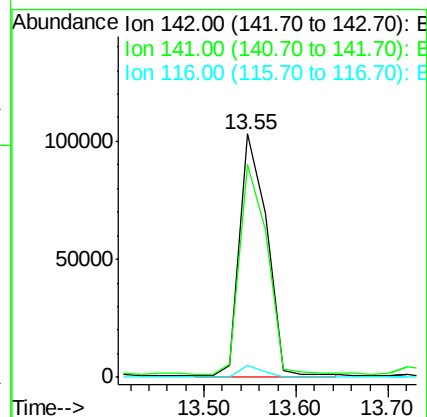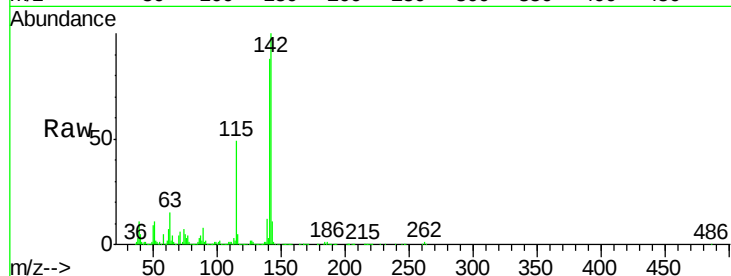

#21

1,2,3,4-Tetrachlorobenzene

Concen: 2.58 ng/uL




RT: 14.34 min Scan# 588




Delta R.T. -0.02 min

Lab File: BB058666.D

Acq: 20 Oct 2016 00:15

Tgt Ion:	216	Resp:	90400
Ion Ratio	Lower	Upper	
216	100		
214	80.2	62.5	93.7
218	45.7	38.4	57.6

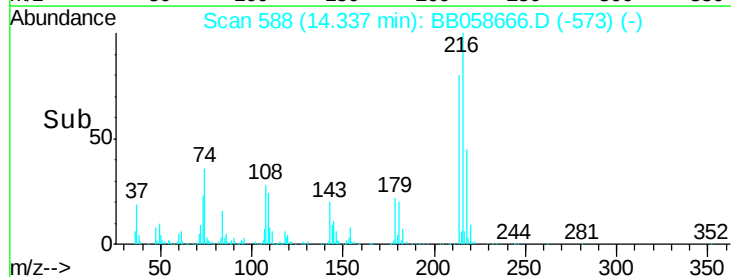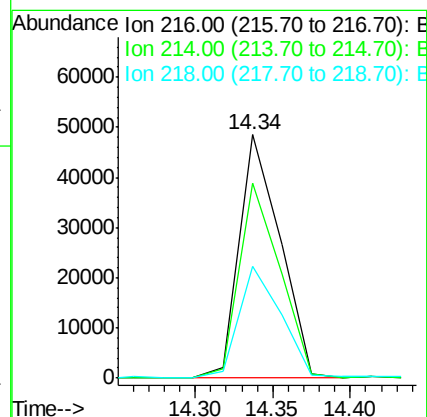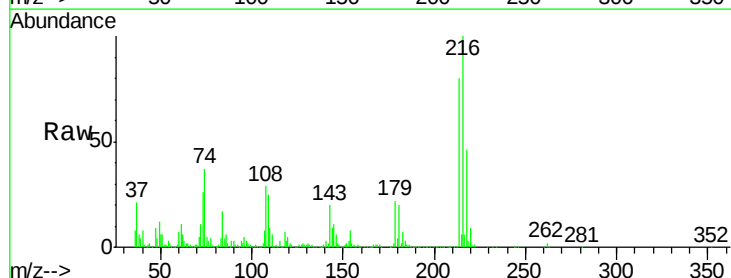

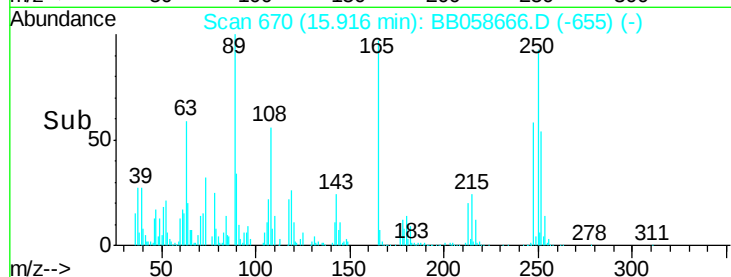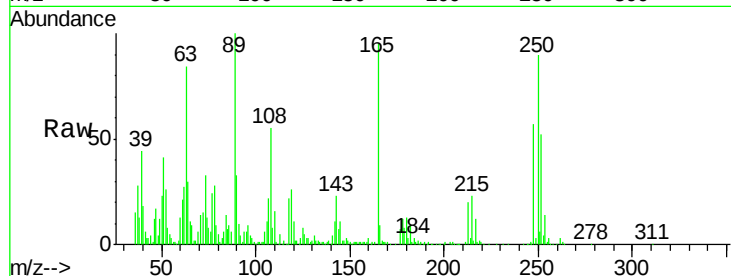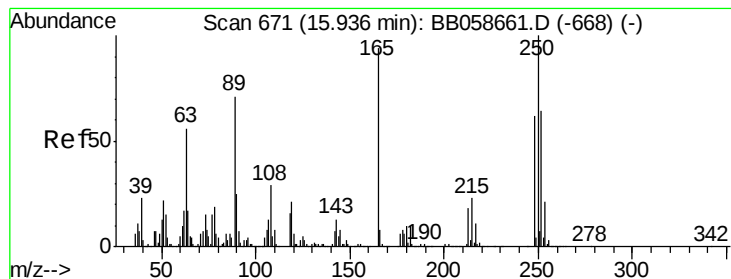

#22

Pentachlorobenzene

Concen: 2.44 ng/uL

RT: 15.92 min Scan# 670

Delta R.T. -0.02 min

Lab File: BB058666.D

Acq: 20 Oct 2016 00:15

Tgt Ion:	250	Resp:	83494
Ion Ratio	Lower	Upper	
250	100		
248	66.6	50.6	75.8
252	58.0	51.4	77.0

Instrument :

BNA_B

ClientSampleId :

MDL-05-S-ML

Manual Integrations
APPROVED

umangi
10/20/2016 5:02:59 PM

