

Data Path : Z:\HPCHEM1\BNA_B\DATA\BB102016\
 Data File : BB058675.D
 Acq On : 20 Oct 2016 11:29
 Operator : UM/SJ
 Sample : MDL-02-W
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_B
 ClientSampleId :
 MDL-02-W

Manual Integrations
 APPROVED

sohil
 10/21/2016 12:56:57 PM

Quant Time: Oct 20 16:30:32 2016
 Quant Method : Z:\HPCHEM1\BNA_B\METHOD\SOM02.2-EPA-BB101916-MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Oct 20 16:25:04 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	8.68	152	570004	20.00	ng/ul	0.00
7) Naphthalene-d8	11.62	136	2269916	20.00	ng/ul	-0.02
13) Acenaphthene-d10	15.57	164	1231596	20.00	ng/ul	-0.02
18) Phenanthrene-d10	18.42	188	2012484	20.00	ng/ul	0.00
23) Chrysene-d12	22.77	240	1858603	20.00	ng/ul	-0.02
25) Perylene-d12	25.85	264	1327794	20.00	ng/ul	0.00

System Monitoring Compounds

2) 1,4-Dioxane-d8	3.65	96	115040	8.77	ng/uL	0.00
3) Phenol-d5	7.81	99	1684129	38.60	ng/ul	0.00
4) Bis-(2-Chloroethyl)ether-d	7.97	67	1275759	41.51	ng/ul	0.00
5) 2-Chlorophenol-d4	8.20	132	1632941	37.72	ng/ul	0.00
6) 4-Methylphenol-d8	9.45	113	1312734	37.36	ng/ul	-0.02
8) Nitrobenzene-d5	9.89	128	844128	37.20	ng/ul	0.00
9) 2-Nitrophenol-d4	10.66	143	908381	36.82	ng/ul	0.00
10) 2,4-Dichlorophenol-d3	11.24	165	1188710	34.99	ng/ul	0.00
11) 4-Chloroaniline-d4	11.76	131	1769610	40.74	ng/ul	0.00
14) Dimethylphthalate-d6	14.95	166	2973085	36.46	ng/ul	0.00
15) Acenaphthylene-d8	15.26	160	3772924	39.34	ng/ul	0.00
16) 4-Nitrophenol-d4	15.78	143	652565	35.49	ng/ul	0.00
17) Fluorene-d10	16.61	176	2784808	41.93	ng/ul	0.00
19) 4,6-Dinitro-2-methylphenol	16.73	200	594851	28.13	ng/ul	0.00
20) Anthracene-d10	18.52	188	3265527	35.70	ng/ul	0.00
24) Pyrene-d10	20.86	212	3759647	45.43	ng/ul	0.00
26) Benzo(a)pyrene-d12	25.66	264	2344855	39.18	ng/ul	0.02

Target Compounds					Qvalue
12) 1-Methylnaphthalene	13.55	142	236210m	3.29	ng/ul
21) 1,2,3,4-Tetrachlorobenzene	14.34	216	103248	2.91	ng/uL 98
22) Pentachlorobenzene	15.92	250	98111	2.83	ng/uL 99

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA_B\DATA\BB102016\
Data File : BB058675.D
Acq On : 20 Oct 2016 11:29
Operator : UM/SJ
Sample : MDL-02-W
Misc :
ALS Vial : 10 Sample Multiplier: 1


Instrument :
BNA_B
ClientSampleId :
MDL-02-W

Manual Integrations
APPROVED

sohil
10/21/2016 12:56:57 PM

Quant Time: Oct 20 16:30:32 2016
Quant Method : Z:\HPCHEM1\BNA_B\METHOD\SOM02.2-EPA-BB101916-MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Oct 20 16:25:04 2016
Response via : Initial Calibration

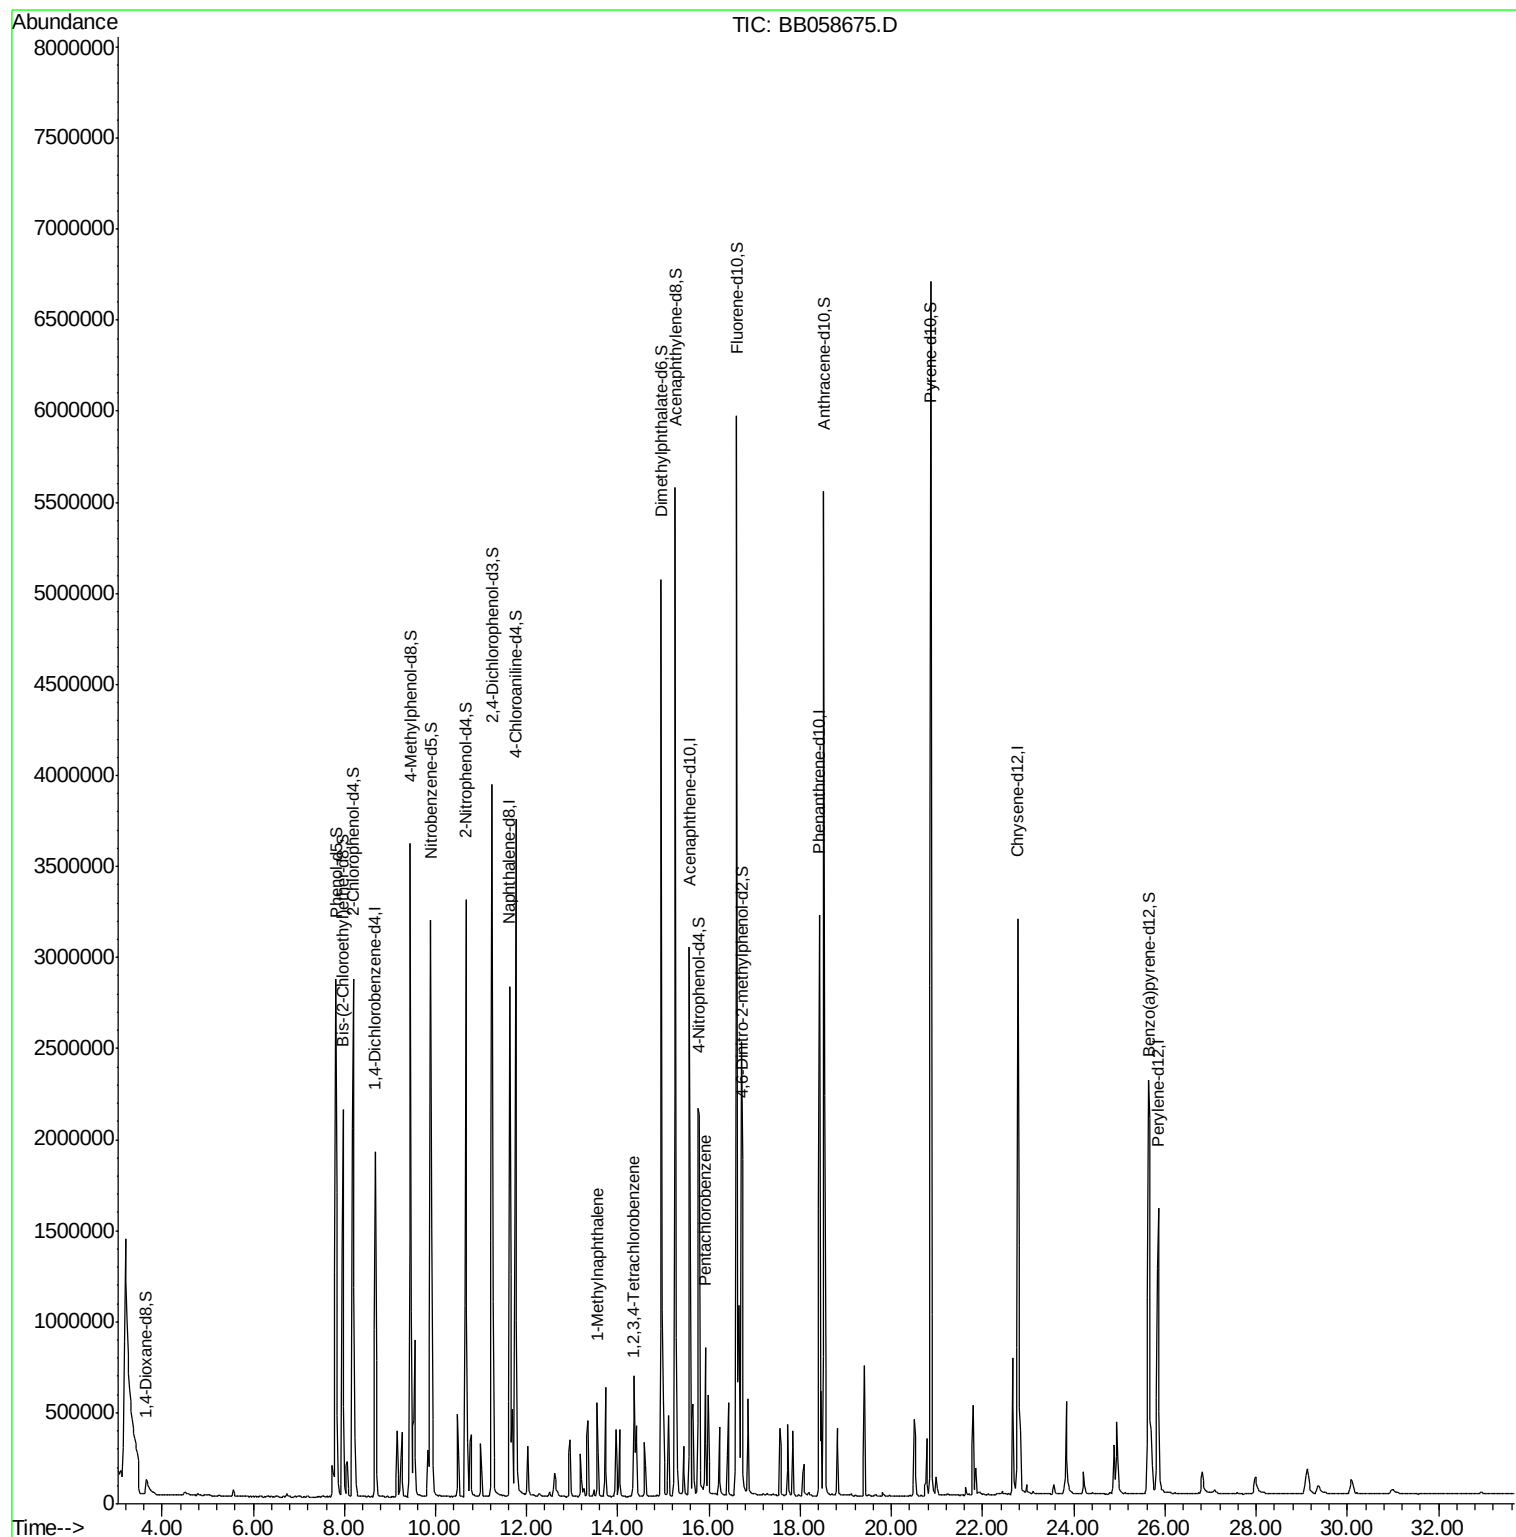

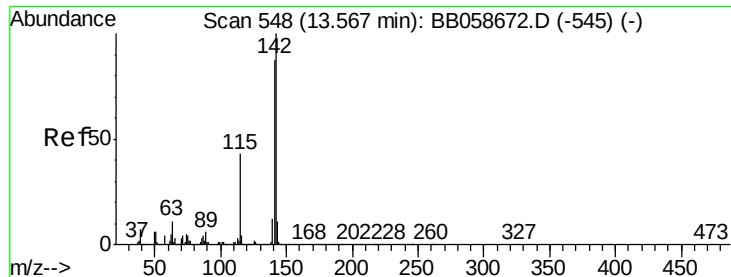

#12

1-Methylnaphthalene

Concen: 3.29 ng/ul m

RT: 13.55 min Scan# 547

Delta R.T. -0.02 min

Lab File: BB058675.D

Acq: 20 Oct 2016 11:29

Instrument :

BNA_B





ClientSampleId :

MDL-02-W

Tgt Ion:	142	Resp:	236210
Ion Ratio	Lower	Upper	
142	100		
141	93.7	74.9	112.3
116	4.9	3.1	4.7#

Manual Integrations
APPROVED

sohil
10/21/2016 12:56:57 PM

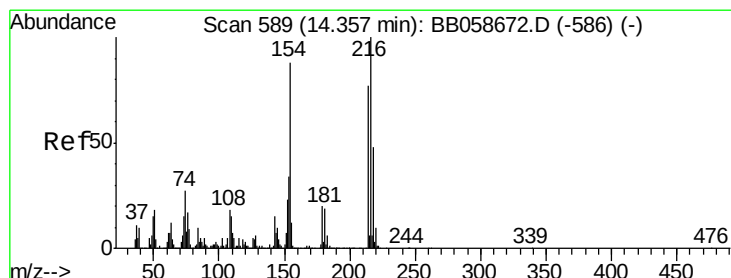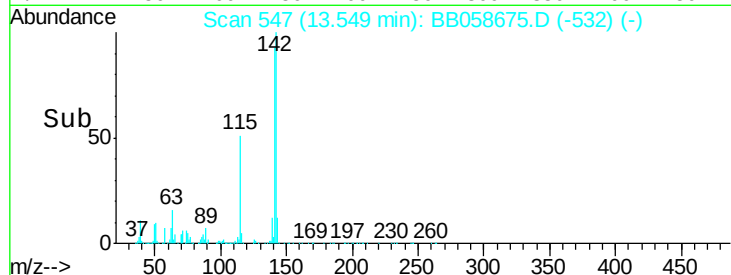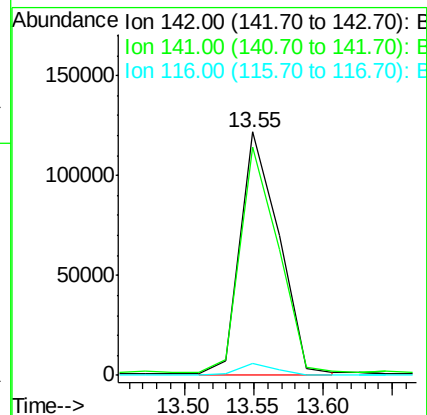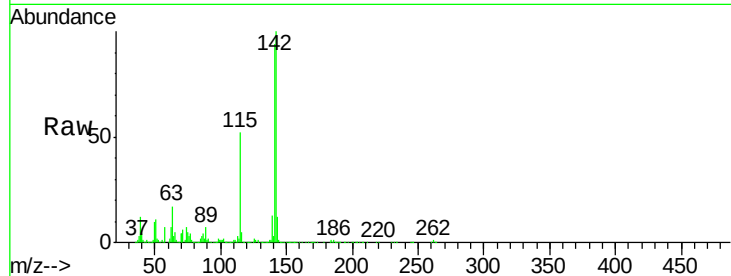

#21

1,2,3,4-Tetrachlorobenzene

Concen: 2.91 ng/uL




RT: 14.34 min Scan# 588




Delta R.T. -0.02 min

Lab File: BB058675.D

Acq: 20 Oct 2016 11:29

Tgt Ion:	216	Resp:	103248
Ion Ratio	Lower	Upper	
216	100		
214	79.9	62.5	93.7
218	46.4	38.4	57.6

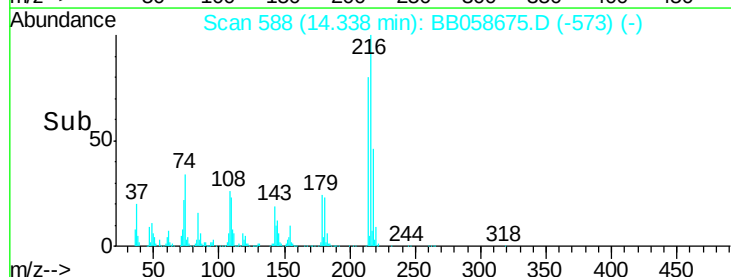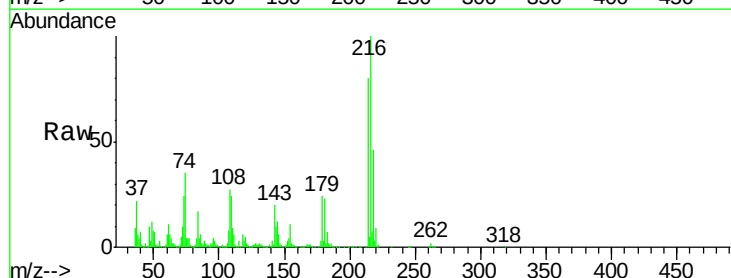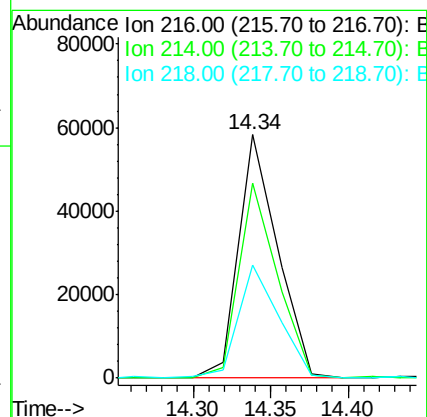

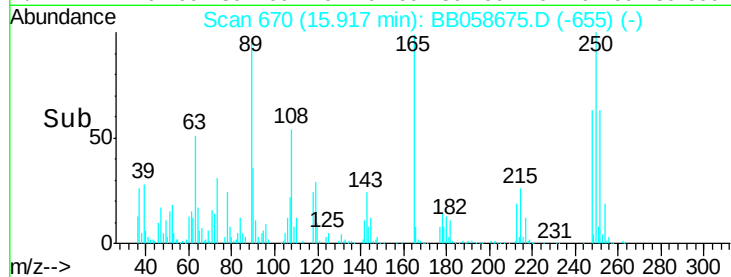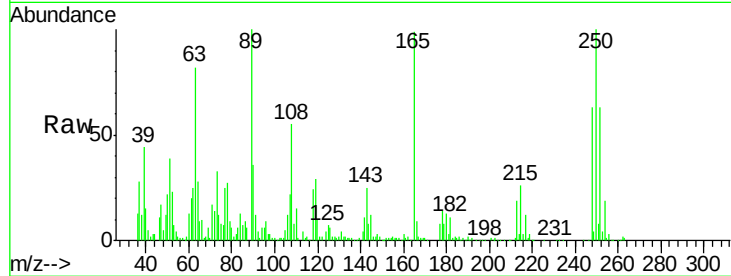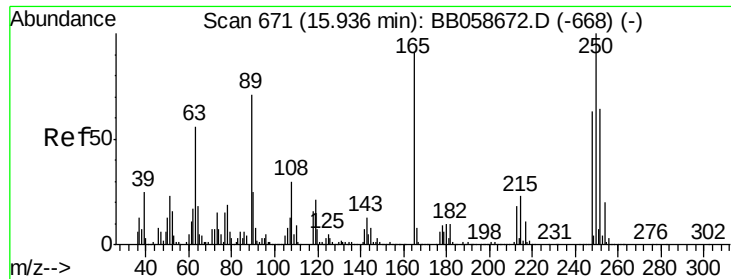

#22
 Pentachlorobenzene
 Concen: 2.83 ng/uL
 RT: 15.92 min Scan# 670
 Delta R.T. -0.02 min
 Lab File: BB058675.D
 Acq: 20 Oct 2016 11:29

Tgt Ion:	250	Resp:	98111
Ion Ratio	Lower	Upper	
250	100		
248	62.9	50.6	75.8
252	62.6	51.4	77.0

Instrument :
 BNA_B
 ClientSampleId :
 MDL-02-W

Manual Integrations
 APPROVED

sohil
 10/21/2016 12:56:57 PM

