


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE010219\  
 Data File : BE098599.D  
 Acq On : 2 Jan 2019 9:07  
 Operator : SJ/JU  
 Sample : DFTPP  
 Misc :  
 ALS Vial : 1 Sample Multiplier: 1

Instrument :  
 BNA\_E  
 ClientSampleId :  
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA\_E\METHODS\8270-SIM-BE121018.M  
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION  
 Last Update : Wed Jan 02 10:30:27 2019

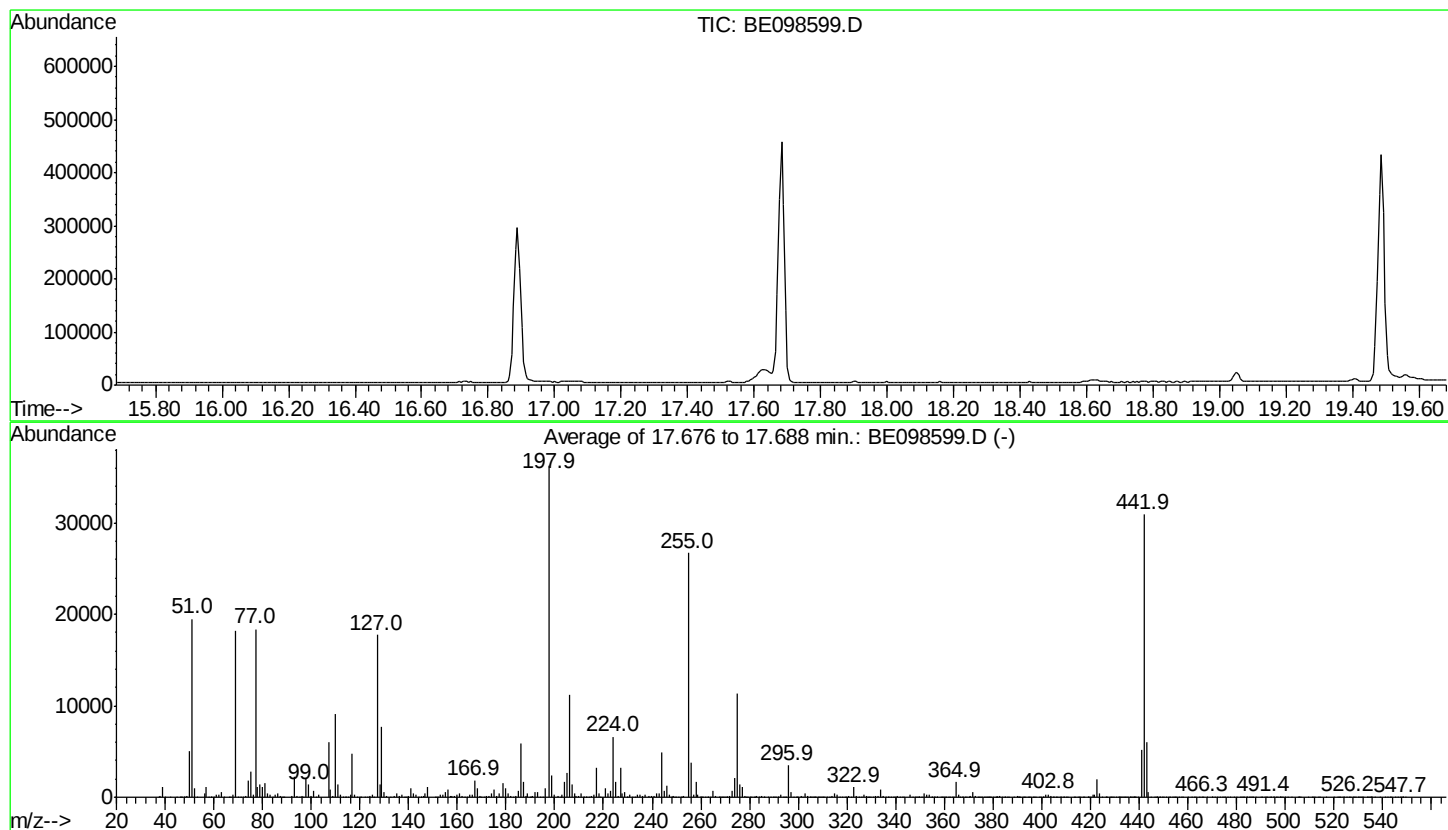

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2559

| Target Mass | Rel. to Mass | Lower Limit% | Upper Limit% | Rel. Abn% | Raw Abn | Result Pass/Fail |
|-------------|--------------|--------------|--------------|-----------|---------|------------------|
| 51          | 198          | 10           | 80           | 53.7      | 19465   | PASS             |
| 68          | 69           | 0.00         | 2            | 1.6       | 286     | PASS             |
| 69          | 198          | 0.00         | 100          | 50.2      | 18197   | PASS             |
| 70          | 69           | 0.00         | 2            | 0.4       | 72      | PASS             |
| 127         | 198          | 10           | 80           | 48.9      | 17729   | PASS             |
| 197         | 198          | 0.00         | 2            | 0.0       | 0       | PASS             |
| 198         | 198          | 100          | 100          | 100.0     | 36267   | PASS             |
| 199         | 198          | 5            | 9            | 6.5       | 2368    | PASS             |
| 275         | 198          | 10           | 60           | 31.2      | 11316   | PASS             |
| 365         | 198          | 1            | 100          | 4.6       | 1665    | PASS             |
| 441         | 198          | 0.01         | 100          | 14.4      | 5209    | PASS             |
| 442         | 198          | 50           | 100          | 85.2      | 30892   | PASS             |
| 443         | 442          | 15           | 24           | 19.6      | 6053    | PASS             |