


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE010419\
Data File : BE098613.D
Acq On : 4 Jan 2019 11:46
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE121018.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Wed Jan 02 10:30:27 2019

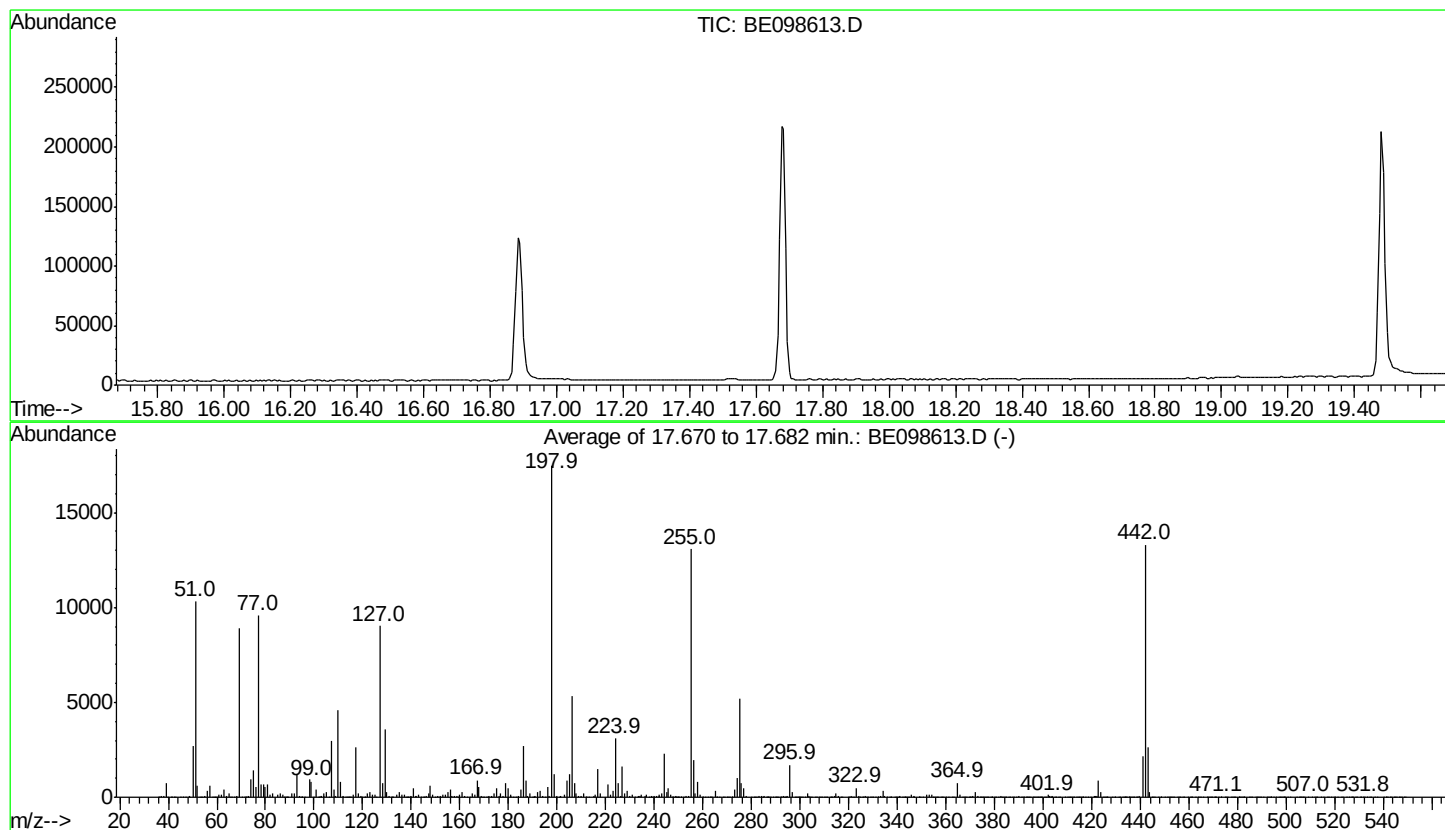

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2561

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.0	10311	PASS
68	69	0.00	2	0.8	74	PASS
69	198	0.00	100	50.8	8877	PASS
70	69	0.00	2	0.4	32	PASS
127	198	10	80	51.6	9020	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	17473	PASS
199	198	5	9	7.1	1238	PASS
275	198	10	60	29.6	5178	PASS
365	198	1	100	4.3	754	PASS
441	198	0.01	100	12.5	2192	PASS
442	198	50	100	76.2	13307	PASS
443	442	15	24	19.6	2603	PASS