


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE010920\
 Data File : BE101009.D
 Acq On : 9 Jan 2020 12:17
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 18:36:25 2020

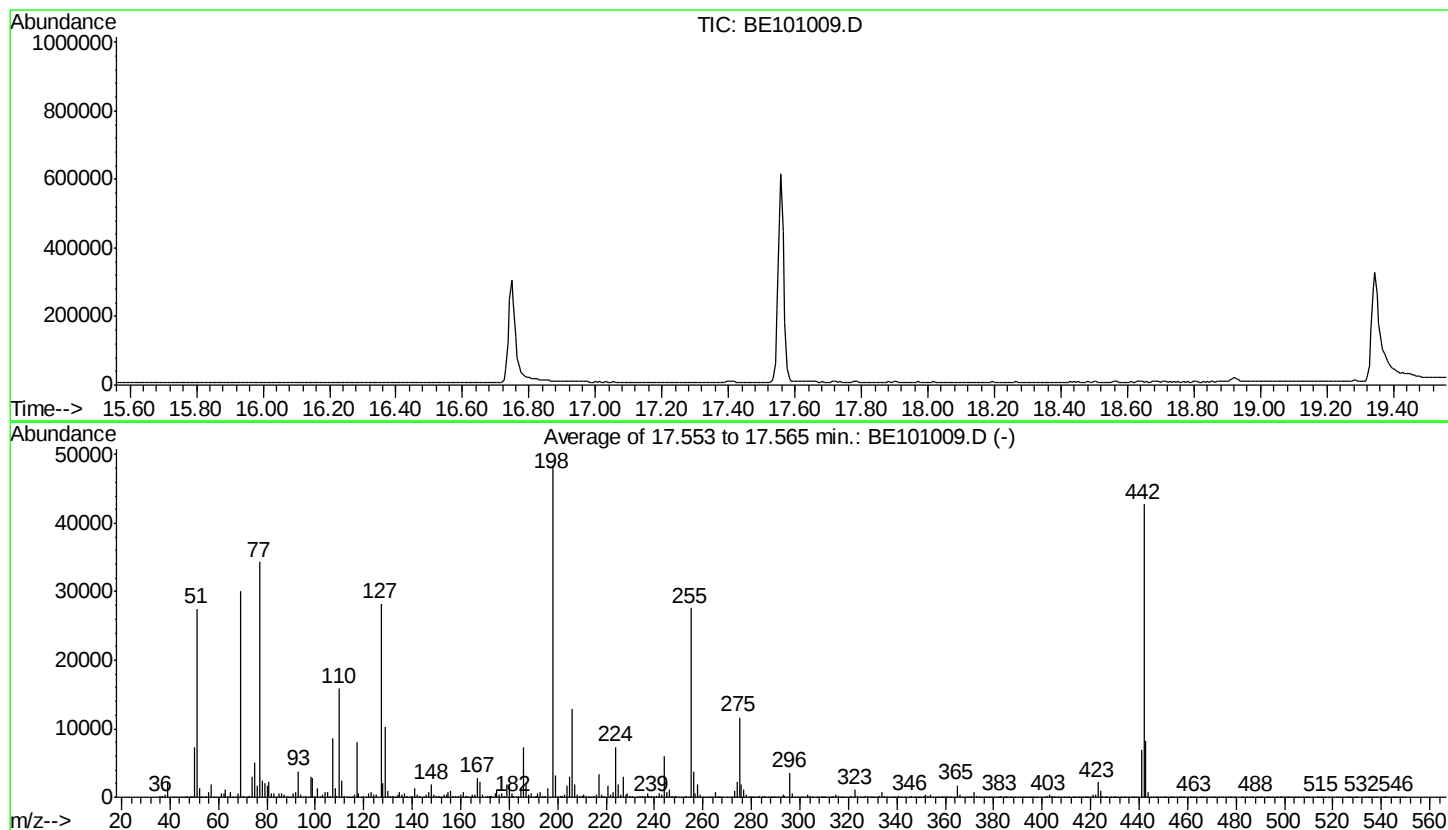

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2538

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.8	27499	PASS
68	69	0.00	2	1.6	487	PASS
69	198	0.00	100	62.1	30071	PASS
70	69	0.00	2	0.6	192	PASS
127	198	10	80	58.3	28216	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	48402	PASS
199	198	5	9	6.6	3211	PASS
275	198	10	60	24.0	11606	PASS
365	198	1	100	3.5	1691	PASS
441	198	0.01	100	14.4	6950	PASS
442	198	50	100	88.3	42749	PASS
443	442	15	24	19.3	8233	PASS