
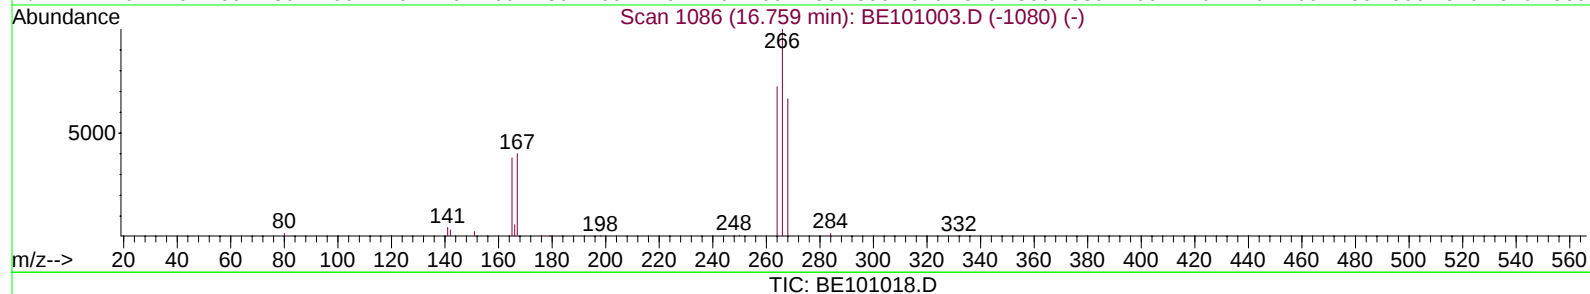
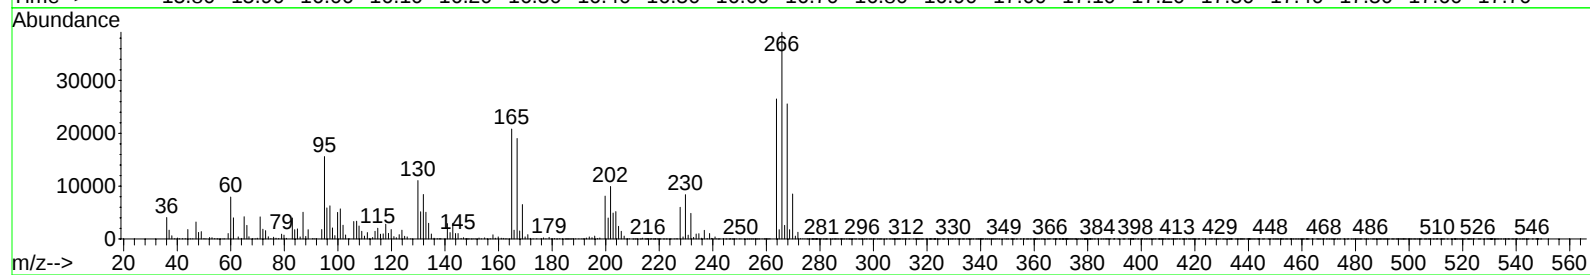


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE011020\
Data File : BE101018.D
Acq On : 10 Jan 2020 9:50
Operator : JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 10 18:01:36 2020
Quant Method : Z:\svoasrv\HPCHEM1\BNA E\Methods\8270-SIM-BE010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 18:36:25 2020
Response via : Initial Calibration

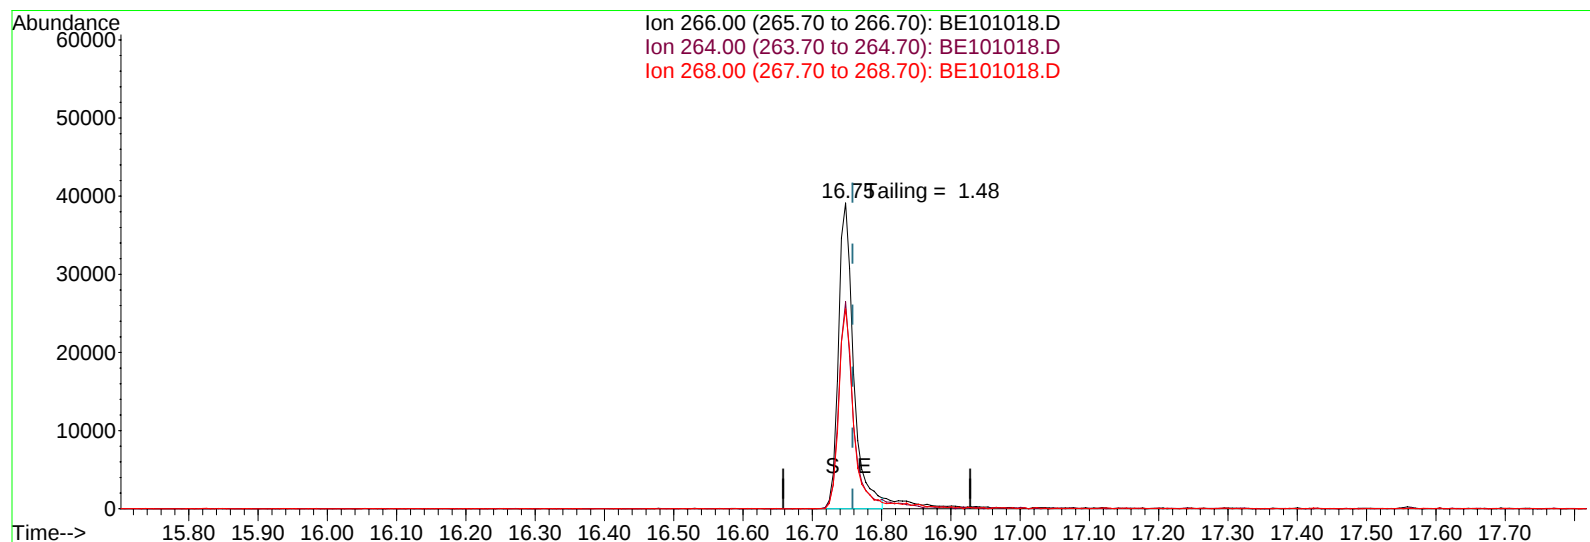

(22) Pentachlorophenol

16.748min (-0.010) 8521.43ng

response 60617

Ion	Exp%	Act%
266.00	100	100
264.00	76.20	67.72
268.00	73.10	69.80
0.00	0.00	0.00