


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE011020\
 Data File : BE101018.D
 Acq On : 10 Jan 2020 9:50
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_E\Methods\8270-SIM-BE010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 18:36:25 2020

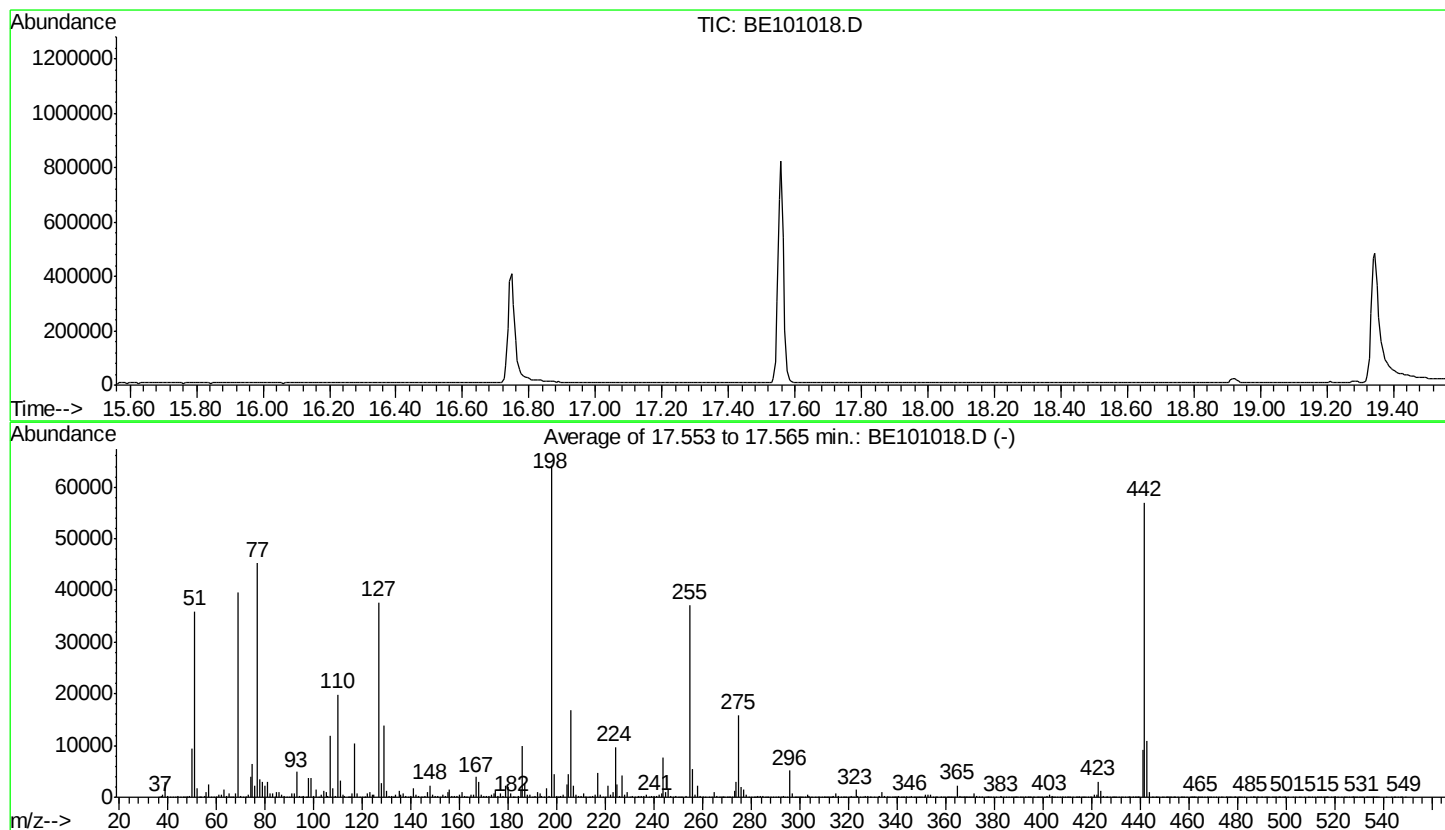

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2538

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.0	35920	PASS
68	69	0.00	2	1.8	733	PASS
69	198	0.00	100	62.0	39748	PASS
70	69	0.00	2	0.6	225	PASS
127	198	10	80	58.7	37666	PASS
197	198	0.00	2	0.3	166	PASS
198	198	100	100	100.0	64144	PASS
199	198	5	9	6.9	4455	PASS
275	198	10	60	24.8	15926	PASS
365	198	1	100	3.6	2332	PASS
441	198	0.01	100	14.3	9150	PASS
442	198	50	100	89.0	57058	PASS
443	442	15	24	19.2	10965	PASS