


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE011120\
 Data File : BE101025.D
 Acq On : 10 Jan 2020 16:22
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 18:36:25 2020

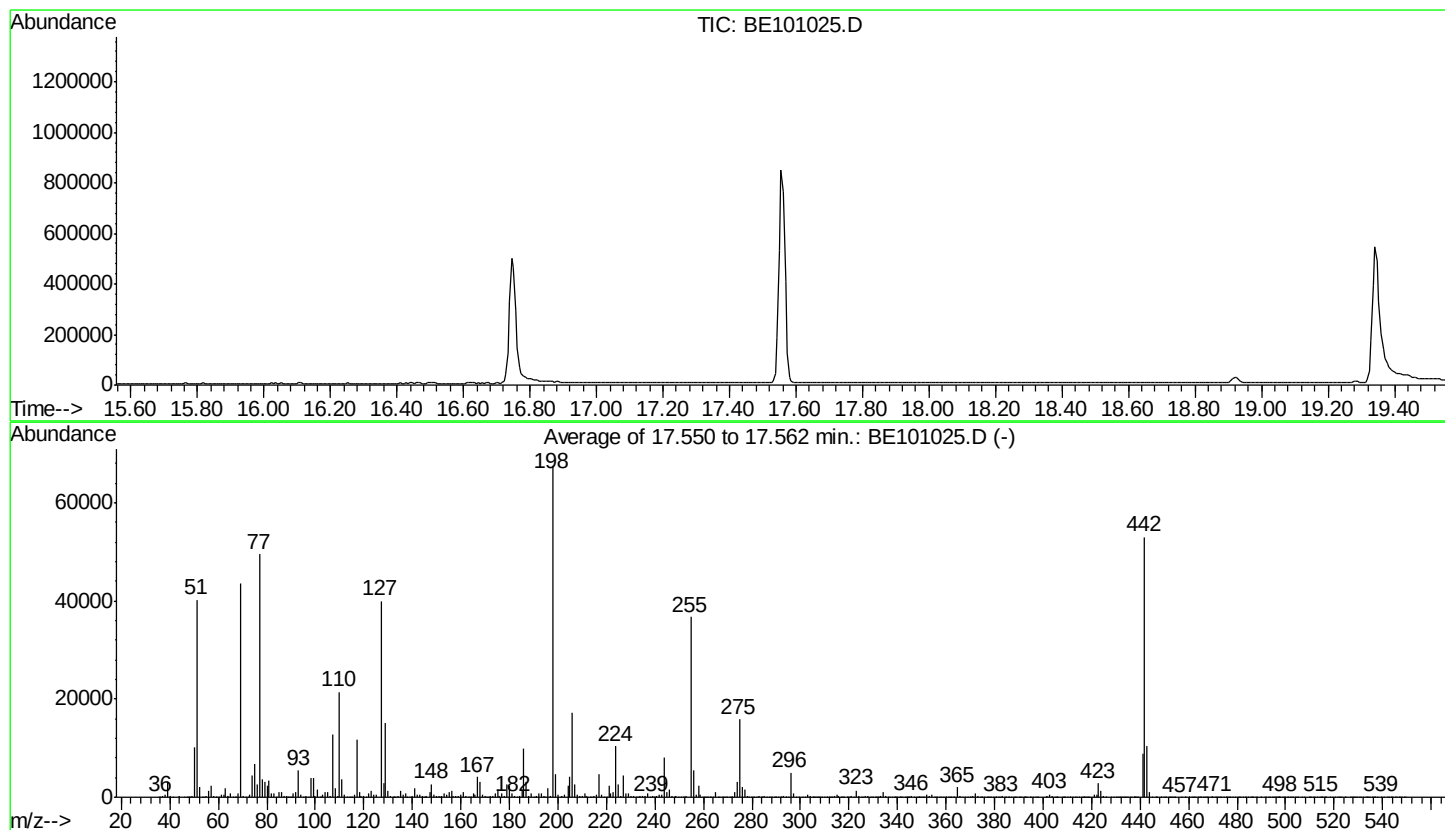

AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2537

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	59.6	40258	PASS
68	69	0.00	2	1.7	727	PASS
69	198	0.00	100	64.5	43591	PASS
70	69	0.00	2	0.4	192	PASS
127	198	10	80	59.1	39957	PASS
197	198	0.00	2	0.3	193	PASS
198	198	100	100	100.0	67603	PASS
199	198	5	9	6.8	4588	PASS
275	198	10	60	23.5	15866	PASS
365	198	1	100	3.1	2065	PASS
441	198	0.01	100	13.3	9000	PASS
442	198	50	100	78.5	53085	PASS
443	442	15	24	19.8	10502	PASS