


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE011320\
 Data File : BE101034.D
 Acq On : 13 Jan 2020 10:14
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 18:36:25 2020

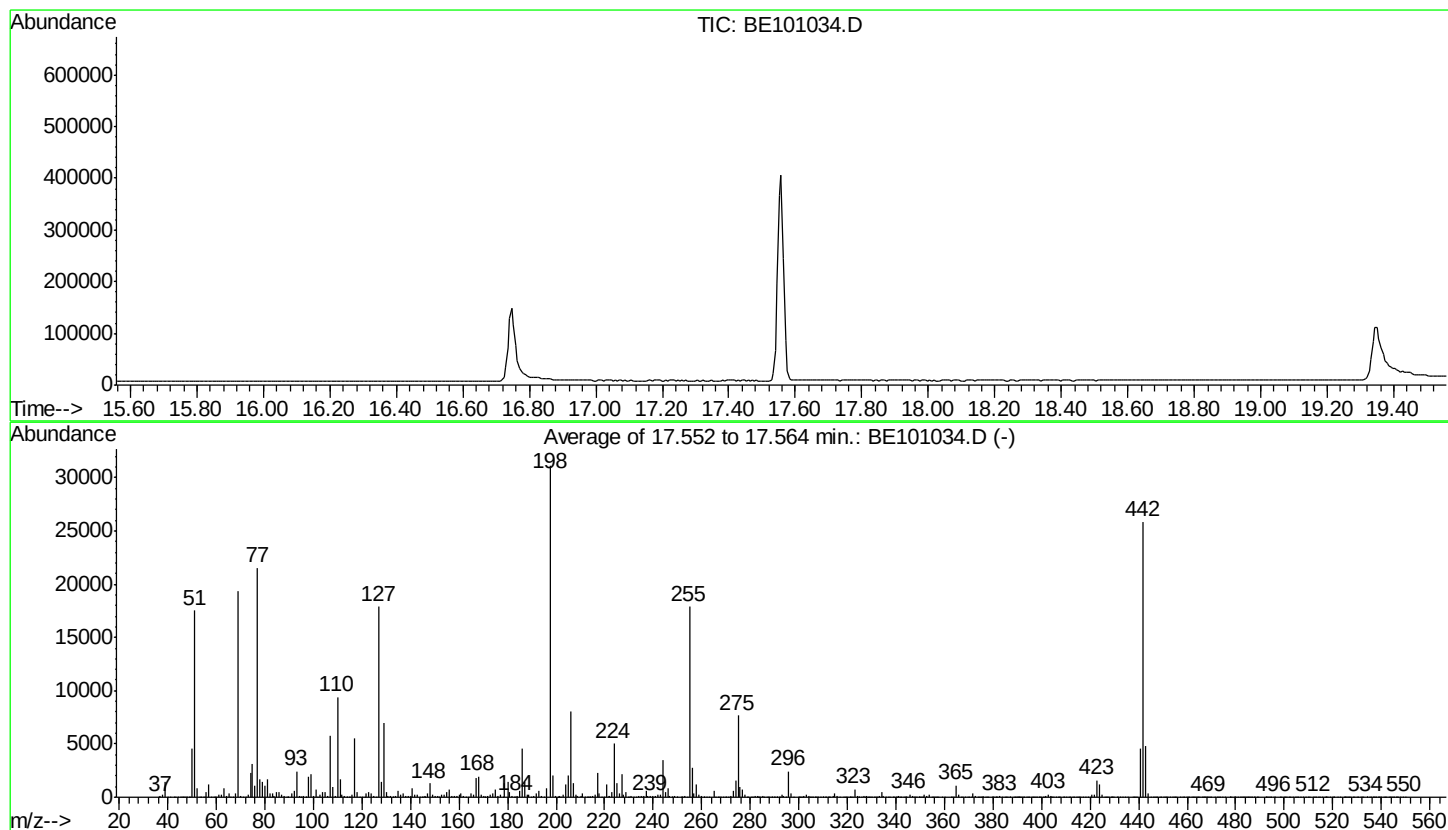

AutoFind: Scans 2547, 2548, 2549; Background Corrected with Scan 2537

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.3	17520	PASS
68	69	0.00	2	1.9	359	PASS
69	198	0.00	100	62.0	19288	PASS
70	69	0.00	2	0.5	93	PASS
127	198	10	80	57.5	17890	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	31122	PASS
199	198	5	9	6.8	2104	PASS
275	198	10	60	24.6	7667	PASS
365	198	1	100	3.5	1088	PASS
441	198	0.01	100	14.6	4554	PASS
442	198	50	100	83.2	25888	PASS
443	442	15	24	18.5	4782	PASS