

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011420\
 Data File : BE101049.D
 Acq On : 14 Jan 2020 12:32
 Operator : JU
 Sample : PB126047BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :

Quant Time: Jan 14 20:41:50 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE010820.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Jan 08 18:36:25 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.72	152	2903	0.40	ng	0.00
7) Naphthalene-d8	10.51	136	12657	0.40	ng	0.01
13) Acenaphthene-d10	14.36	164	8446	0.40	ng	0.00
19) Phenanthrene-d10	17.09	188	19923	0.40	ng	0.00
27) Chrysene-d12	21.27	240	18244	0.40	ng	-0.01
34) Perylene-d12	23.69	264	19872	0.40	ng	-0.01
System Monitoring Compounds						
4) 2-Fluorophenol	5.34	112	1681	0.26	ng	0.00
5) Phenol-d6	6.93	99	1905	0.23	ng	0.01
8) Nitrobenzene-d5	8.90	82	1927	0.21	ng	0.03
11) 2-Methylnaphthalene-d10	12.11	152	6350	0.26	ng	0.00
14) 2,4,6-Tribromophenol	15.85	330	348	0.15	ng	0.00
15) 2-Fluorobiphenyl	13.00	172	10150	0.32	ng	0.00
25) Fluoranthene-d10	19.13	212	82759	0.30	ng	0.00
29) Terphenyl-d14	19.73	244	15260	0.34	ng	0.00
Target Compounds						
3) n-Nitrosodimethylamine	3.64	42	113	0.028	ng	# 1
22) Pentachlorophenol	16.80	266	26	0.257	ng	# 78
32) Bis(2-ethylhexyl)phthalate	21.20	149	7912	0.091	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011420\
Data File : BE101049.D
Acq On : 14 Jan 2020 12:32
Operator : JU
Sample : PB126047BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :

Quant Time: Jan 14 20:41:50 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE010820.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 08 18:36:25 2020
Response via : Initial Calibration

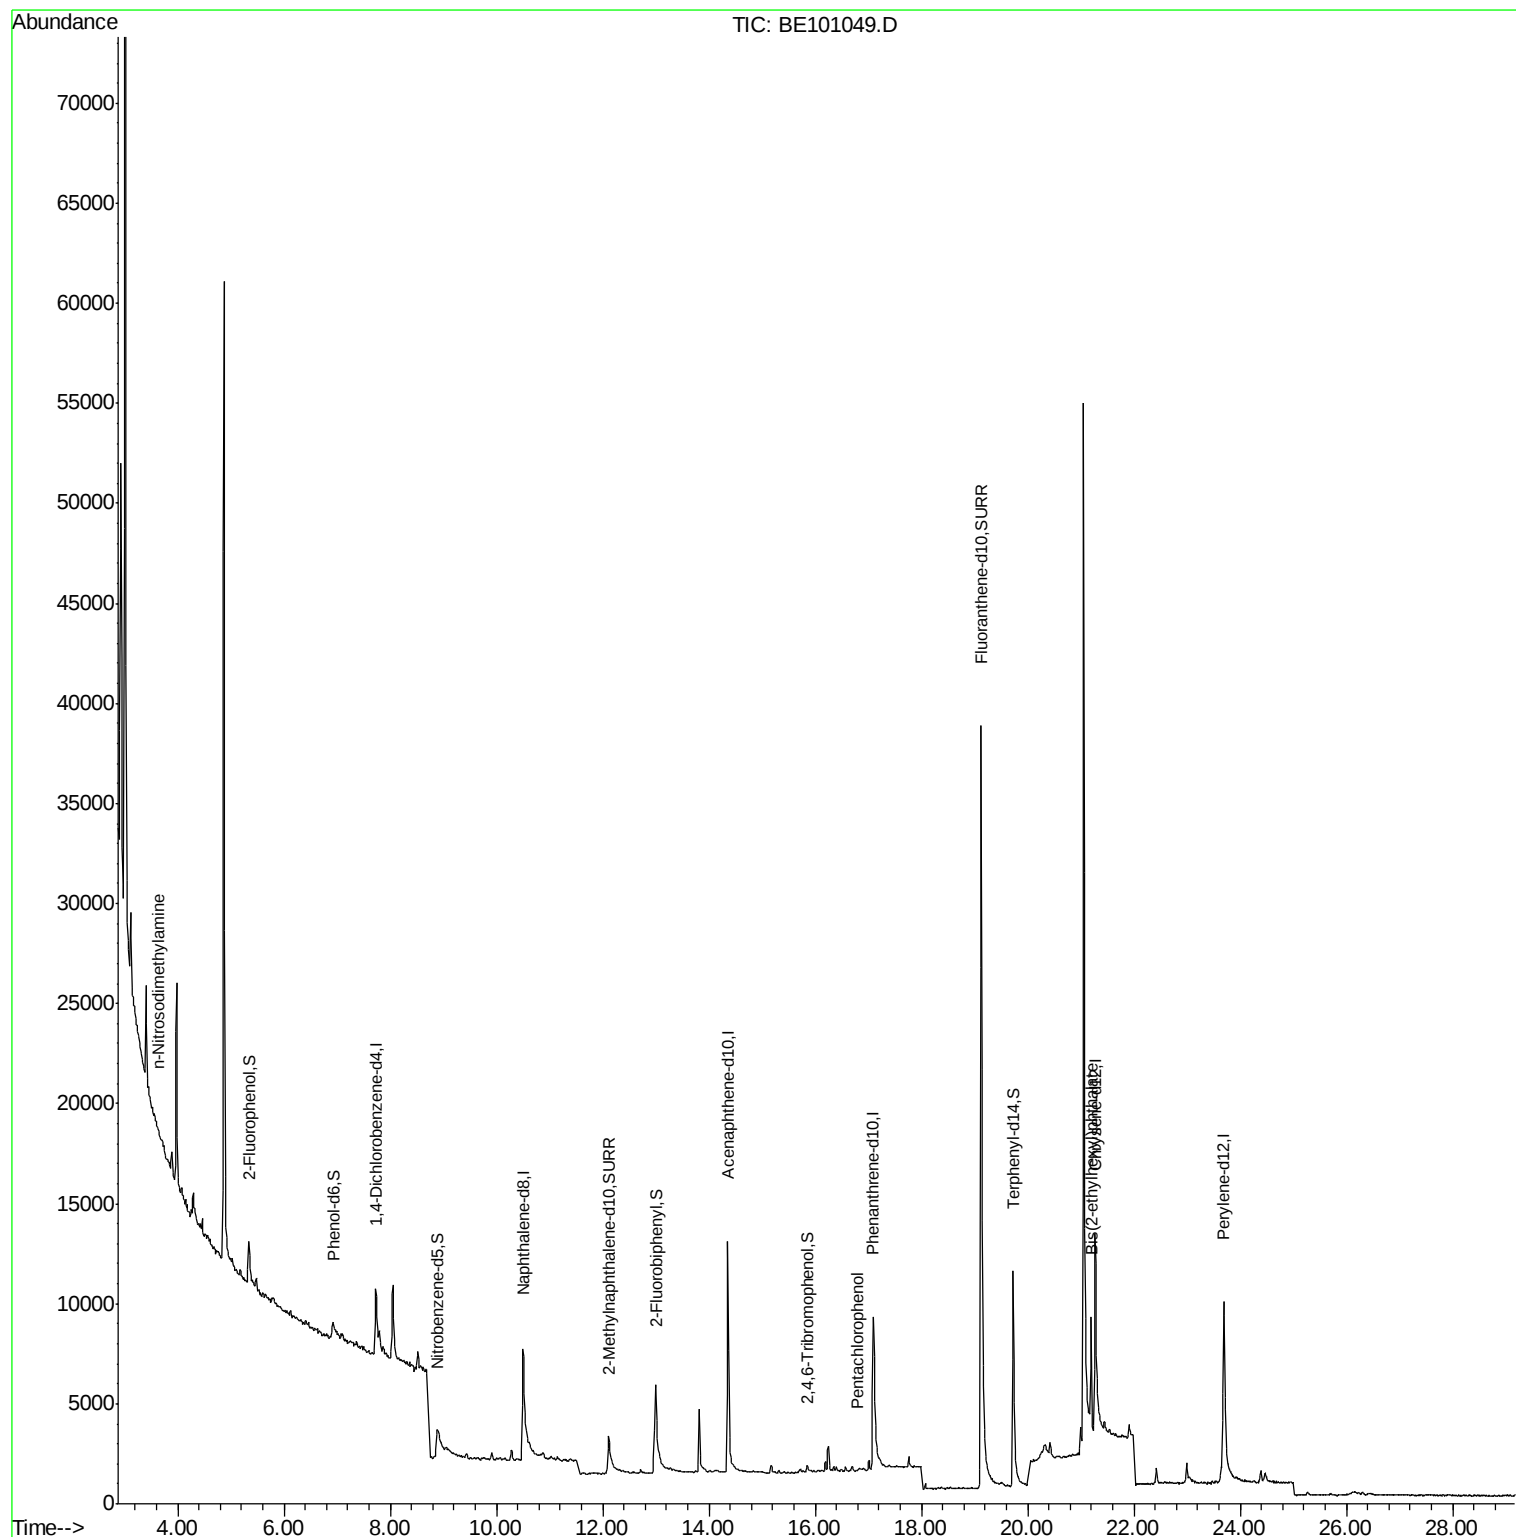

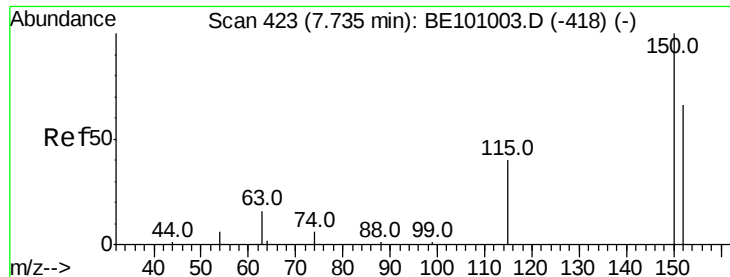


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.72 min Scan# 422
Delta R.T. -0.01 min
Lab File: BE101049.D
Acq: 14 Jan 2020 12:32

Instrument :
BNA_E
ClientSampleId :

Tot Ion:152 Resp: 2903
Ion Ratio Lower Upper
152 100
150 153.0 120.3 180.5
115 75.8 51.7 77.5

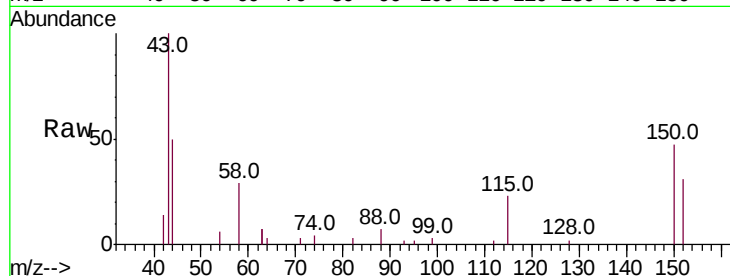


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

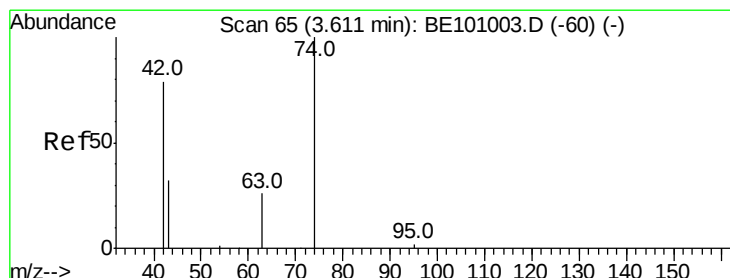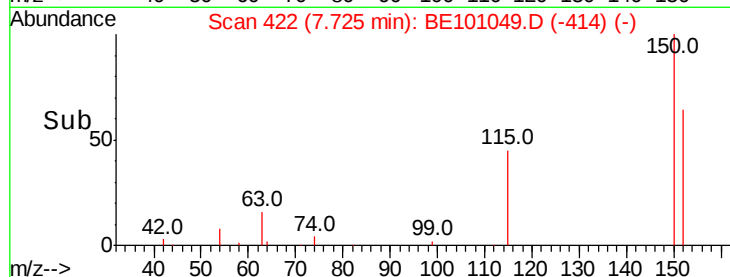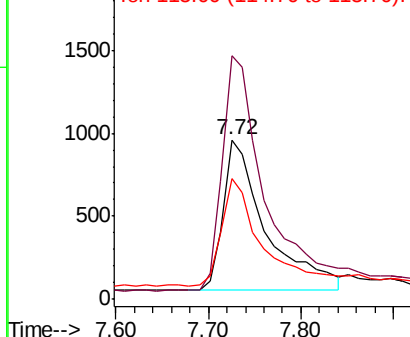



#3


n-Nitrosodimethylamine
Concen: 0.028 ng
RT: 3.64 min Scan# 67
Delta R.T. 0.02 min
Lab File: BE101049.D
Acq: 14 Jan 2020 12:32

Tgt Ion: 42 Resp: 113
Ion Ratio Lower Upper
42 100
74 7.1 105.7 158.5#
44 0.0 10.0 15.0#

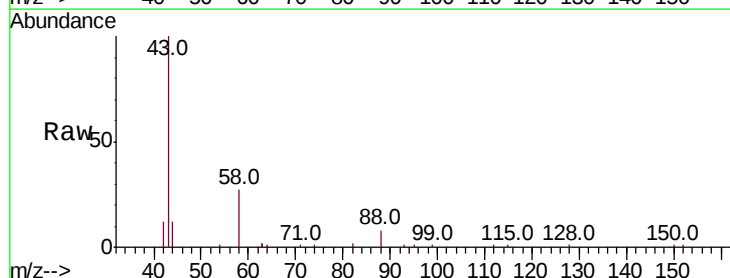

Abundance Ion 42.00 (41.70 to 42.70): BE1
Ion 74.00 (73.70 to 74.70): BE1
Ion 44.00 (43.70 to 44.70): BE1

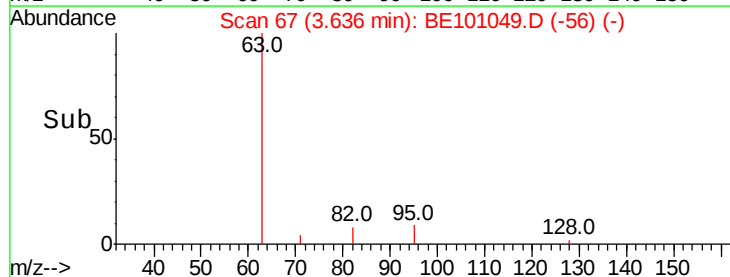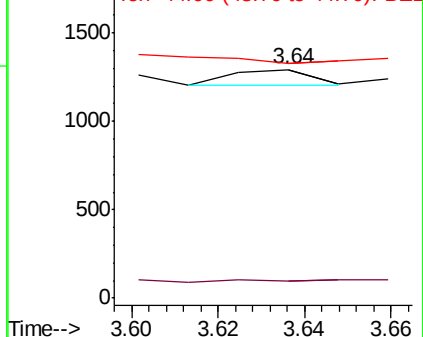

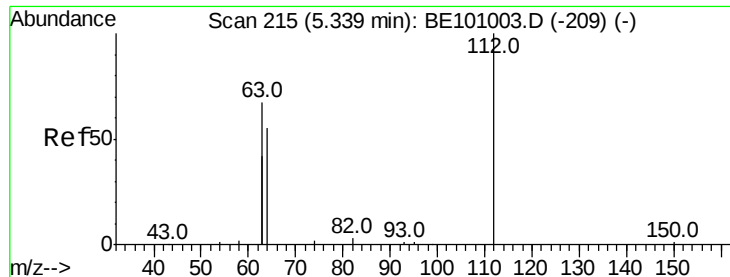

#4

2-Fluorophenol

Concen: 0.257 ng

RT: 5.34 min Scan# 215

Delta R.T. 0.00 min

Lab File: BE101049.D

Acq: 14 Jan 2020 12:32

Instrument :

BNA_E

ClientSampleId :


Tot Ion:112 Resp: 1681

Ion Ratio Lower Upper

112 100

64 70.9 53.6 80.4




63 156.3 114.6 172.0

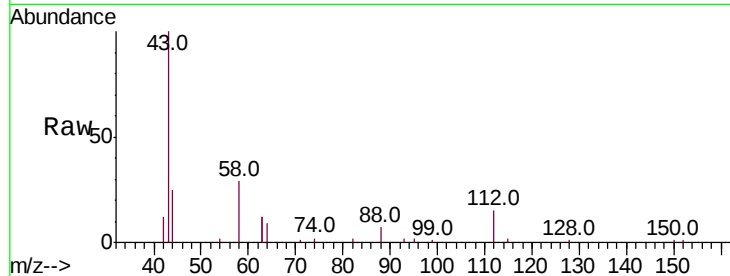

Abundance Ion 112.00 (111.70 to 112.70): BE1

Ion 64.00 (63.70 to 64.70): BE1

Ion 63.00 (62.70 to 63.70): BE1

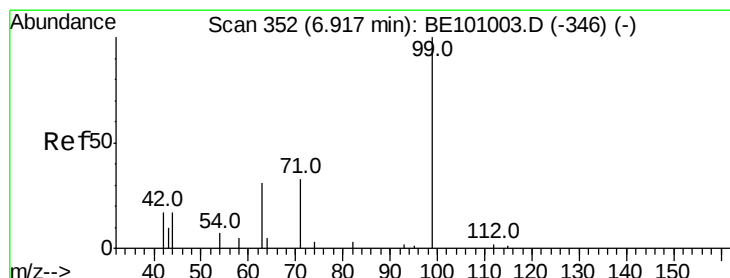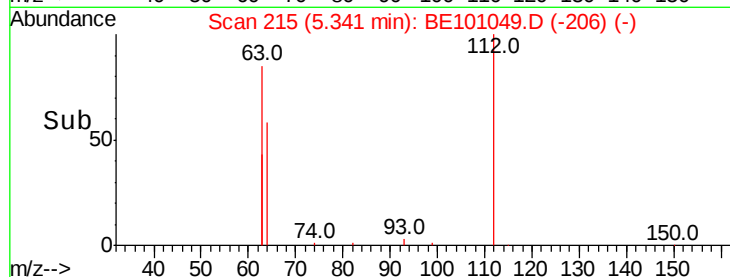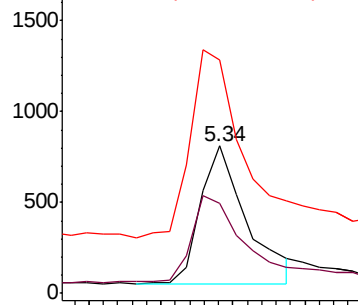

#5

Phenol-d6

Concen: 0.230 ng

RT: 6.93 min Scan# 353

Delta R.T. 0.01 min

Lab File: BE101049.D

Acq: 14 Jan 2020 12:32


Tgt Ion: 99 Resp: 1905

Ion Ratio Lower Upper

99 100

42 18.5 18.3 27.5



71 39.2 28.0 42.0

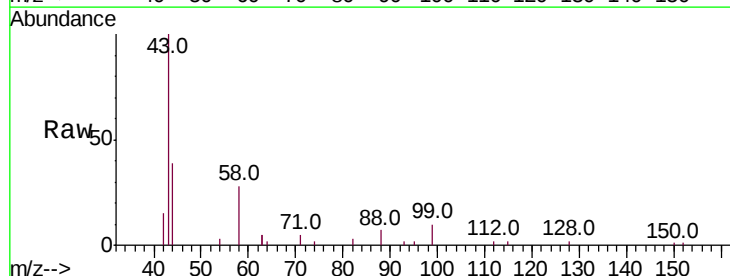


Abundance Ion 99.00 (98.70 to 99.70): BE1

Ion 42.00 (41.70 to 42.70): BE1

Ion 71.00 (70.70 to 71.70): BE1

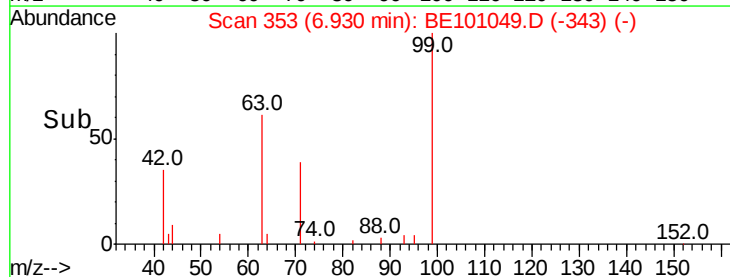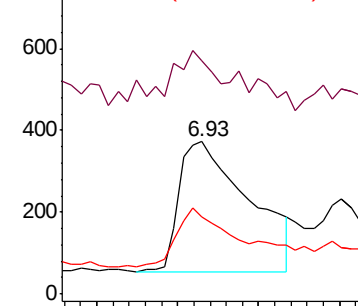



#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.51 min Scan# 642

Delta R.T. 0.01 min

Lab File: BE101049.D

Acq: 14 Jan 2020 12:32

Instrument :

BNA_E

ClientSampleId :

Tot Ion:136 Resp: 12657





Ion Ratio Lower Upper

136 100

137 12.5 9.3 13.9

54 36.6 36.8 55.2#

68 8.2 8.4 12.6#

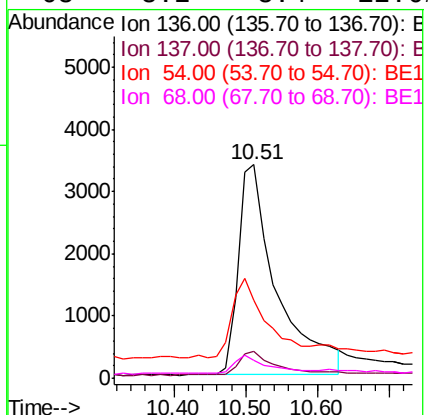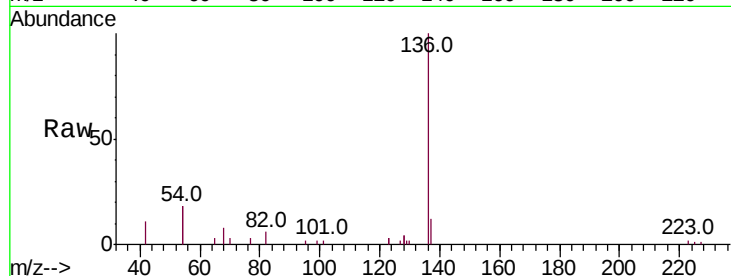

#8

Nitrobenzene-d5

Concen: 0.213 ng

RT: 8.90 min Scan# 518

Delta R.T. 0.03 min

Lab File: BE101049.D

Acq: 14 Jan 2020 12:32




Tgt Ion: 82 Resp: 1927


Ion Ratio Lower Upper

82 100

128 164.7 109.8 164.6#

54 224.6 174.5 261.7

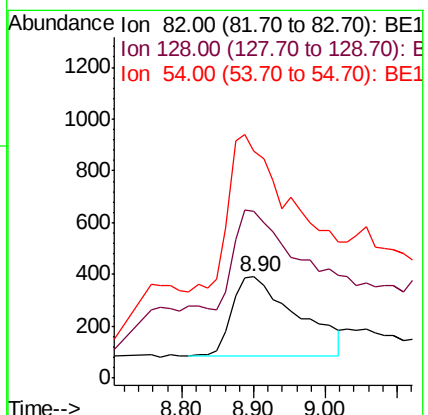

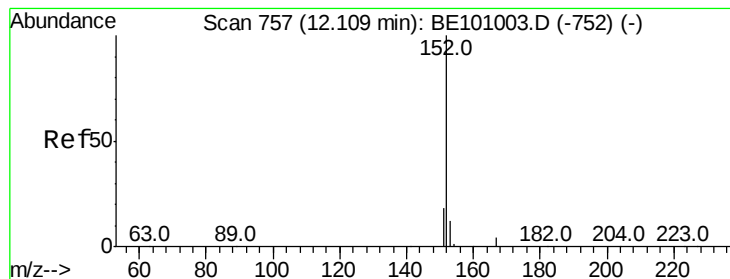

#11

2-Methylnaphthalene-d10

Concen: 0.263 ng

RT: 12.11 min Scan# 756

Delta R.T. 0.00 min

Lab File: BE101049.D

Acq: 14 Jan 2020 12:32

Instrument :

BNA_E





ClientSampleId :

Tot Ion:152 Resp: 6350

Ion Ratio Lower Upper

152 100

151 21.2 15.0 22.6

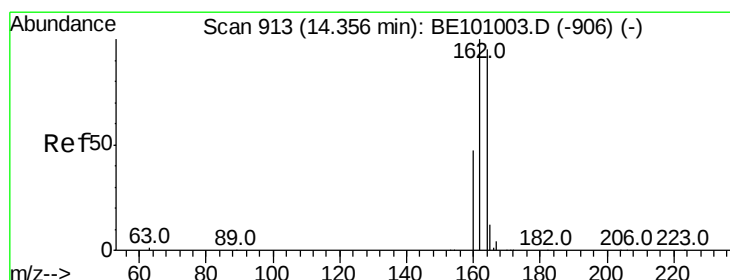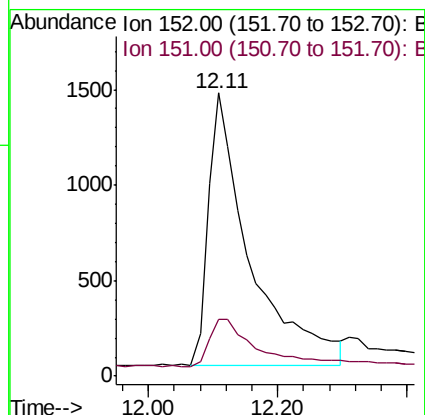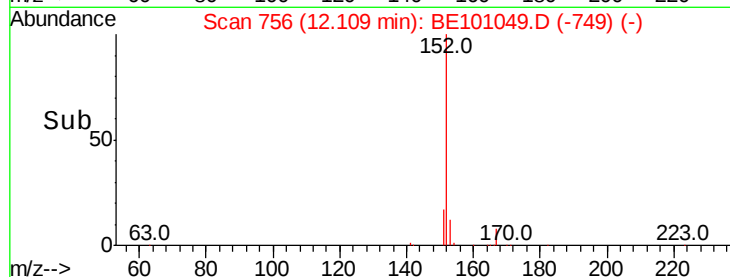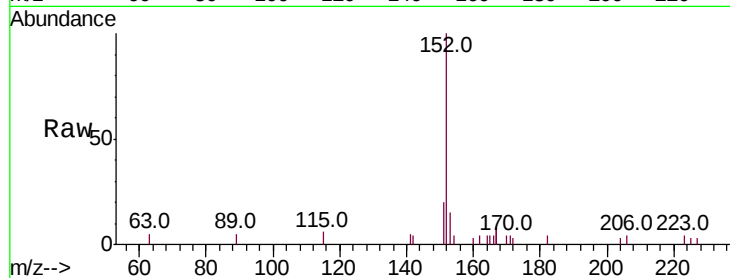

#13

Acenaphthene-d10

Concen: 0.400 ng

RT: 14.36 min Scan# 912

Delta R.T. 0.00 min

Lab File: BE101049.D

Acq: 14 Jan 2020 12:32




Tgt Ion:164 Resp: 8446


Ion Ratio Lower Upper

164 100

162 105.5 84.1 126.1

160 49.8 40.4 60.6


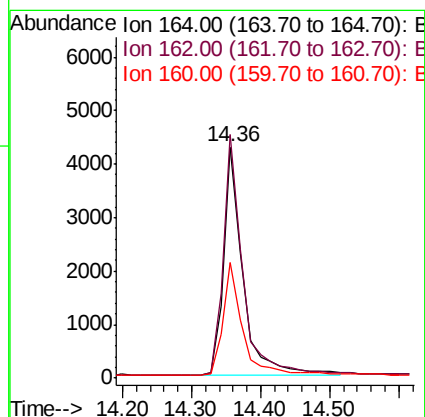
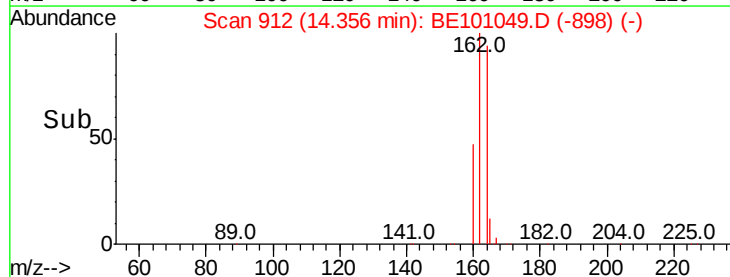
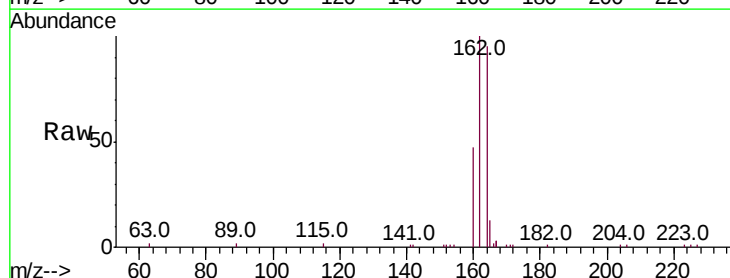




#14
 2,4,6-Tribromophenol
 Concen: 0.146 ng
 RT: 15.85 min Scan# 1017
 Delta R.T. 0.00 min
 Lab File: BE101049.D
 Acq: 14 Jan 2020 12:32




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:330 Resp: 348
 Ion Ratio Lower Upper
 330 100
 332 92.2 78.4 117.6
 141 39.7 37.0 55.4

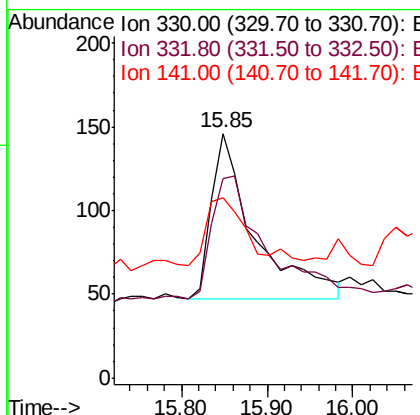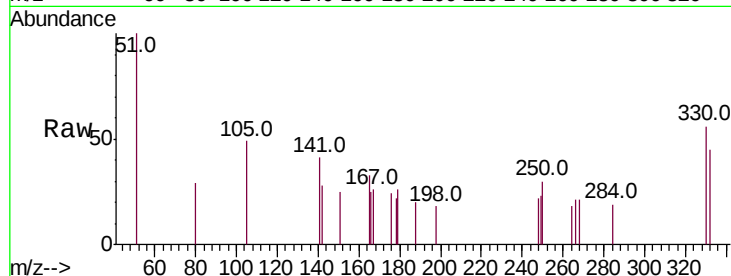

#15
 2-Fluorobiphenyl
 Concen: 0.316 ng
 RT: 13.00 min Scan# 818
 Delta R.T. 0.00 min
 Lab File: BE101049.D
 Acq: 14 Jan 2020 12:32

Tgt Ion:172 Resp: 10150
 Ion Ratio Lower Upper
 172 100
 171 34.7 28.2 42.2
 170 22.8 18.9 28.3

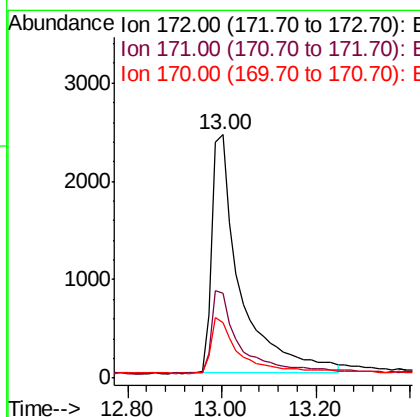

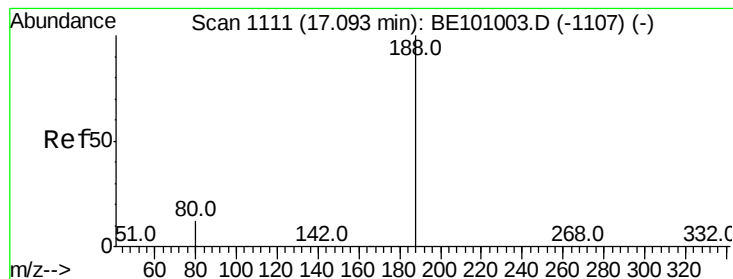

#19

Phenanthrene-d10

Concen: 0.400 ng

RT: 17.09 min Scan# 1110

Delta R.T. 0.00 min

Lab File: BE101049.D

Acq: 14 Jan 2020 12:32

Instrument :

BNA_E

ClientSampleId :


Tot Ion:188 Resp: 19923

Ion Ratio Lower Upper

188 100

94 0.0 0.0 0.0




80 13.7 10.8 16.2

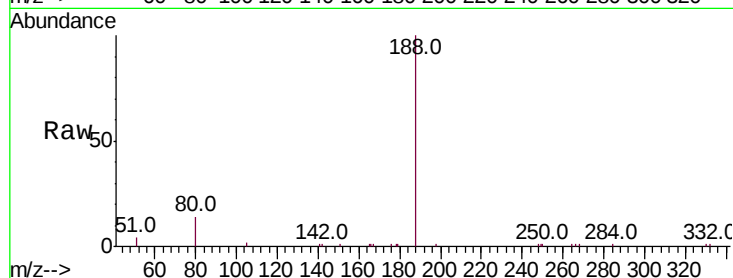

Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BE1

Ion 80.00 (79.70 to 80.70): BE1

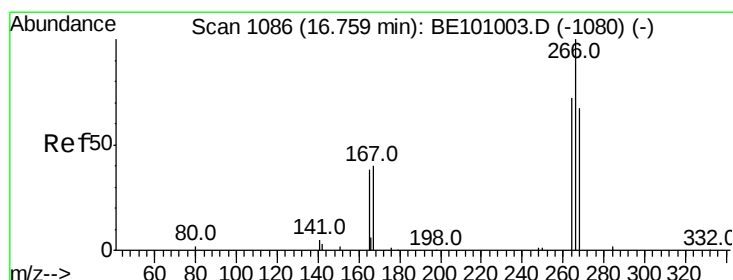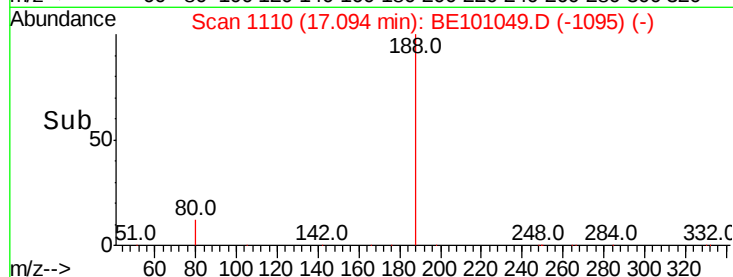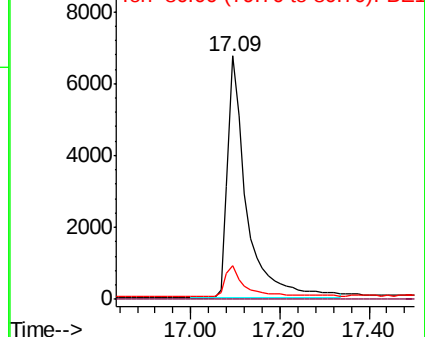

#22

Pentachlorophenol

Concen: 0.257 ng

RT: 16.80 min Scan# 1088

Delta R.T. 0.04 min

Lab File: BE101049.D

Acq: 14 Jan 2020 12:32


Tgt Ion:266 Resp: 26

Ion Ratio Lower Upper

266 100

264 91.2 61.0 91.4



268 94.7 58.5 87.7#

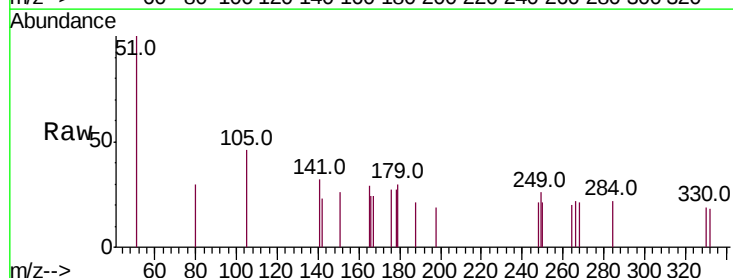


Abundance Ion 266.00 (265.70 to 266.70): E

Ion 264.00 (263.70 to 264.70): E

Ion 268.00 (267.70 to 268.70): E



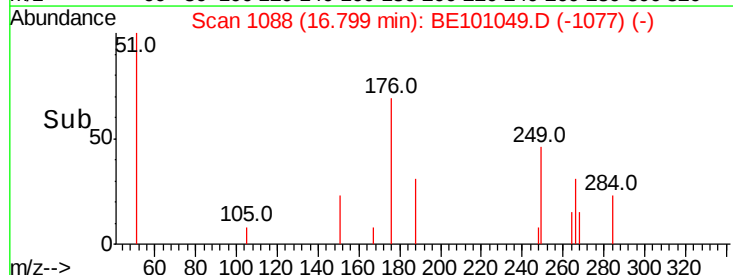
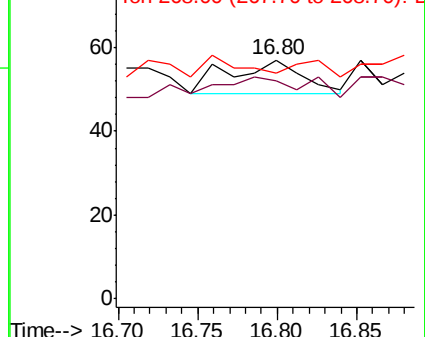




#25
 Fluoranthene-d10
 Concen: 0.299 ng
 RT: 19.13 min Scan# 1368
 Delta R.T. -0.01 min
 Lab File: BE101049.D
 Acq: 14 Jan 2020 12:32




Instrument :
 BNA_E
 ClientSampleId :


Tot Ion:212 Resp: 82759
 Ion Ratio Lower Upper
 212 100
 106 3.4 2.6 3.8
 104 1.9 1.4 2.0

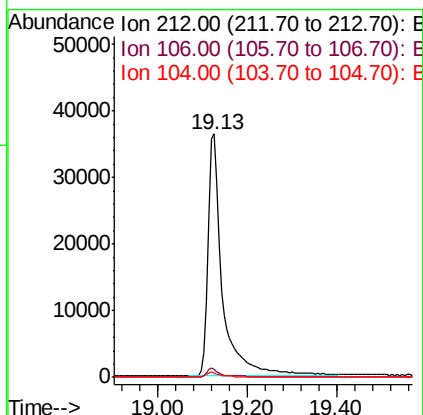

#27
 Chrysene-d12
 Concen: 0.400 ng
 RT: 21.27 min Scan# 1622
 Delta R.T. -0.01 min
 Lab File: BE101049.D
 Acq: 14 Jan 2020 12:32

Tgt Ion:240 Resp: 18244
 Ion Ratio Lower Upper
 240 100
 120 15.4 8.6 13.0#
 236 27.9 22.2 33.4

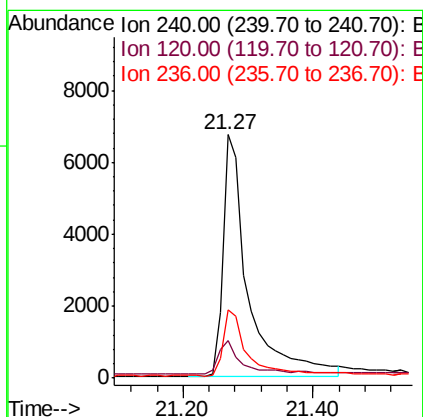

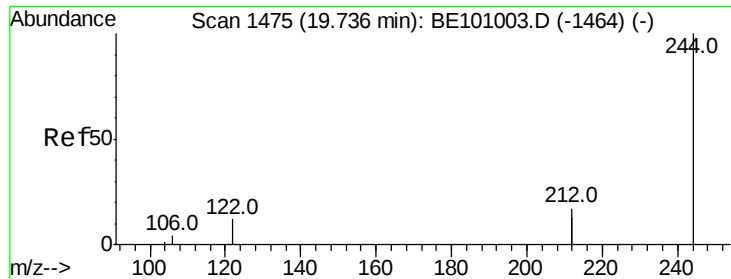

#29

Terphenyl-d14

Concen: 0.341 ng

RT: 19.73 min Scan# 1473

Delta R.T. -0.01 min

Lab File: BE101049.D

Acq: 14 Jan 2020 12:32

Instrument :

BNA_E

ClientSampleId :


Tot Ion:244 Resp: 15260

Ion Ratio Lower Upper

244 100

212 33.9 27.2 40.8




122 12.0 9.8 14.8



Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

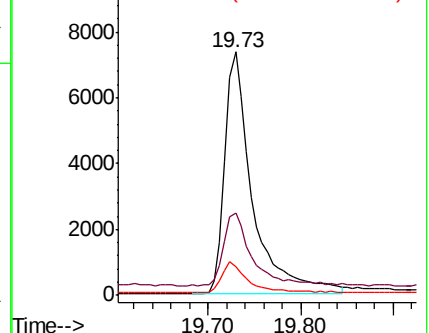

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.091 ng

RT: 21.20 min Scan# 1616

Delta R.T. -0.00 min

Lab File: BE101049.D

Acq: 14 Jan 2020 12:32


Tgt Ion:149 Resp: 7912

Ion Ratio Lower Upper

149 100

167 5.6 5.2 7.8



279 0.9 0.8 1.2






Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

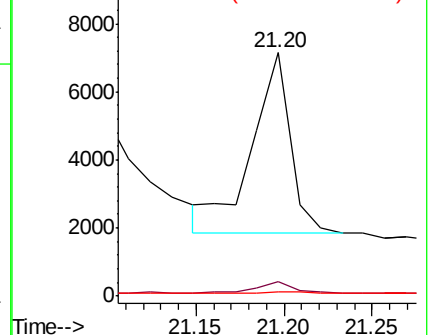

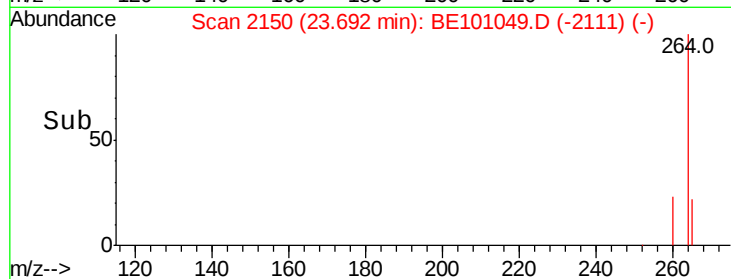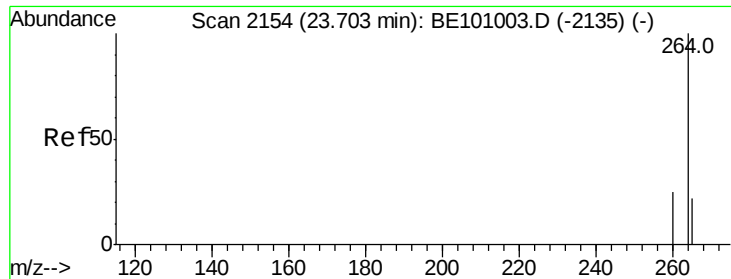

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.69 min Scan# 2150

Delta R.T. -0.01 min

Lab File: BE101049.D

Acq: 14 Jan 2020 12:32

Instrument :

BNA_E

ClientSampleId :

Tot Ion:264 Resp: 19872

Ion Ratio Lower Upper

264 100

260 24.0 20.3 30.5

265 29.0 27.0 40.4

