


Data Path : Z:\SVOASRV\HPCHEM1\BNA_E\DATA\BE011420\
 Data File : BE101046.D
 Acq On : 14 Jan 2020 8:58
 Operator : JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE010820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Jan 08 18:36:25 2020

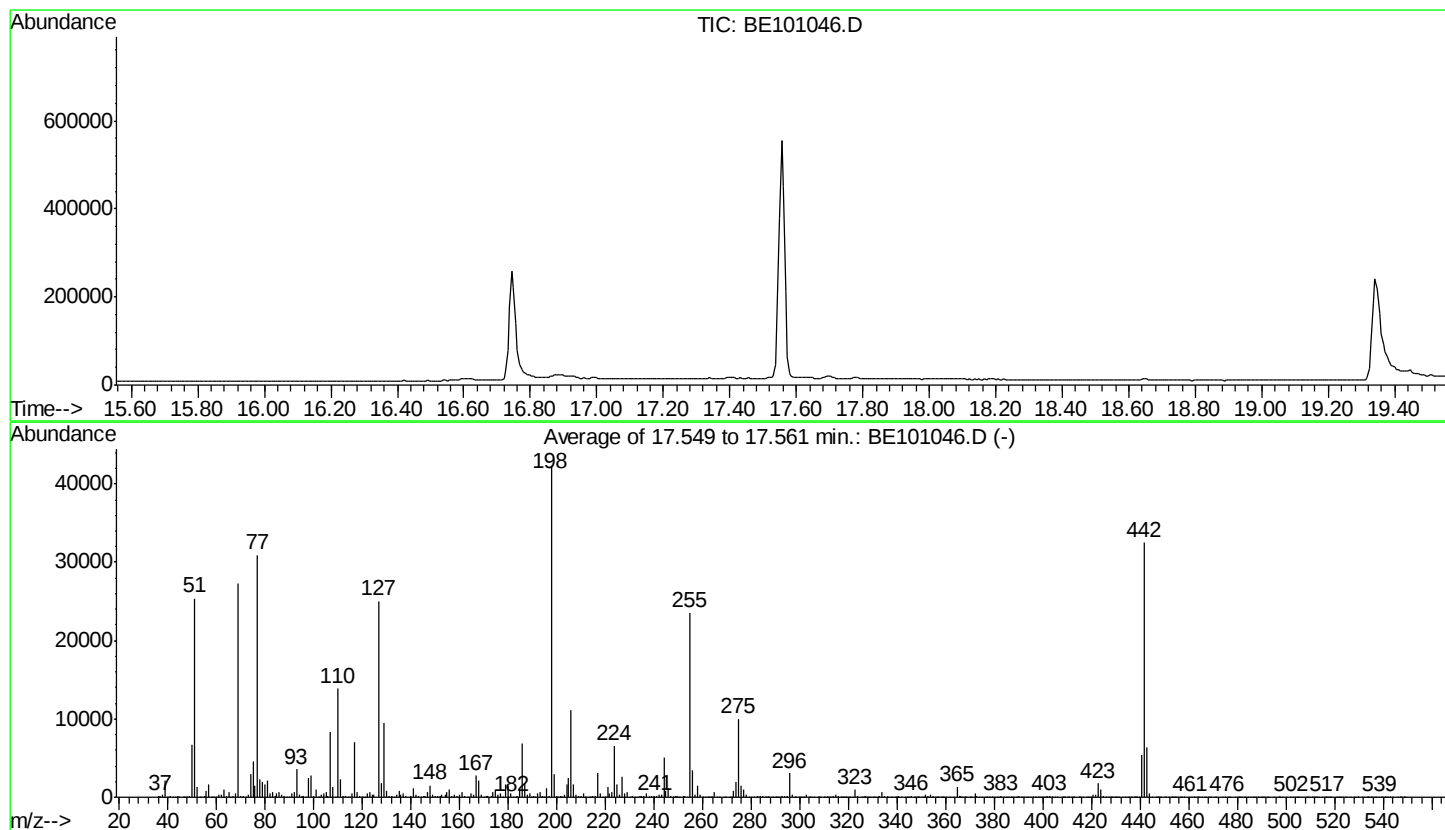

AutoFind: Scans 2546, 2547, 2548; Background Corrected with Scan 2538

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	60.0	25386	PASS
68	69	0.00	2	1.8	479	PASS
69	198	0.00	100	64.4	27280	PASS
70	69	0.00	2	0.3	91	PASS
127	198	10	80	59.2	25049	PASS
197	198	0.00	2	0.3	131	PASS
198	198	100	100	100.0	42344	PASS
199	198	5	9	6.9	2937	PASS
275	198	10	60	23.7	10048	PASS
365	198	1	100	3.2	1350	PASS
441	198	0.01	100	12.6	5338	PASS
442	198	50	100	76.7	32480	PASS
443	442	15	24	19.6	6357	PASS