


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011519\
 Data File : BE098620.D
 Acq On : 15 Jan 2019 10:20
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 15 14:30:55 2019

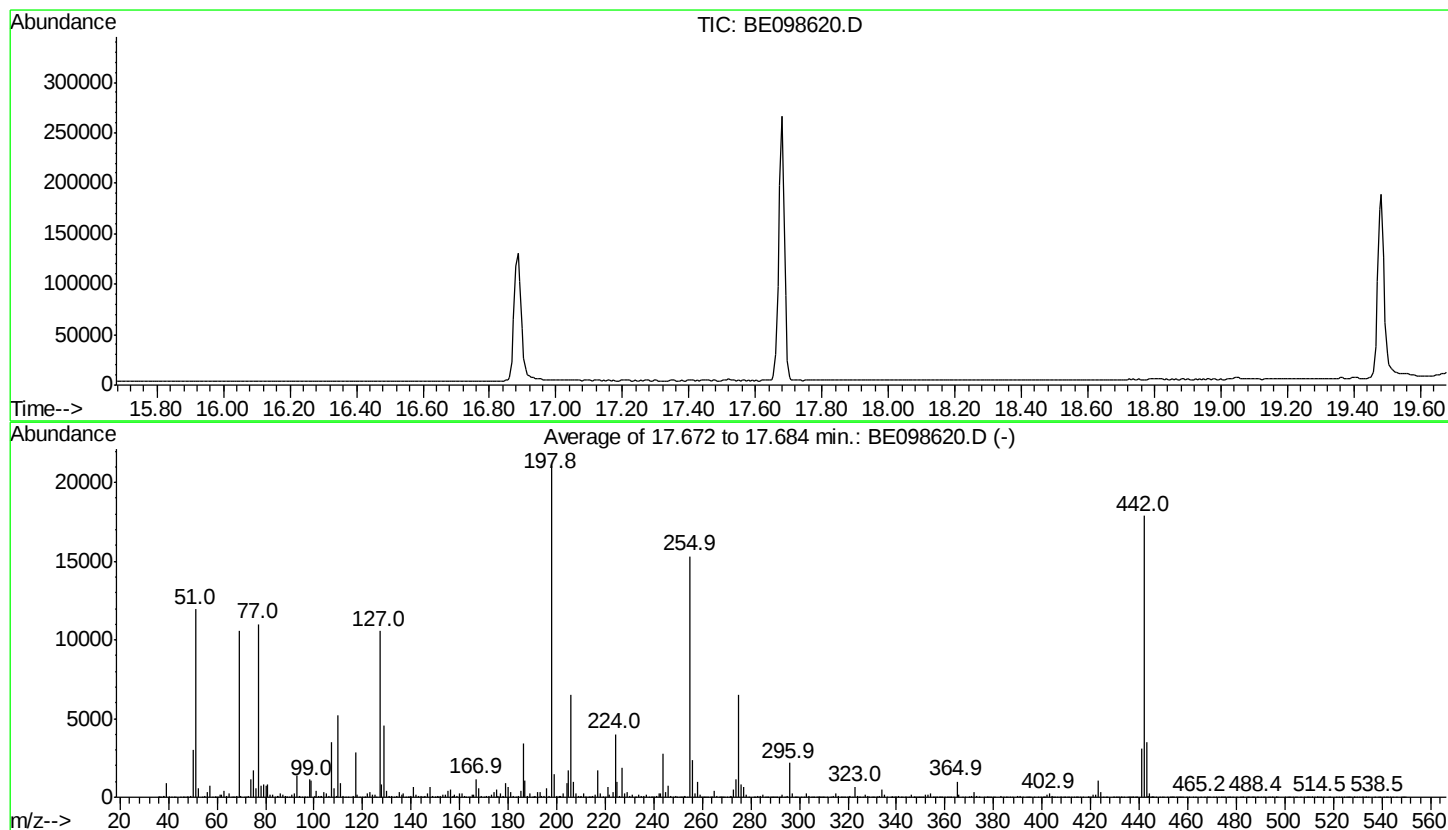

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	56.6	11937	PASS
68	69	0.00	2	1.0	107	PASS
69	198	0.00	100	50.3	10606	PASS
70	69	0.00	2	0.5	57	PASS
127	198	10	80	50.1	10550	PASS
197	198	0.00	2	0.2	45	PASS
198	198	100	100	100.0	21074	PASS
199	198	5	9	7.1	1503	PASS
275	198	10	60	30.8	6489	PASS
365	198	1	100	4.8	1015	PASS
441	198	0.01	100	14.5	3065	PASS
442	198	50	100	84.8	17864	PASS
443	442	15	24	19.5	3484	PASS