

Data File : BE098635.D

Acq On : 16 Jan 2019 15:35

Operator : SJ/JU

Sample : DFTPP

Misc :

ALS Vial : 1 Sample Multiplier: 1




Quant Time: Jan 17 01:24:26 2019

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M

Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

QLast Update : Wed Jan 09 14:23:53 2019

Response via : Initial Calibration

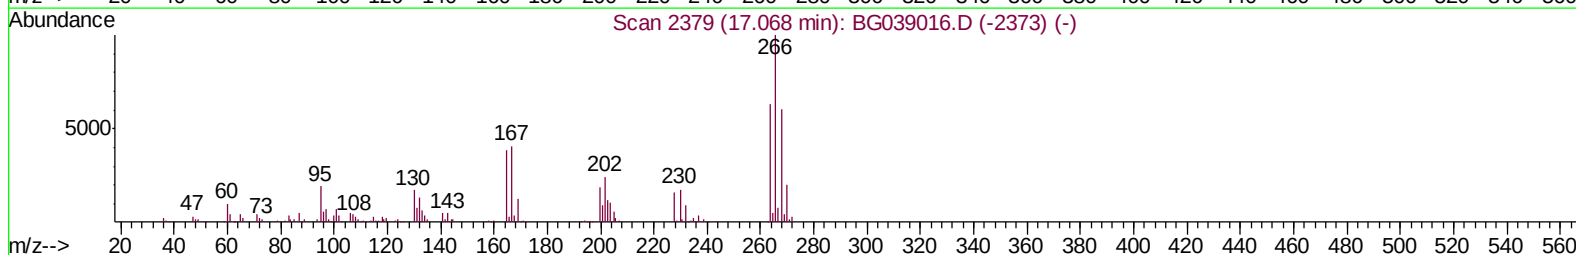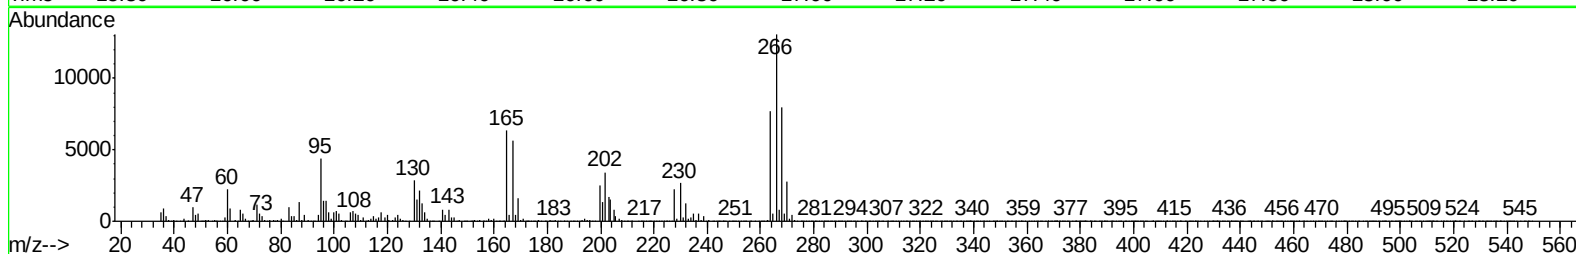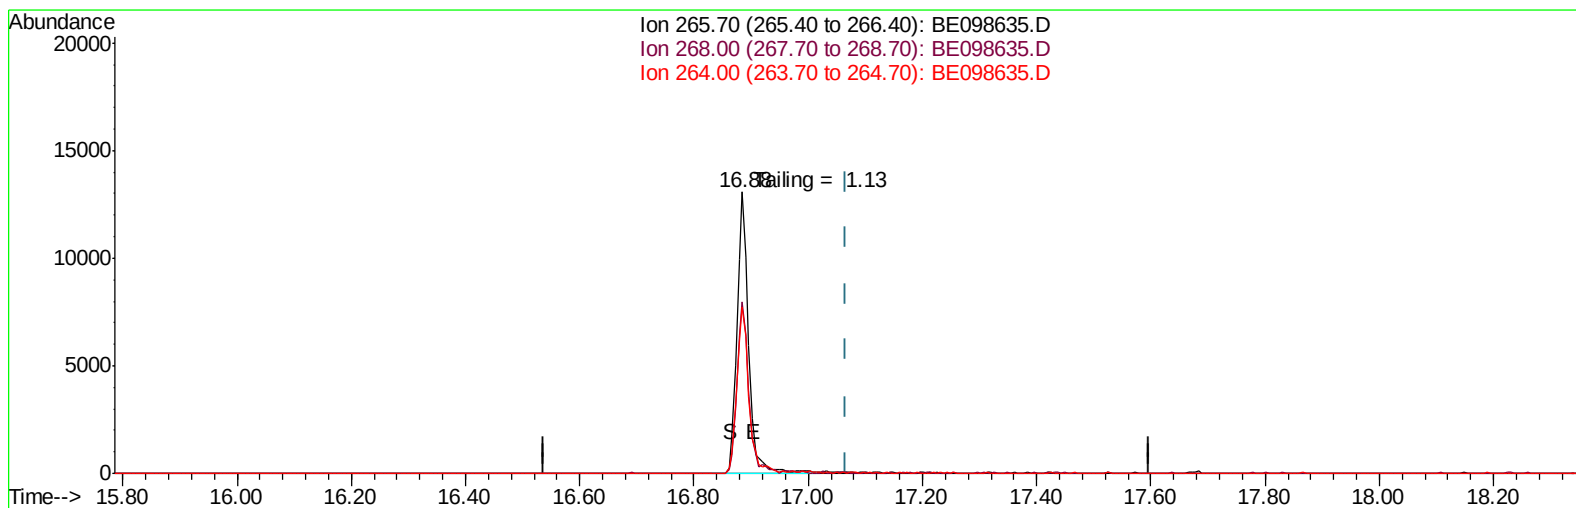

TIC: BE098635.D

(70) Pentachlorophenol (C)




16.885min (-0.182) 141070.89ng

response 18453

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.05
264.00	68.20	59.07
0.00	0.00	0.00

Data File : BE098635.D
Acq On : 16 Jan 2019 15:35
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 01:24:26 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_G\METHODS\8270-BG010919.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Jan 09 14:23:53 2019
Response via : Initial Calibration

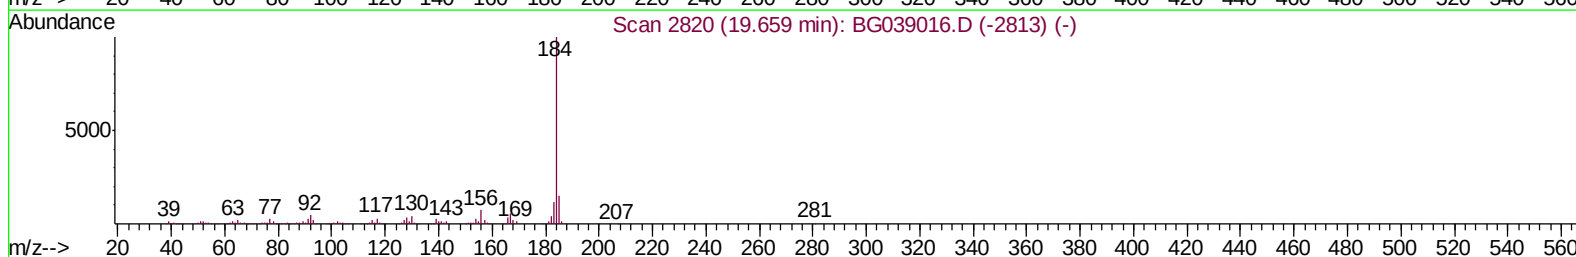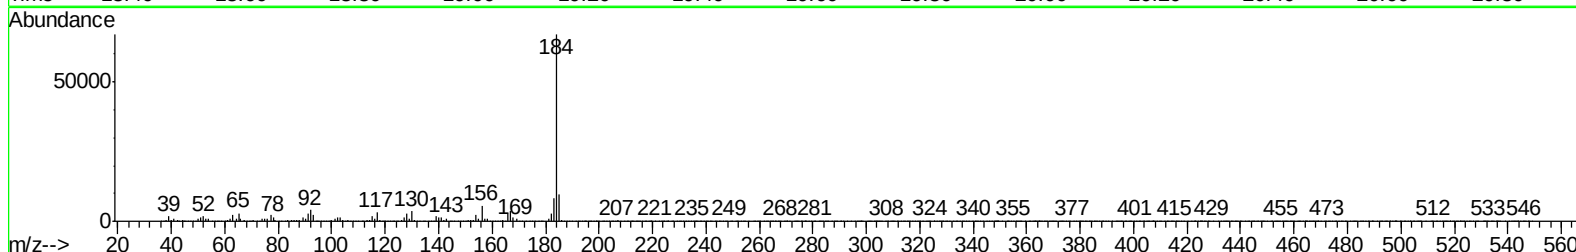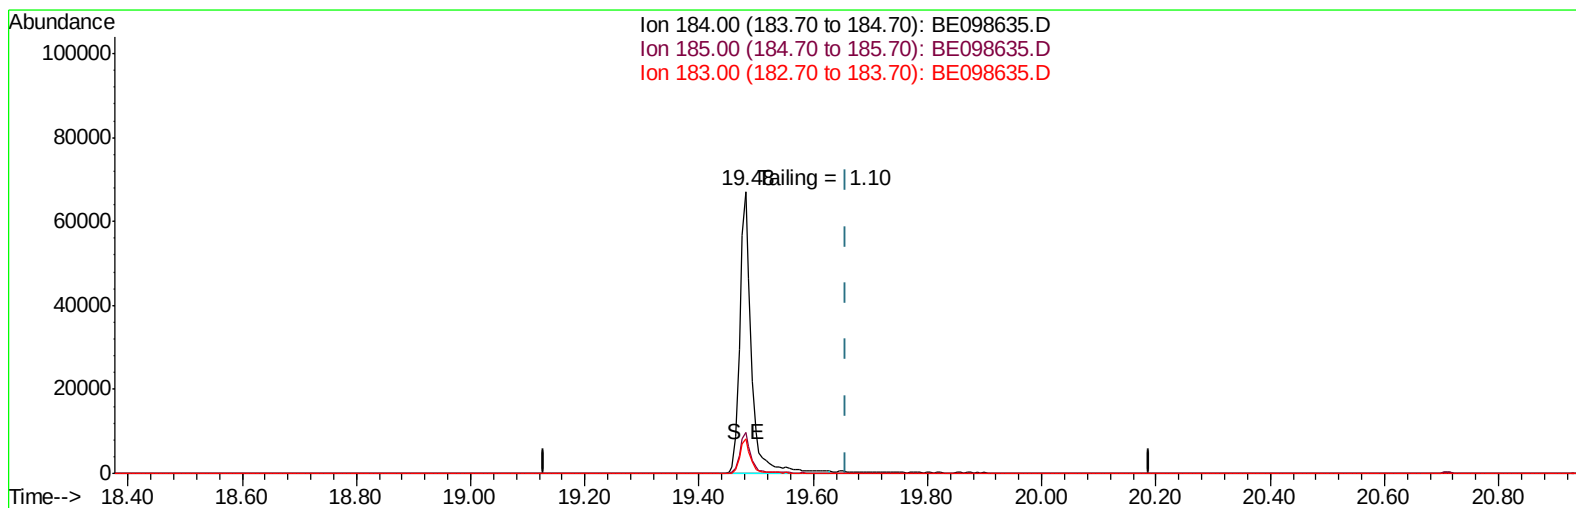

TIC: BE098635.D

(77) Benzidine

19.482min (-0.177) 222890.18ng

response 95443

Ion	Exp%	Act%
184.00	100	100
185.00	15.10	14.41
183.00	11.90	12.22
0.00	0.00	0.00