

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011619\
 Data File : BE098643.D
 Acq On : 16 Jan 2019 22:06
 Operator : SJ/JU
 Sample : K1151-03
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 OUTFALL001-190115

Quant Time: Jan 17 00:43:00 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE011519.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Jan 15 14:30:55 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.81	152	812	0.40	ng	0.00
7) Naphthalene-d8	10.60	136	3538	0.40	ng	0.00
13) Acenaphthene-d10	14.47	164	2415	0.40	ng	0.00
19) Phenanthrene-d10	17.23	188	5835	0.40	ng	0.00
27) Chrysene-d12	21.41	240	6747	0.40	ng	0.00
34) Perylene-d12	23.92	264	6682	0.40	ng	0.00
System Monitoring Compounds						
4) 2-Fluorophenol	5.40	112	322	0.15	ng	0.00
5) Phenol-d6	7.00	99	295	0.10	ng	0.00
8) Nitrobenzene-d5	8.98	82	898	0.32	ng	0.01
11) 2-Methylnaphthalene-d10	12.21	152	2264	0.39	ng	0.00
14) 2,4,6-Tribromophenol	15.97	330	460	0.44	ng	0.00
15) 2-Fluorobiphenyl	13.09	172	3604	0.36	ng	0.00
25) Fluoranthene-d10	19.26	212	28949	0.40	ng	0.00
29) Terphenyl-d14	19.86	244	7401	0.50	ng	0.00
Target Compounds						Qvalue
32) Bis(2-ethylhexyl)phthalate	21.32	149	3522	0.092	ng	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011619\
Data File : BE098643.D
Acq On : 16 Jan 2019 22:06
Operator : SJ/JU
Sample : K1151-03
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_E
ClientSampleId :
OUTFALL001-190115

Quant Time: Jan 17 00:43:00 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE011519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 15 14:30:55 2019
Response via : Initial Calibration

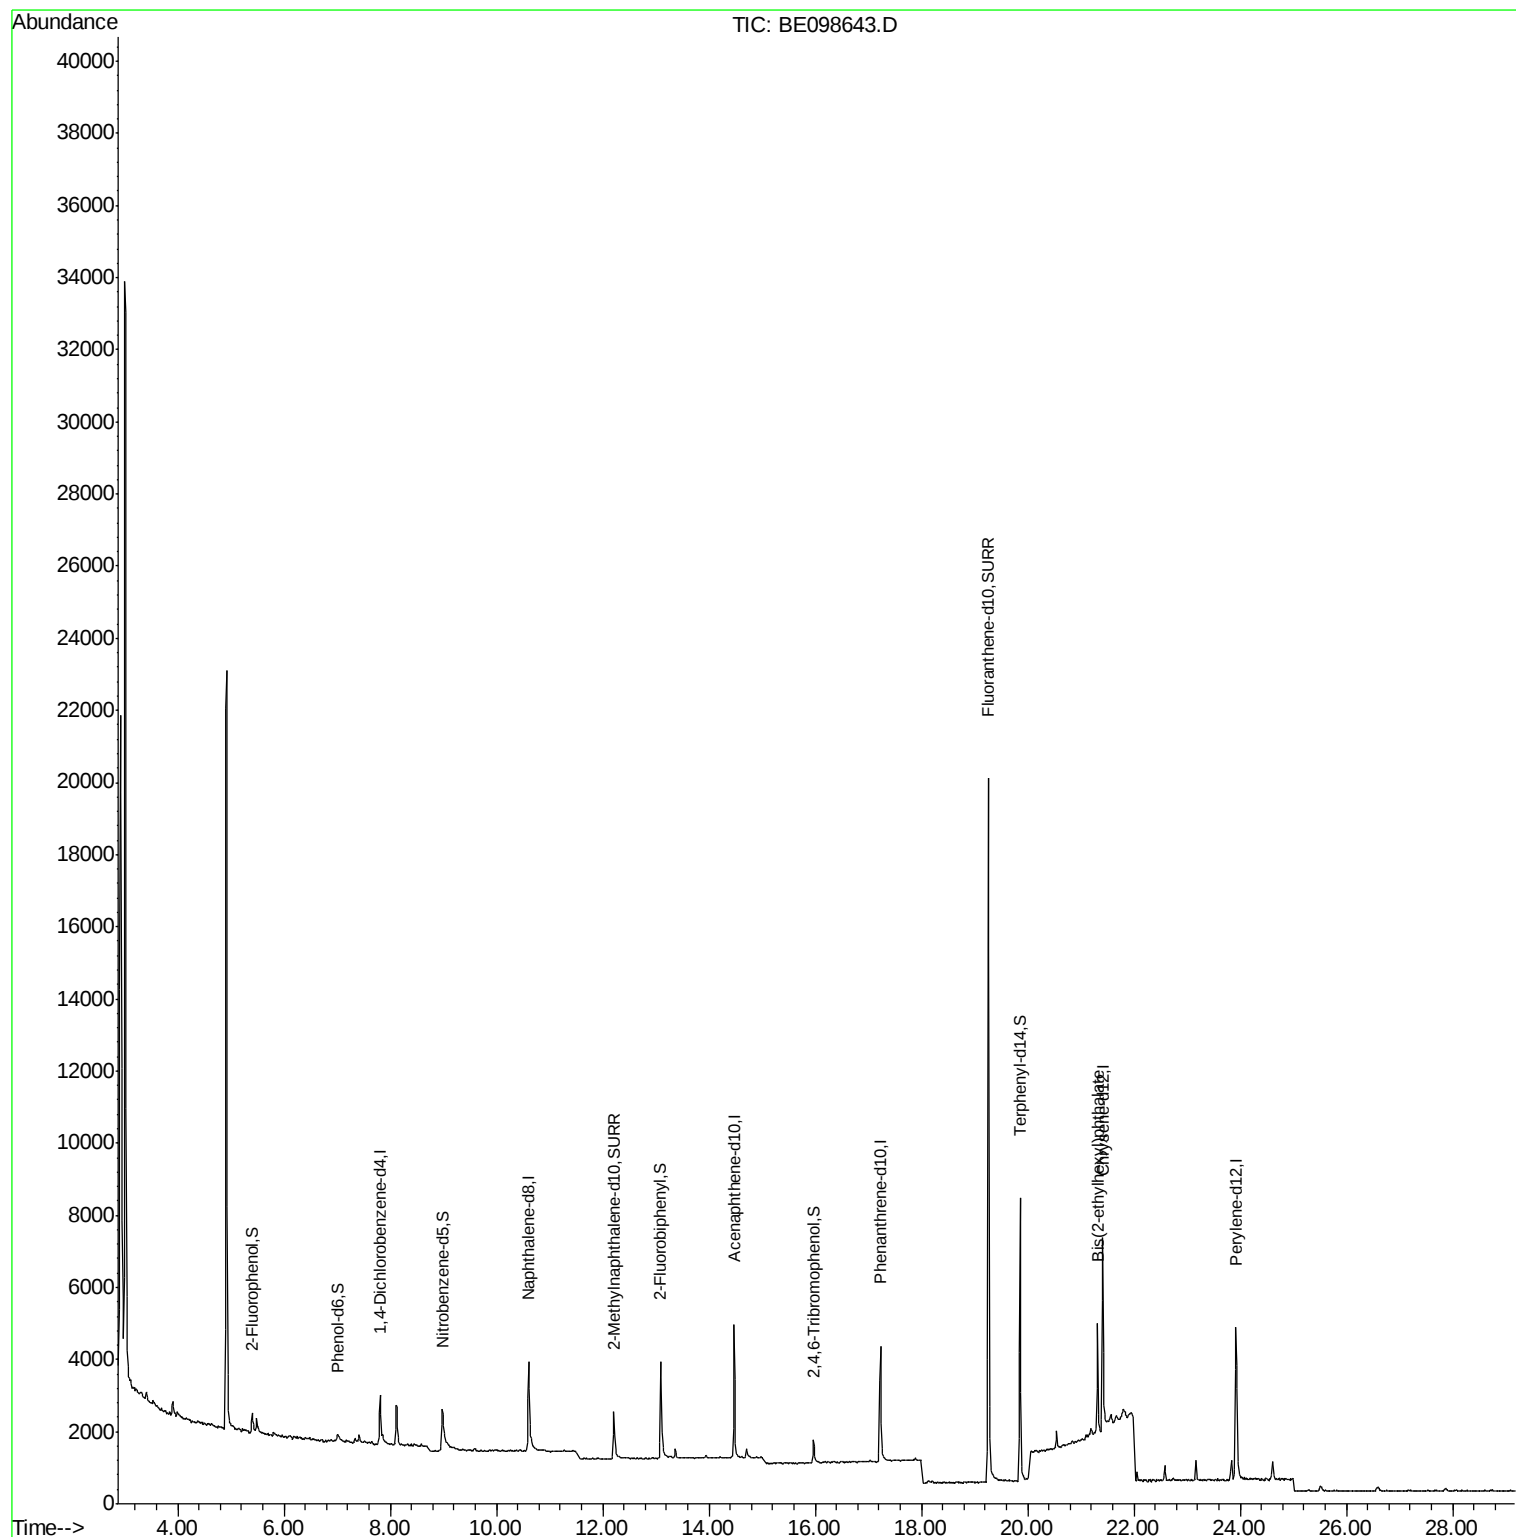

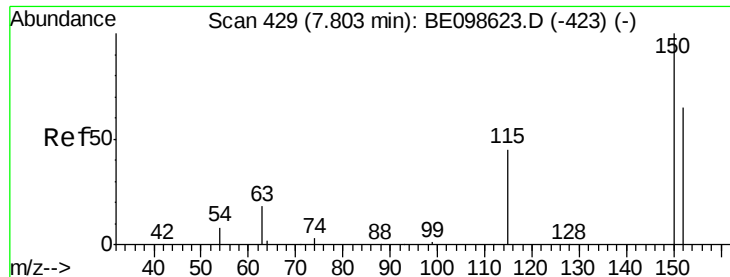


#1




1,4-Dichlorobenzene-d4
Concen: 0.400 ng
RT: 7.81 min Scan# 429
Delta R.T. 0.00 min
Lab File: BE098643.D
Acq: 16 Jan 2019 22:06

Instrument :
BNA_E
ClientSampleId :
OUTFALL001-190115

Tot Ion:152 Resp: 812
Ion Ratio Lower Upper
152 100
150 151.3 121.4 182.2
115 75.7 59.1 88.7

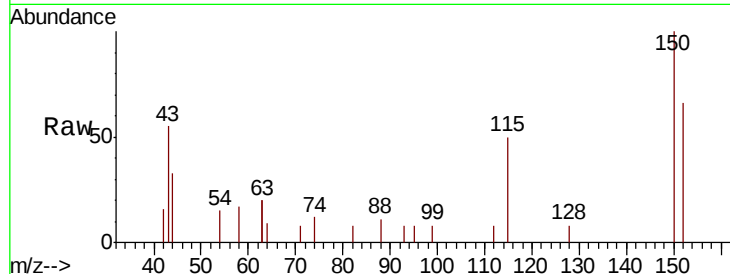


Abundance Ion 152.00 (151.70 to 152.70): E
Ion 150.00 (149.70 to 150.70): E
Ion 115.00 (114.70 to 115.70): E

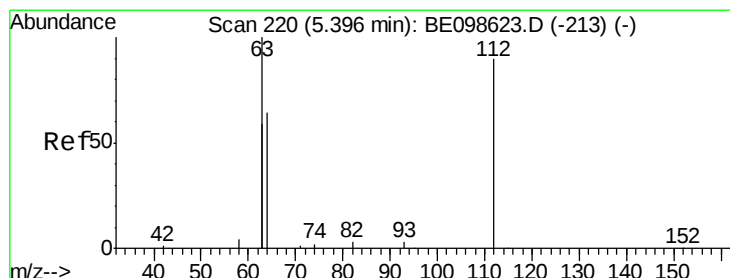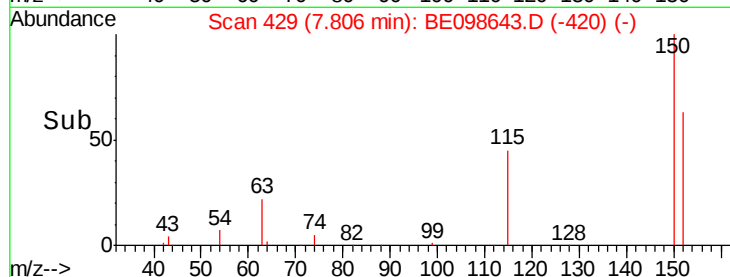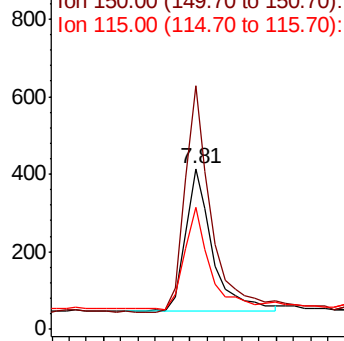



#4


2-Fluorophenol
Concen: 0.149 ng
RT: 5.40 min Scan# 220
Delta R.T. 0.00 min
Lab File: BE098643.D
Acq: 16 Jan 2019 22:06

Tgt Ion:112 Resp: 322
Ion Ratio Lower Upper
112 100
64 97.2 62.9 94.3#
63 202.5 152.2 228.4

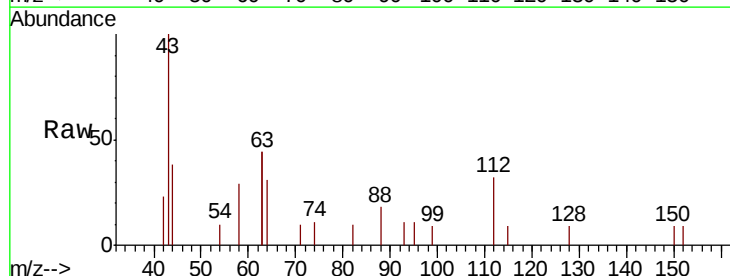

Abundance Ion 112.00 (111.70 to 112.70): E
Ion 64.00 (63.70 to 64.70): BE0
Ion 63.00 (62.70 to 63.70): BE0

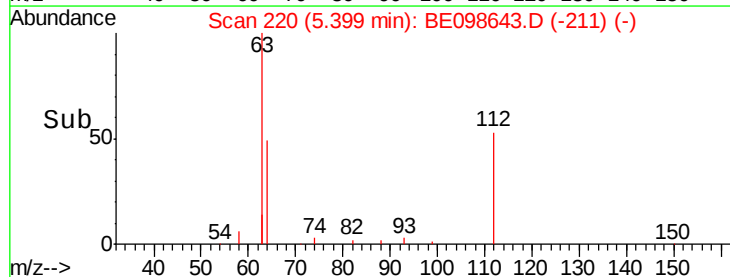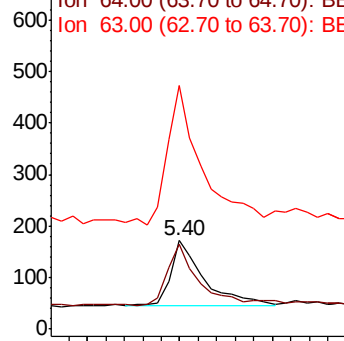

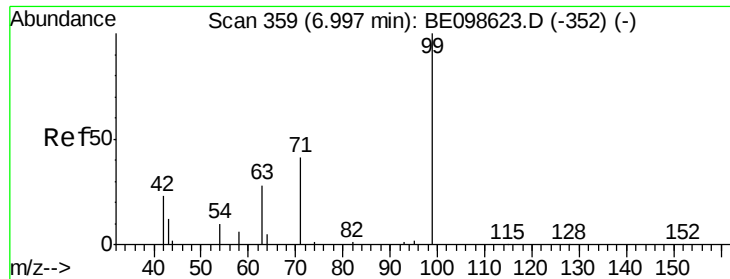

#5

Phenol-d6

Concen: 0.096 ng

RT: 7.00 min Scan# 359

Delta R.T. 0.00 min

Lab File: BE098643.D

Acq: 16 Jan 2019 22:06

Instrument :

BNA_E

ClientSampleId :

OUTFALL001-190115


Tot Ion: 99 Resp: 295

Ion Ratio Lower Upper

99 100

42 36.6 24.6 37.0

71 48.8 35.1 52.7

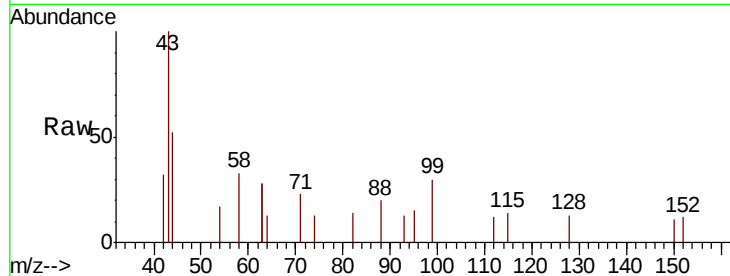

Abundance Ion 99.00 (98.70 to 99.70): BE0

Ion 42.00 (41.70 to 42.70): BE0

Ion 71.00 (70.70 to 71.70): BE0

7.00

150



100

50

0

6.90 7.00 7.10 7.20

Time-->

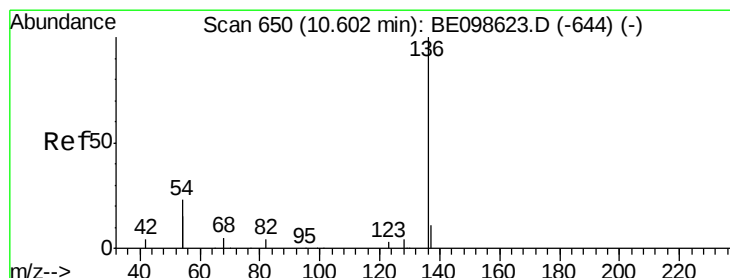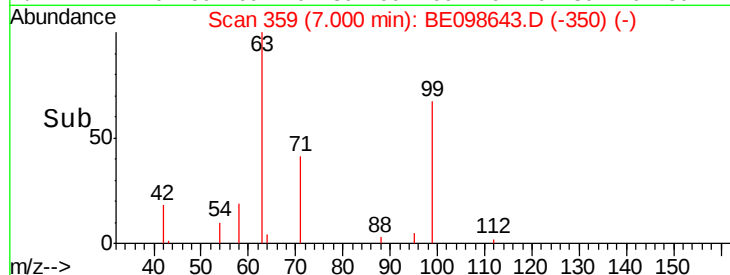

#7

Naphthalene-d8

Concen: 0.400 ng

RT: 10.60 min Scan# 649

Delta R.T. -0.00 min

Lab File: BE098643.D

Acq: 16 Jan 2019 22:06

Tgt Ion: 136 Resp: 3538


Ion Ratio Lower Upper

136 100

137 13.4 9.7 14.5

54 54.8 35.5 53.3#

68 8.3 5.0 7.6#

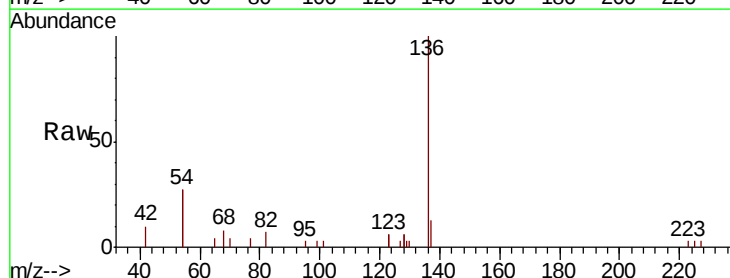

Abundance Ion 136.00 (135.70 to 136.70): E

Ion 137.00 (136.70 to 137.70): E

Ion 54.00 (53.70 to 54.70): BE0

Ion 68.00 (67.70 to 68.70): BE0

2000

1500


1000


500

0

10.50 10.60 10.70 10.80

Time-->

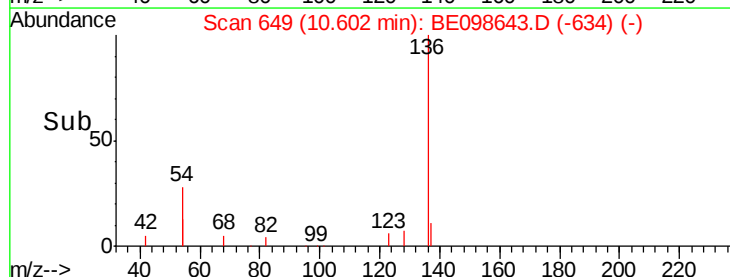

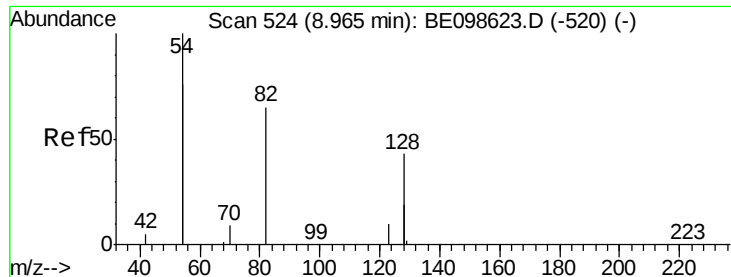

#8

Nitrobenzene-d5

Concen: 0.320 ng

RT: 8.98 min Scan# 524

Delta R.T. 0.01 min

Lab File: BE098643.D

Acq: 16 Jan 2019 22:06

Instrument :

BNA_E

ClientSampleId :

OUTFALL001-190115


Tot Ion: 82 Resp: 898

Ion Ratio Lower Upper

82 100

128 165.1 96.5 144.7#




54 301.1 224.7 337.1

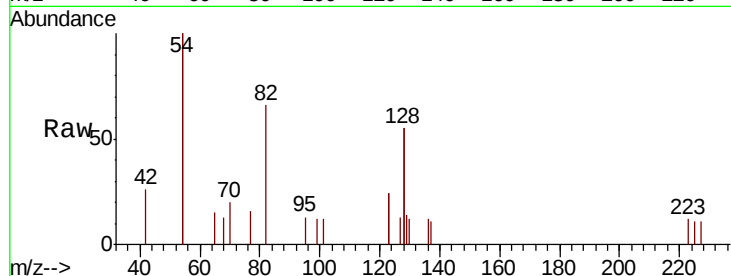

Abundance Ion 82.00 (81.70 to 82.70): BE0

Ion 128.00 (127.70 to 128.70): E

Ion 54.00 (53.70 to 54.70): BE0

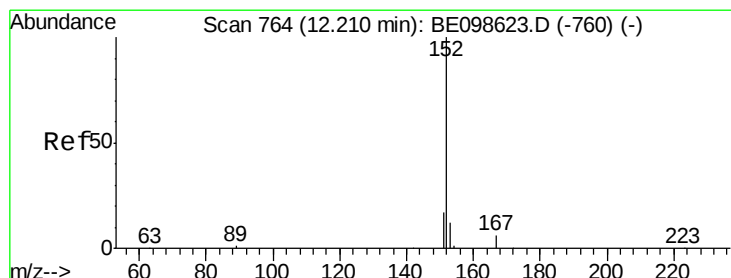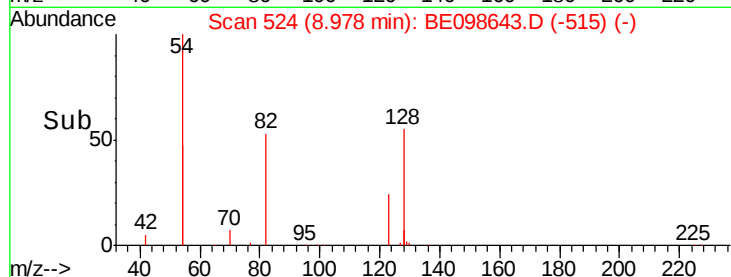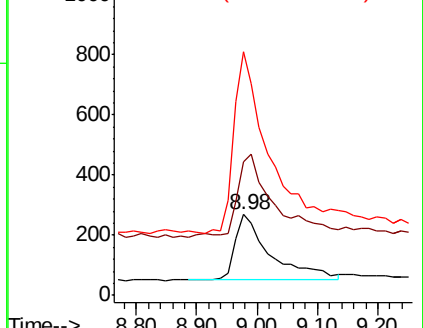

#11

2-Methylnaphthalene-d10

Concen: 0.389 ng

RT: 12.21 min Scan# 763

Delta R.T. 0.00 min

Lab File: BE098643.D


Acq: 16 Jan 2019 22:06

Tgt Ion:152 Resp: 2264

Ion Ratio Lower Upper



152 100


151 19.0 16.2 24.4

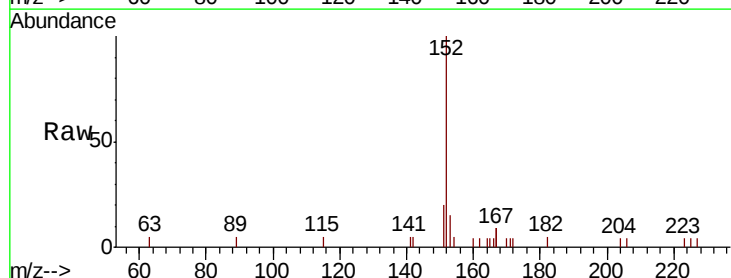

Abundance Ion 152.00 (151.70 to 152.70): E

Ion 151.00 (150.70 to 151.70): E

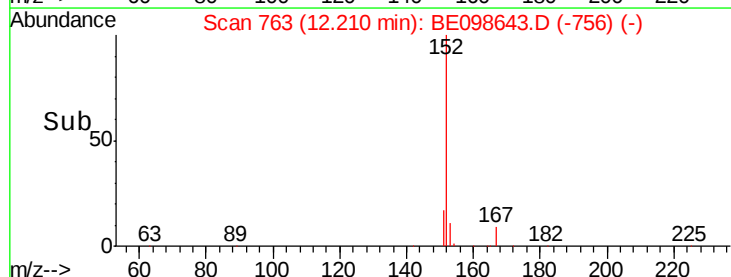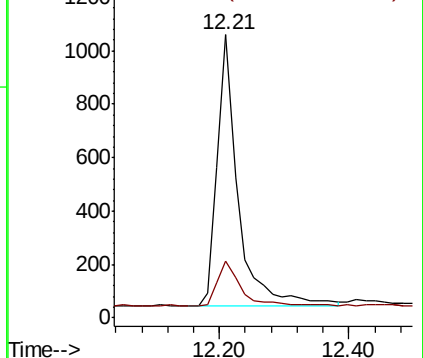


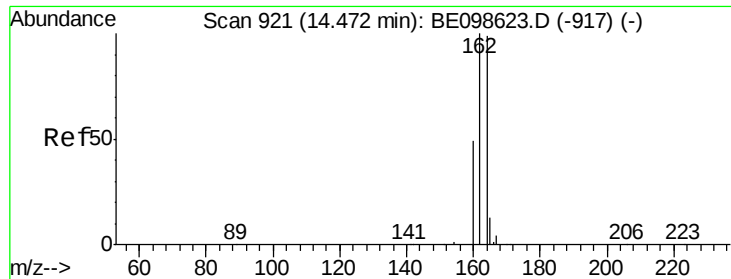




#13
Acenaphthene-d10
Concen: 0.400 ng
RT: 14.47 min Scan# 920
Delta R.T. 0.00 min
Lab File: BE098643.D
Acq: 16 Jan 2019 22:06

Instrument :
BNA_E
ClientSampleId :
OUTFALL001-190115

Tot Ion:164 Resp: 2415
Ion Ratio Lower Upper
164 100
162 101.7 80.5 120.7
160 50.7 40.1 60.1

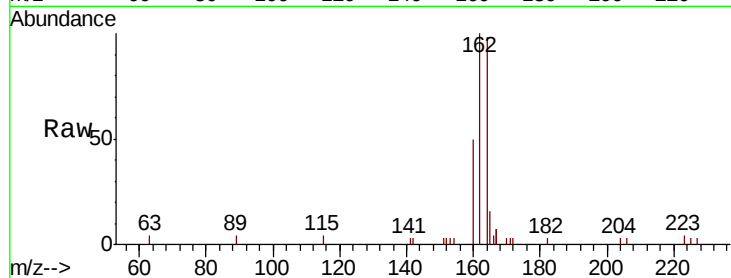


Abundance Ion 164.00 (163.70 to 164.70): E
Ion 162.00 (161.70 to 162.70): E
Ion 160.00 (159.70 to 160.70): E

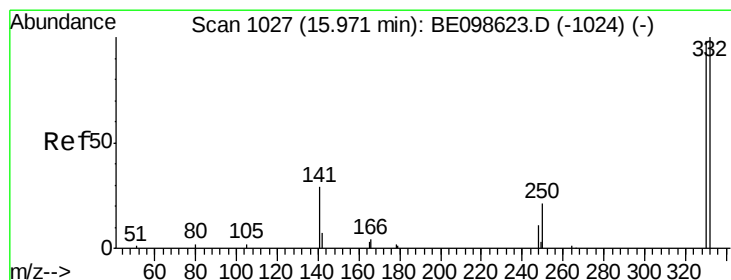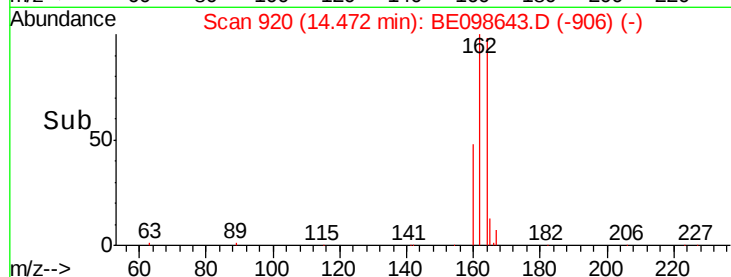
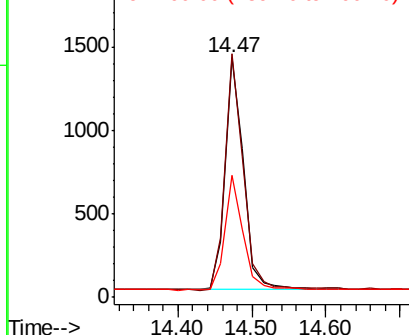



#14
2,4,6-Tribromophenol
Concen: 0.438 ng
RT: 15.97 min Scan# 1026
Delta R.T. -0.00 min
Lab File: BE098643.D
Acq: 16 Jan 2019 22:06

Tgt Ion:330 Resp: 460
Ion Ratio Lower Upper
330 100
332 101.3 73.3 109.9
141 39.3 33.1 49.7

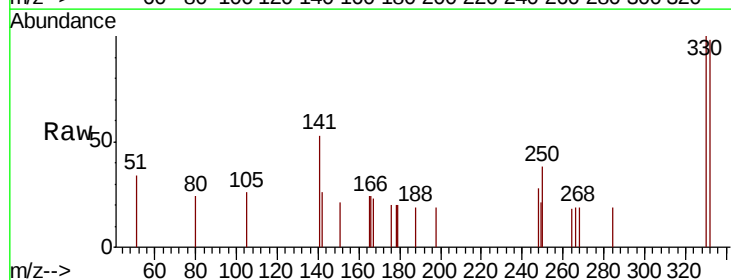

Abundance Ion 330.00 (329.70 to 330.70): E
Ion 331.80 (331.50 to 332.50): E
Ion 141.00 (140.70 to 141.70): E

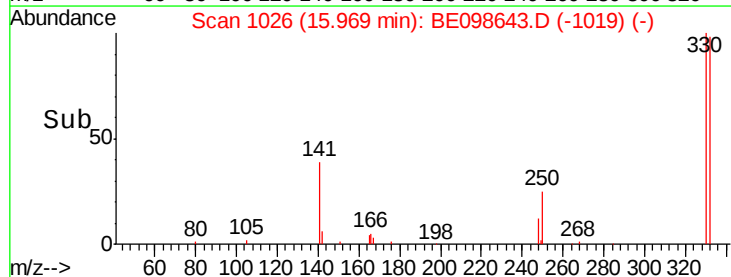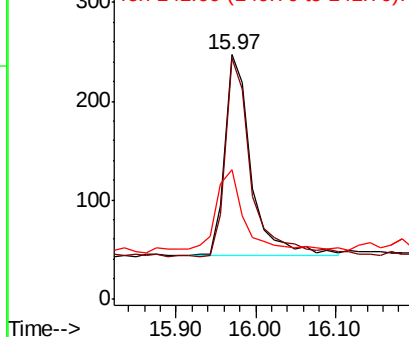


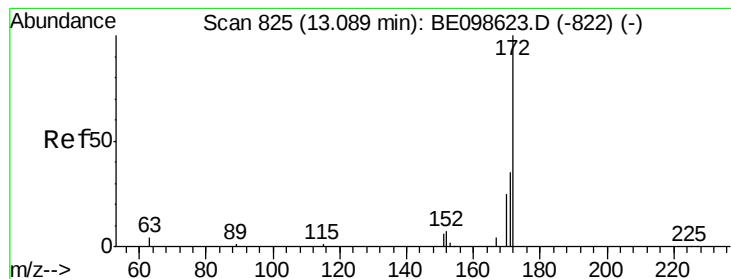




#15
2-Fluorobiphenyl
Concen: 0.364 ng
RT: 13.09 min Scan# 824
Delta R.T. 0.00 min
Lab File: BE098643.D
Acq: 16 Jan 2019 22:06

Instrument :
BNA_E
ClientSampleId :
OUTFALL001-190115

Tot Ion:172 Resp: 3604
Ion Ratio Lower Upper
172 100
171 38.2 29.0 43.4
170 26.8 20.8 31.2

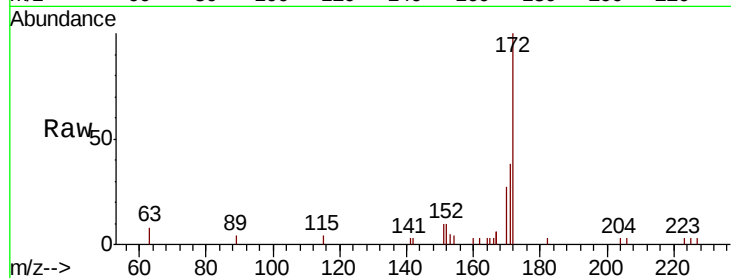


Abundance Ion 172.00 (171.70 to 172.70): E
Ion 171.00 (170.70 to 171.70): E
Ion 170.00 (169.70 to 170.70): E

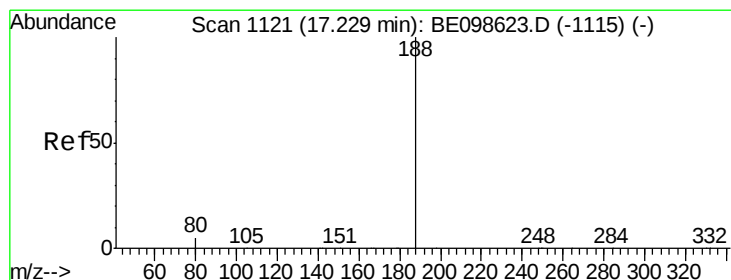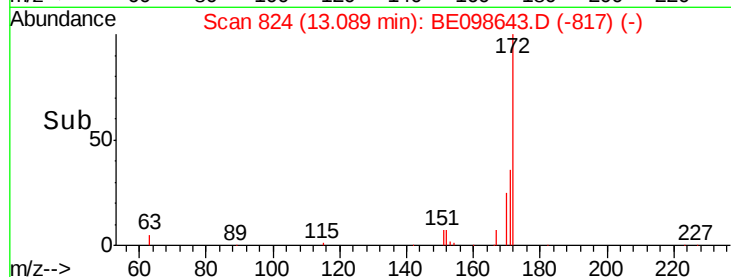
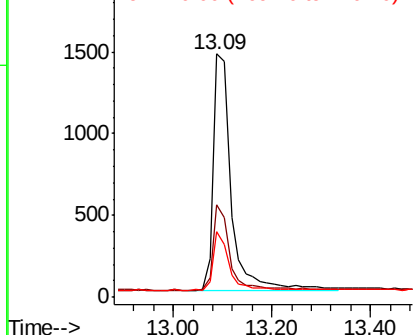



#19
Phenanthrene-d10
Concen: 0.400 ng
RT: 17.23 min Scan# 1120
Delta R.T. -0.00 min
Lab File: BE098643.D
Acq: 16 Jan 2019 22:06

Tgt Ion:188 Resp: 5835
Ion Ratio Lower Upper
188 100
94 0.0 0.0 0.0
80 8.1 4.7 7.1#

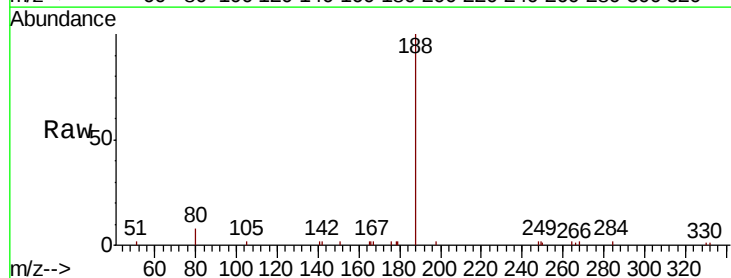

Abundance Ion 188.00 (187.70 to 188.70): E
Ion 94.00 (93.70 to 94.70): BE0
Ion 80.00 (79.70 to 80.70): BE0

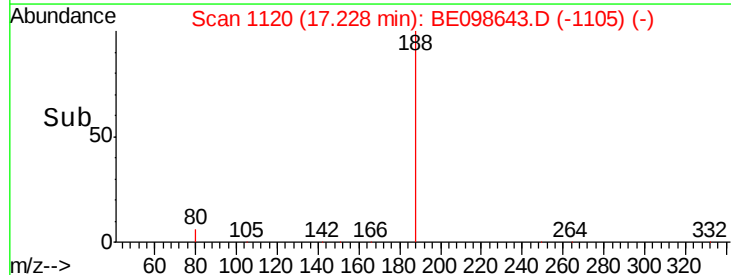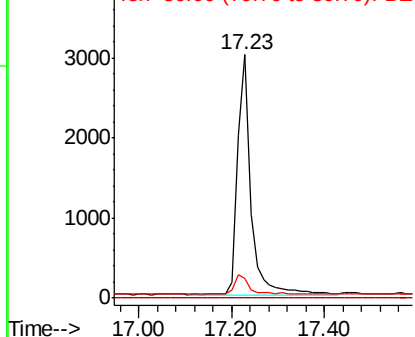

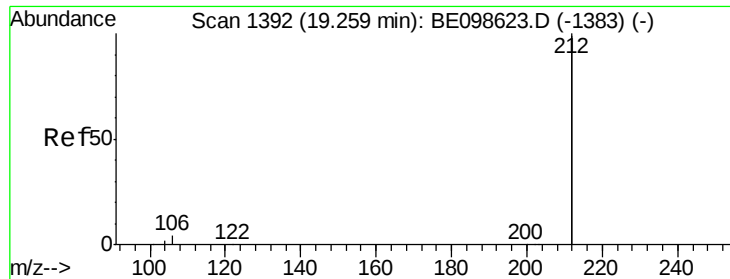

#25

Fluoranthene-d10

Concen: 0.401 ng

RT: 19.26 min Scan# 1391

Delta R.T. 0.00 min

Lab File: BE098643.D

Acq: 16 Jan 2019 22:06

Instrument :

BNA_E

ClientSampleId :

OUTFALL001-190115


Tot Ion:212 Resp: 28949

Ion Ratio Lower Upper

212 100

106 1.9 1.7 2.5

104 1.2 1.0 1.6



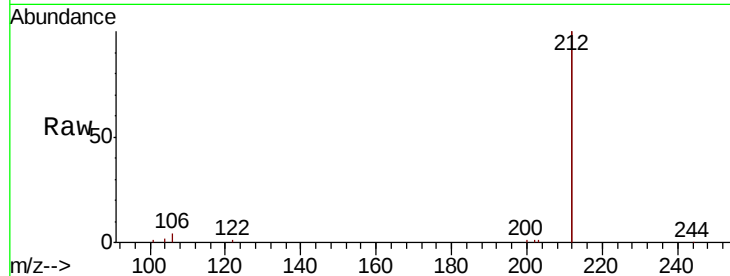


Abundance

Ion 212.00 (211.70 to 212.70): E

Ion 106.00 (105.70 to 106.70): E

Ion 104.00 (103.70 to 104.70): E

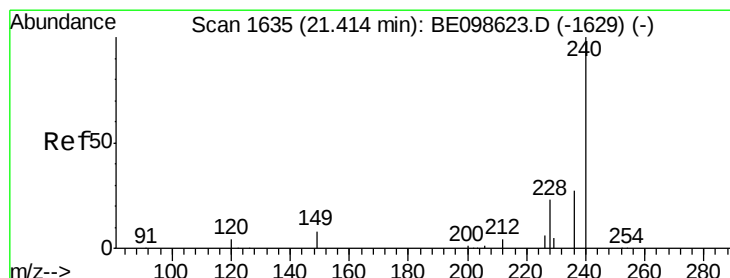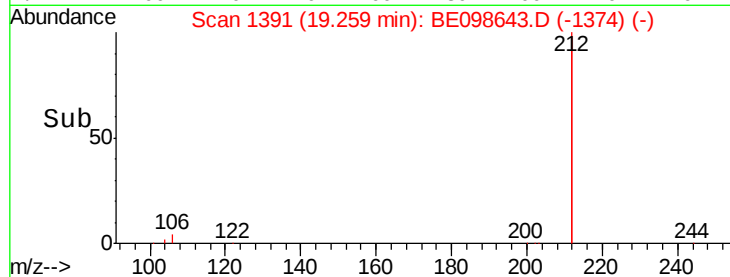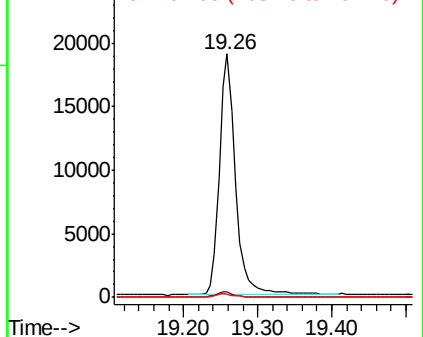

#27

Chrysene-d12

Concen: 0.400 ng

RT: 21.41 min Scan# 1634

Delta R.T. 0.00 min

Lab File: BE098643.D

Acq: 16 Jan 2019 22:06


Tgt Ion:240 Resp: 6747

Ion Ratio Lower Upper

240 100

120 5.8 4.7 7.1

236 27.6 21.9 32.9


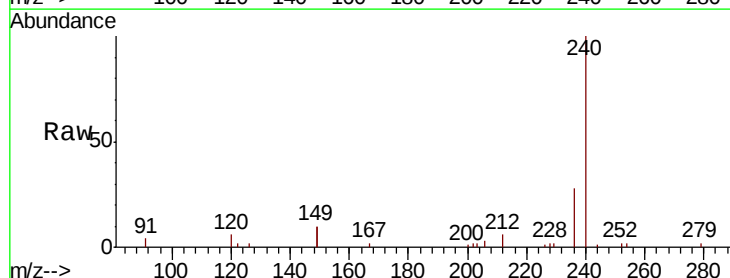



Abundance

Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

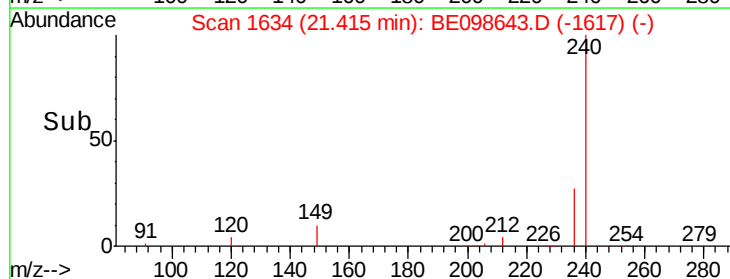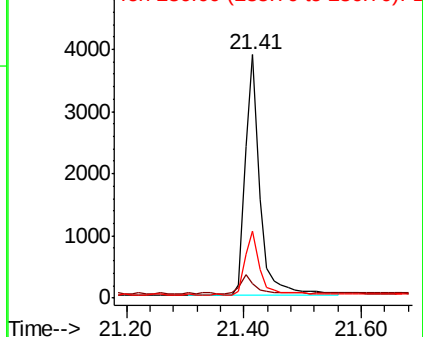

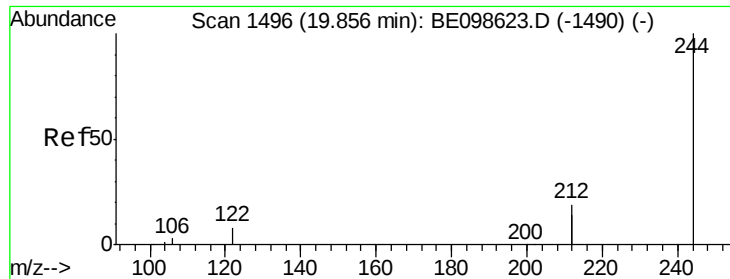

#29

Terphenyl-d14

Concen: 0.496 ng

RT: 19.86 min Scan# 1495

Delta R.T. 0.00 min

Lab File: BE098643.D

Acq: 16 Jan 2019 22:06

Instrument :

BNA_E

ClientSampleId :

OUTFALL001-190115


Tot Ion:244 Resp: 7401

Ion Ratio Lower Upper

244 100

212 36.4 29.4 44.2




122 7.7 7.1 10.7

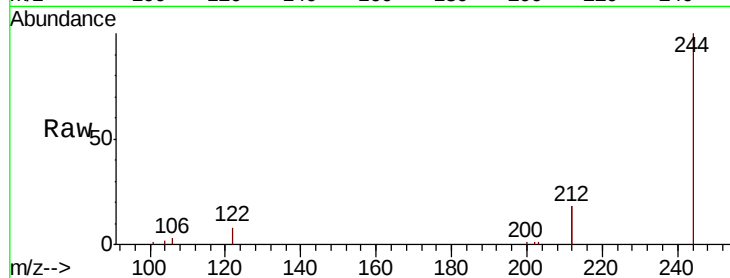

Abundance Ion 244.00 (243.70 to 244.70): E

Ion 212.00 (211.70 to 212.70): E

Ion 122.00 (121.70 to 122.70): E

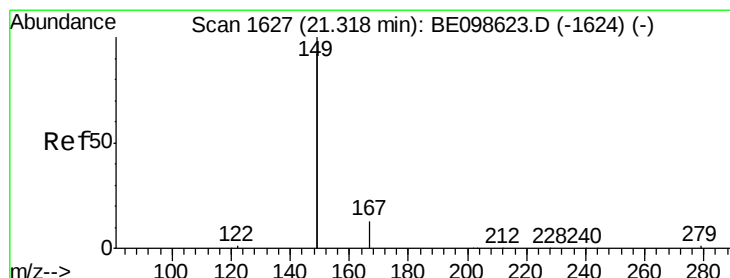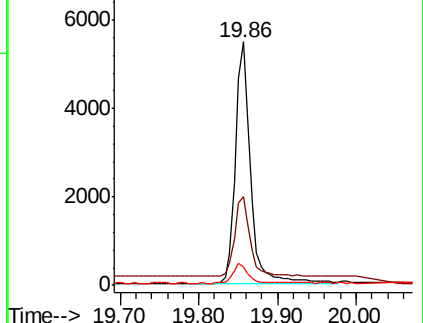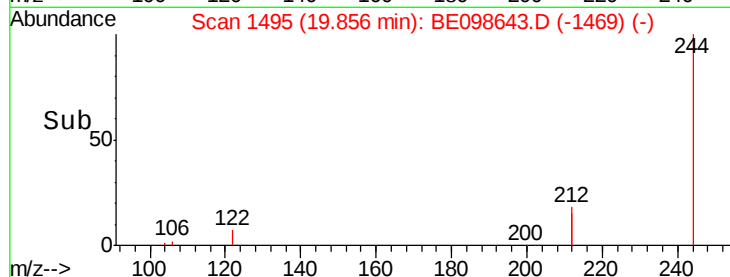

#32

Bis(2-ethylhexyl)phthalate

Concen: 0.092 ng

RT: 21.32 min Scan# 1626

Delta R.T. 0.00 min

Lab File: BE098643.D

Acq: 16 Jan 2019 22:06


Tgt Ion:149 Resp: 3522

Ion Ratio Lower Upper

149 100

167 7.7 5.4 8.2



279 1.2 1.0 1.4



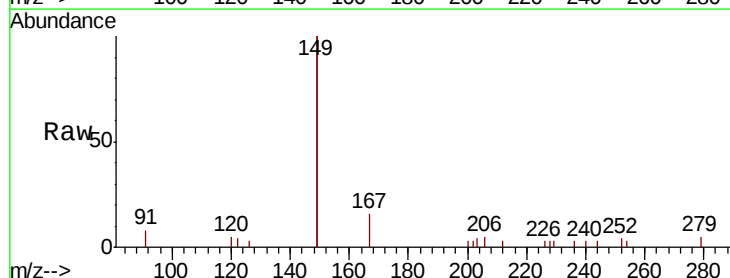


Abundance Ion 149.00 (148.70 to 149.70): E

Ion 167.00 (166.70 to 167.70): E

Ion 279.00 (278.70 to 279.70): E

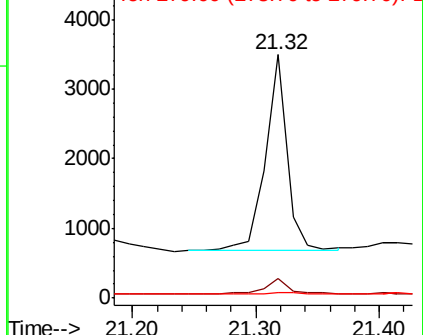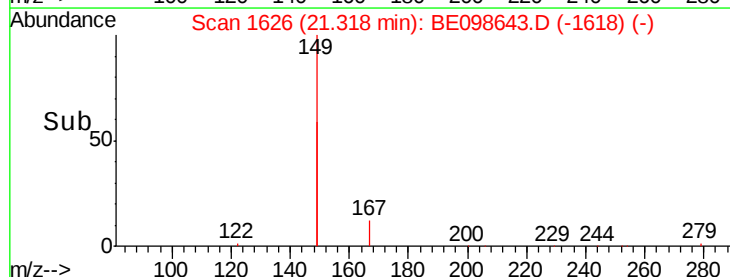

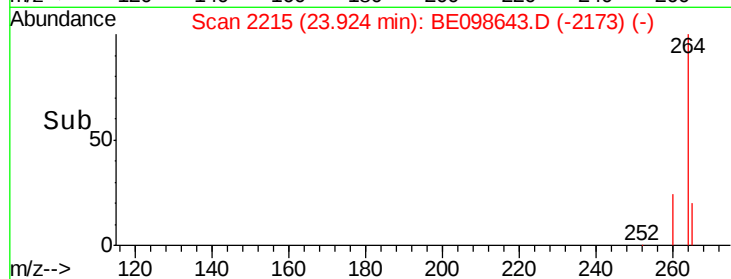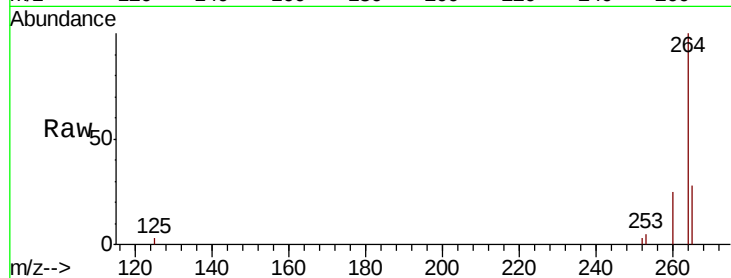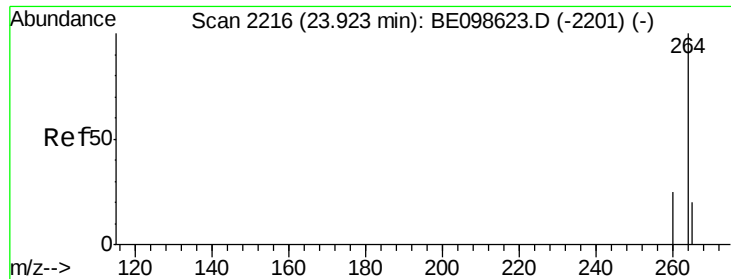

#34

Pervlene-d12

Concen: 0.400 ng

RT: 23.92 min Scan# 2215

Delta R.T. 0.00 min

Lab File: BE098643.D

Acq: 16 Jan 2019 22:06

Instrument :

BNA_E

ClientSampleId :

OUTFALL001-190115

Tot Ion: 264 Resp: 6682

Ion Ratio Lower Upper

264 100

260 24.8 20.5 30.7

265 28.5 22.3 33.5

