


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011619\
 Data File : BE098635.D
 Acq On : 16 Jan 2019 15:35
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 15 14:30:55 2019

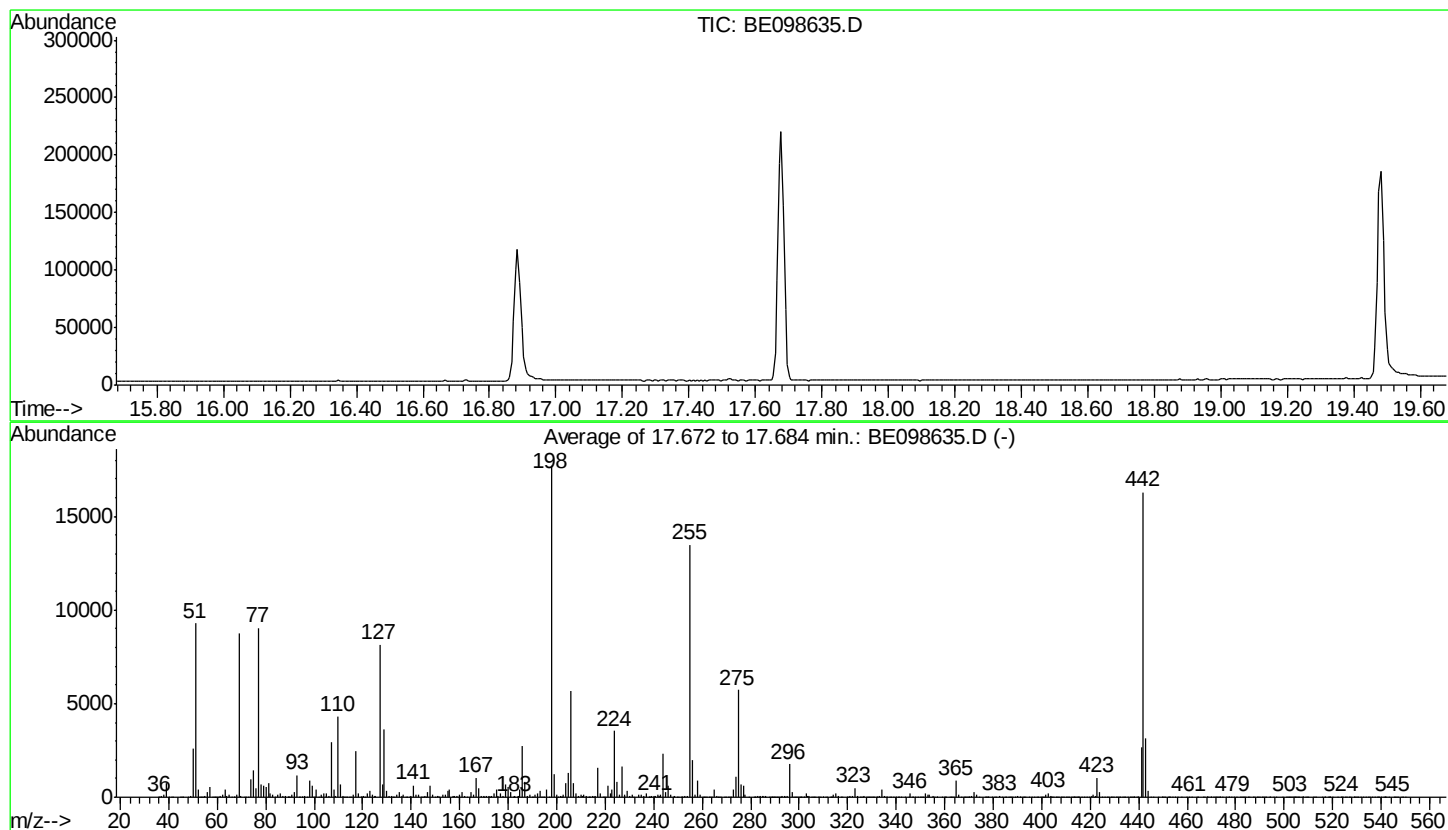

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2559

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	52.4	9286	PASS
68	69	0.00	2	1.9	167	PASS
69	198	0.00	100	49.4	8757	PASS
70	69	0.00	2	0.6	49	PASS
127	198	10	80	46.1	8162	PASS
197	198	0.00	2	0.2	29	PASS
198	198	100	100	100.0	17711	PASS
199	198	5	9	7.1	1250	PASS
275	198	10	60	32.4	5738	PASS
365	198	1	100	5.0	881	PASS
441	198	0.01	100	14.9	2643	PASS
442	198	50	100	92.1	16308	PASS
443	442	15	24	19.5	3176	PASS