
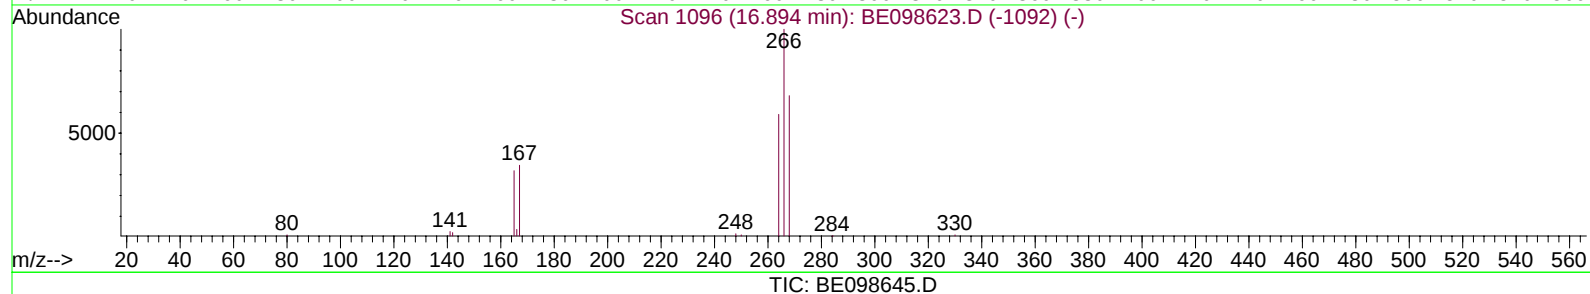
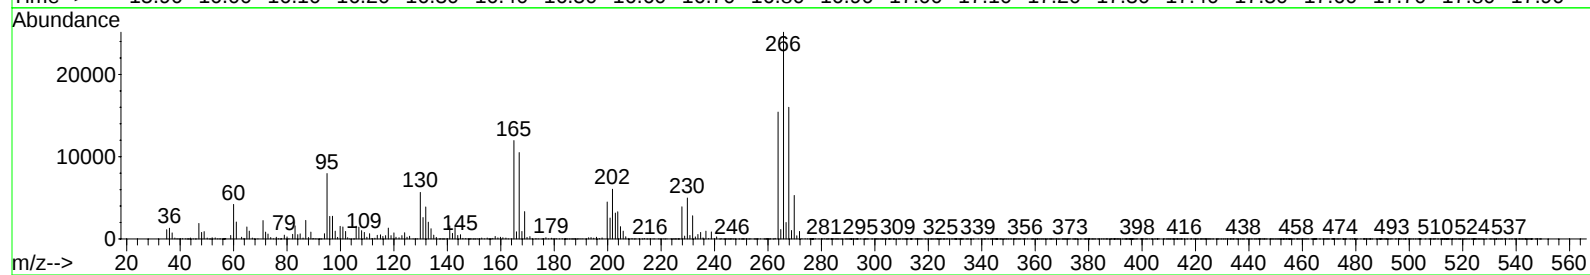


Data Path : Z:\svoasrv\HPCHEM1\BNA E\Data\BE011719\
Data File : BE098645.D
Acq On : 17 Jan 2019 8:42
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 17 18:00:22 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE011519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 15 14:30:55 2019
Response via : Initial Calibration

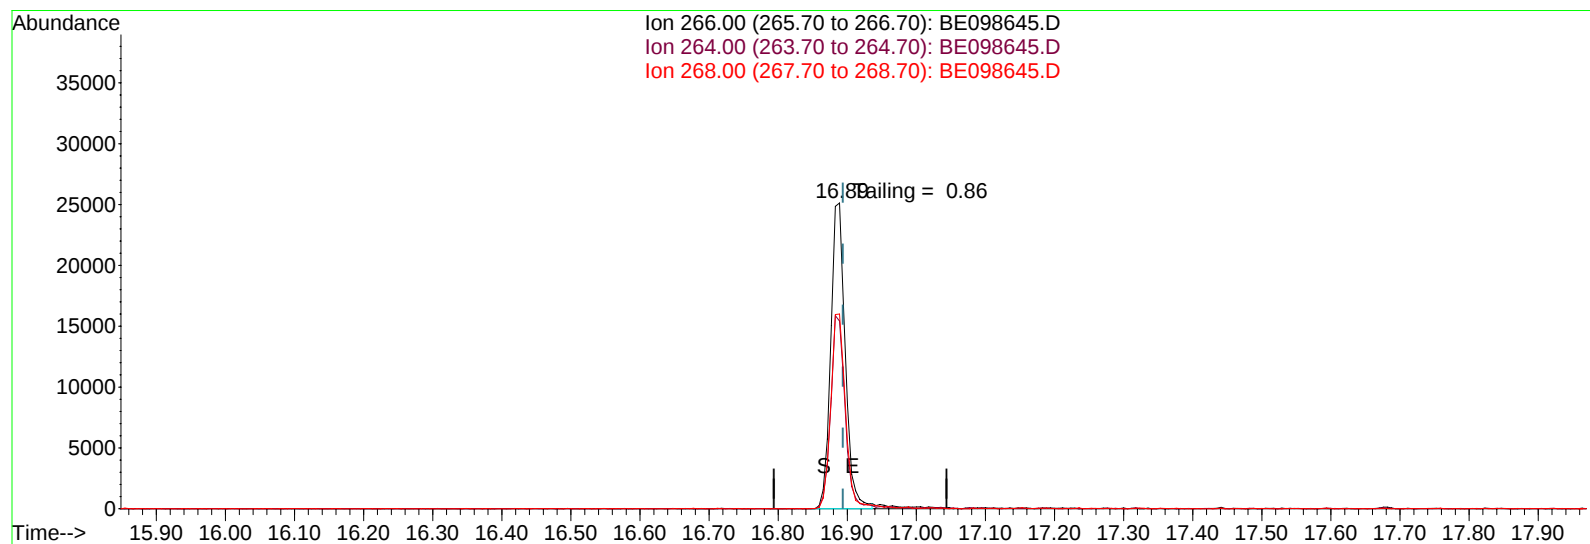

TIC: BE098645.D

(22) Pentachlorophenol

16.889min (-0.005) 10804.59ng

response 37183

Ion	Exp%	Act%
266.00	100	100
264.00	67.10	61.41
268.00	74.80	63.67
0.00	0.00	0.00