


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011719\
 Data File : BE098645.D
 Acq On : 17 Jan 2019 8:42
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 15 14:30:55 2019

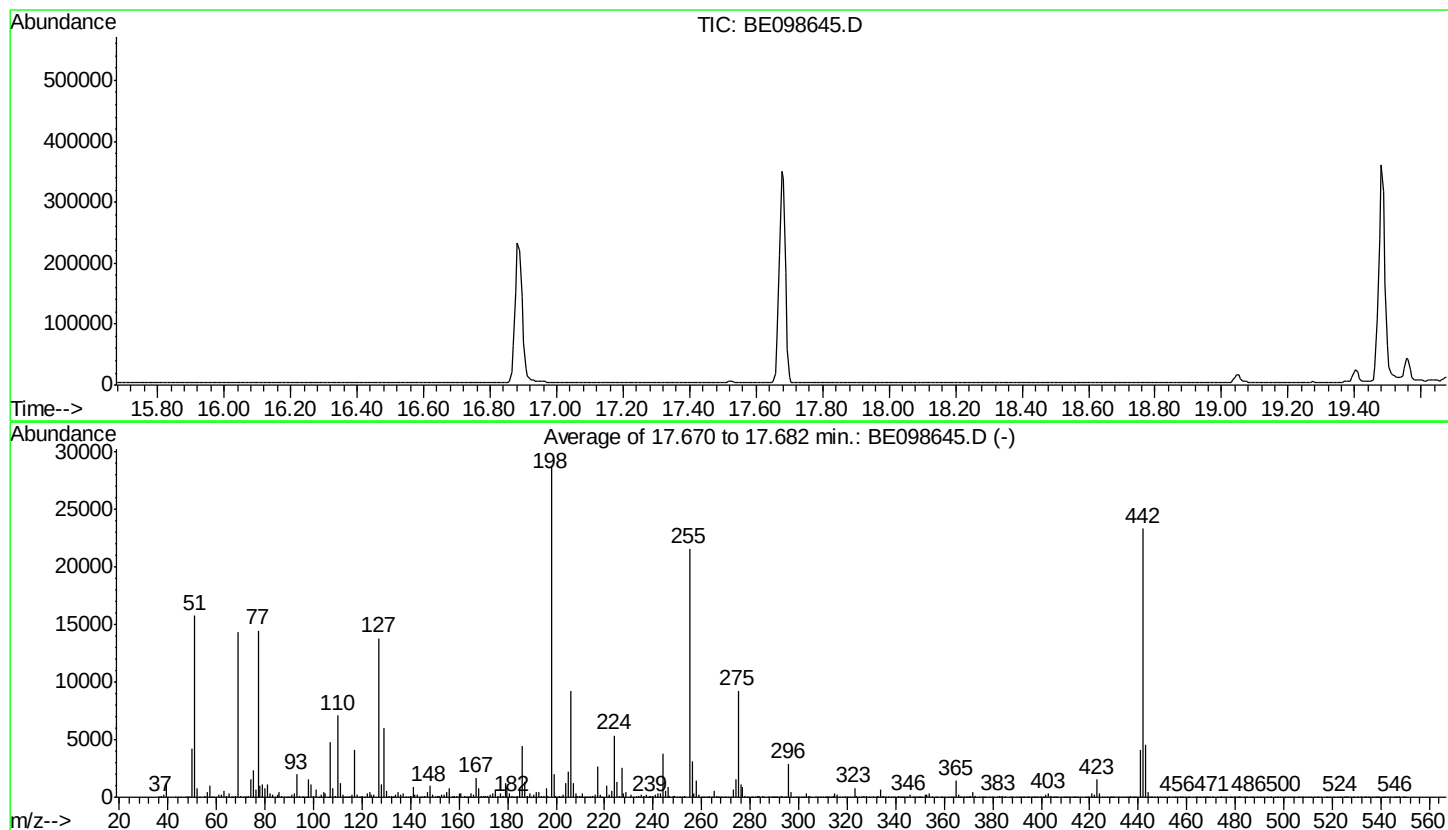

AutoFind: Scans 2567, 2568, 2569; Background Corrected with Scan 2560

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	54.7	15739	PASS
68	69	0.00	2	0.5	74	PASS
69	198	0.00	100	49.8	14336	PASS
70	69	0.00	2	0.7	103	PASS
127	198	10	80	47.9	13785	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	28781	PASS
199	198	5	9	7.1	2054	PASS
275	198	10	60	32.1	9246	PASS
365	198	1	100	4.9	1410	PASS
441	198	0.01	100	14.1	4071	PASS
442	198	50	100	80.9	23292	PASS
443	442	15	24	19.7	4595	PASS