


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011719\
 Data File : BE098650.D
 Acq On : 17 Jan 2019 15:49
 Operator : SJ/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_E
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_E\METHODS\8270-SIM-BE011519.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Tue Jan 15 14:30:55 2019

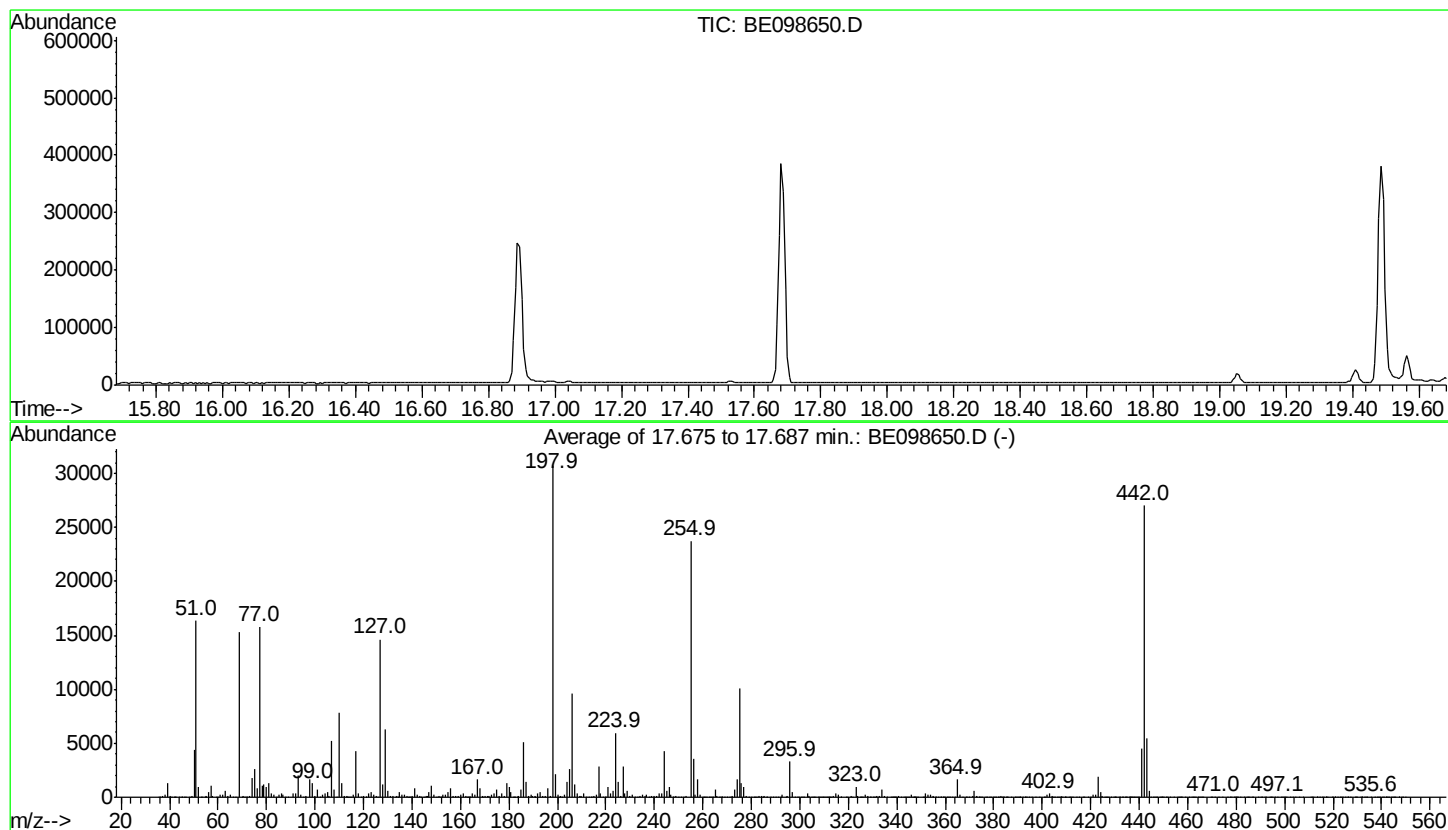

AutoFind: Scans 2568, 2569, 2570; Background Corrected with Scan 2558

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.3	16355	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	49.7	15260	PASS
70	69	0.00	2	0.5	70	PASS
127	198	10	80	47.5	14594	PASS
197	198	0.00	2	0.2	66	PASS
198	198	100	100	100.0	30711	PASS
199	198	5	9	7.0	2137	PASS
275	198	10	60	32.7	10029	PASS
365	198	1	100	5.3	1614	PASS
441	198	0.01	100	14.8	4542	PASS
442	198	50	100	88.0	27021	PASS
443	442	15	24	20.0	5407	PASS