
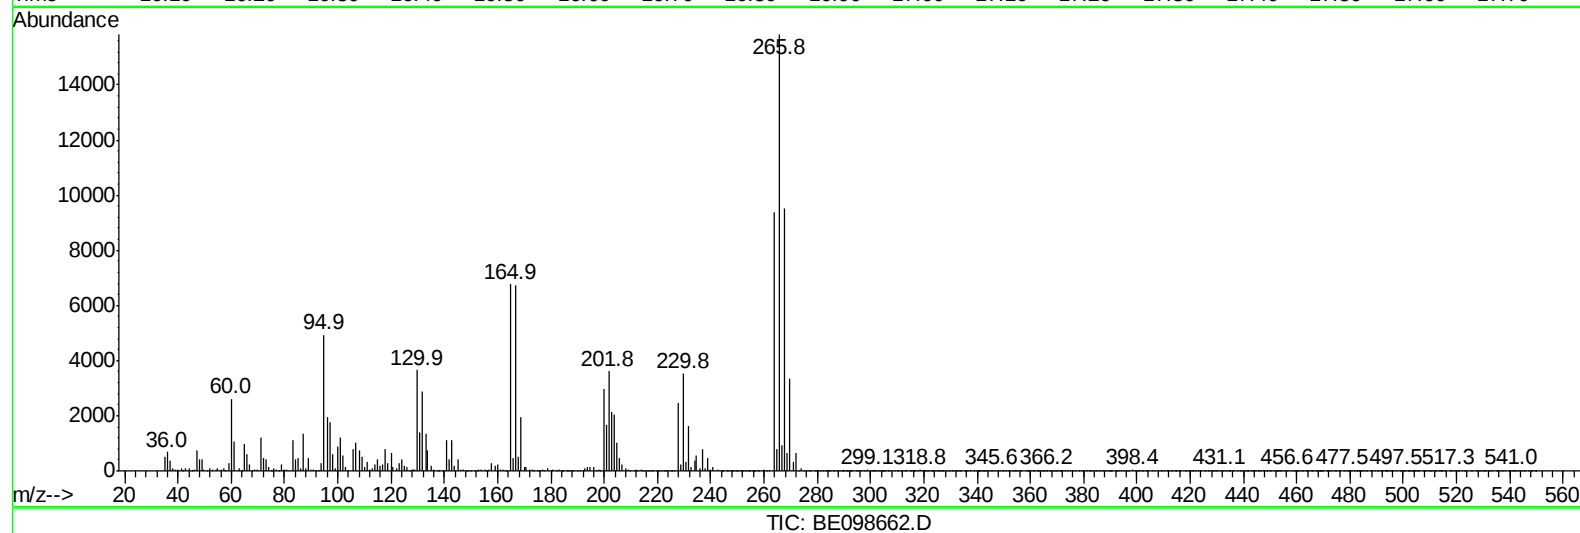


Data Path : Z:\SVOASRV\HPCHEM1\BNA E\DATA\BE011819\
Data File : BE098662.D
Acq On : 18 Jan 2019 7:58
Operator : SJ/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Jan 18 21:43:20 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA E\METHODS\8270-SIM-BE011519.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Jan 15 14:30:55 2019
Response via : Initial Calibration

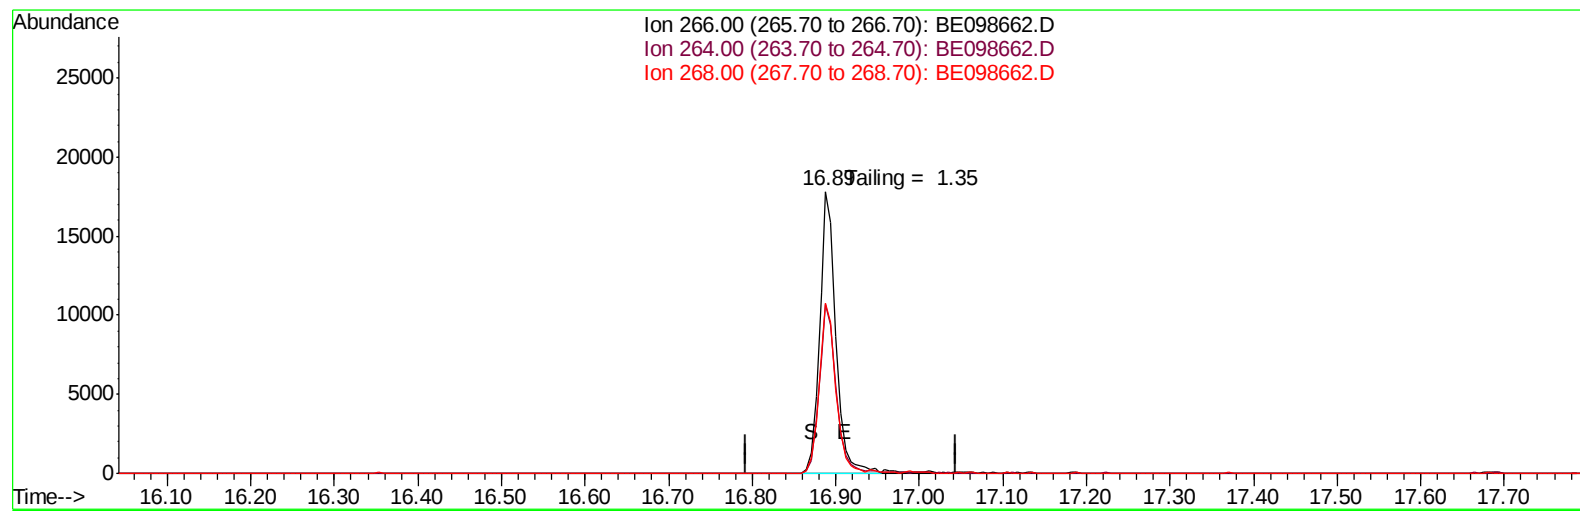

TIC: BE098662.D

(22) Pentachlorophenol

16.894min (-16.894) 0.00ng

response 0

Ion	Exp%	Act%
266.00	100	0.00
264.00	67.10	0.00#
268.00	74.80	0.00#
0.00	0.00	0.00